
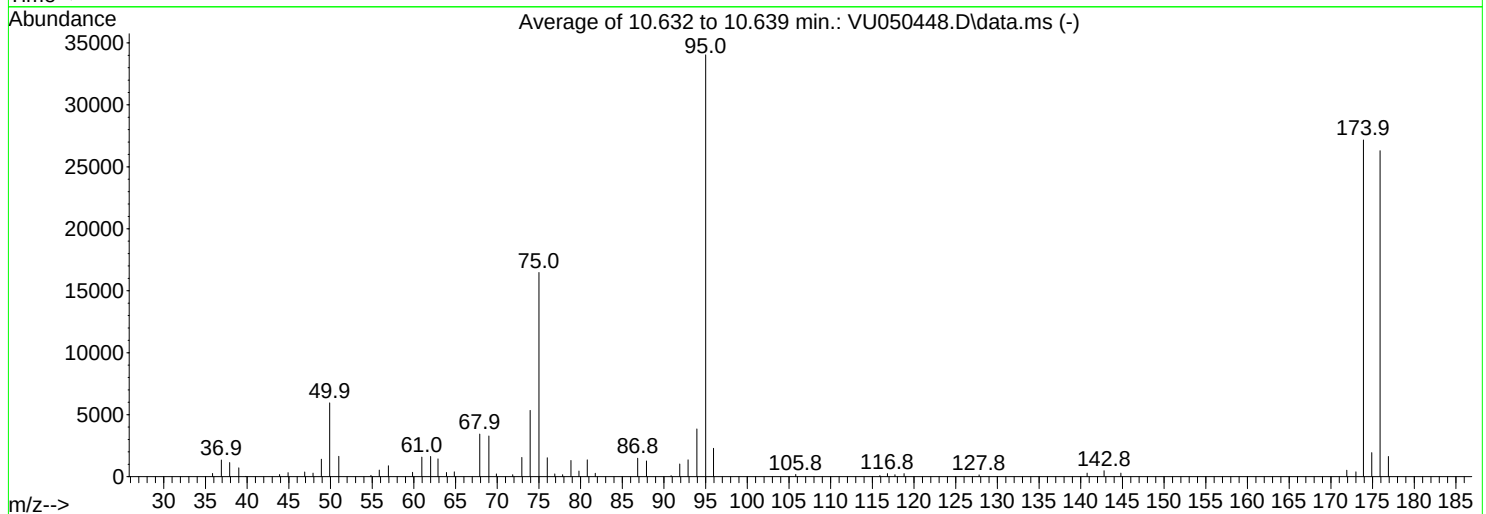


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082622\
 Data File : VU050448.D
 Acq On : 26 Aug 2022 09:08
 Operator : SY/MD
 Sample : BFB113
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB113

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 27 02:44:18 2022

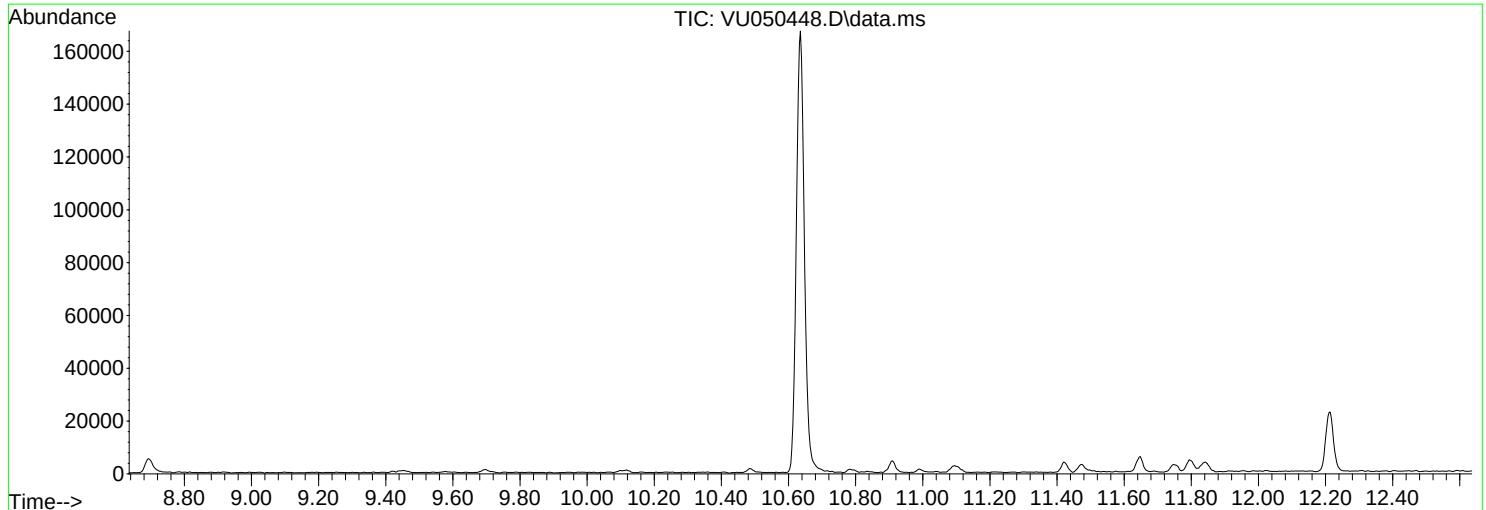

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	5949	PASS
75	95	30	80	48.4	16481	PASS
95	95	100	100	100.0	34037	PASS
96	95	5	9	6.7	2290	PASS
173	174	0.00	2	1.4	386	PASS
174	95	50	120	79.8	27165	PASS
175	174	5	9	7.1	1932	PASS
176	174	95	101	96.8	26301	PASS
177	176	5	9	6.2	1622	PASS

m/z	Abundance
39.90	149.0
43.90	431.0

Instrument :
MSVOA_U
ClientSampleId :
BFB113

m/z	Abundance
35.90	246.0
36.90	1427.0
37.90	1195.0
39.00	733.0
39.90	165.0
43.90	601.0
44.90	312.0
46.90	418.0
47.90	253.0
48.90	1502.0
49.90	5863.0
51.00	1683.0
54.80	108.0
55.80	596.0
57.00	880.0
59.80	343.0
60.90	1637.0
62.00	1659.0
62.90	1414.0
63.90	315.0
64.80	325.0
67.90	3451.0
69.00	3255.0
69.90	260.0
71.90	189.0
73.00	1522.0
74.00	5712.0
75.00	16920.0
76.00	1597.0
76.90	245.0
77.90	165.0
78.90	1337.0
79.80	458.0
80.80	1360.0
81.80	266.0
86.90	1540.0
87.90	1322.0
90.80	133.0
91.90	961.0
92.90	1453.0
94.00	3847.0
95.00	33904.0
95.90	2426.0
105.80	175.0
115.90	137.0
116.80	246.0
117.70	172.0
118.80	255.0
127.80	137.0
140.70	310.0
142.80	499.0
144.80	296.0
171.90	497.0
173.00	366.0
173.90	26776.0
174.90	1911.0
175.90	25496.0
176.90	1662.0

Instrument :
MSVOA_U
ClientSampleId :
BFB113

m/z	Abundance
35.80	260.0
36.90	1371.0
37.90	1164.0
39.00	737.0
39.90	183.0
43.90	621.0
44.90	352.0
46.90	382.0
47.90	305.0
48.90	1469.0
49.90	6200.0
51.00	1697.0
54.90	109.0
55.90	520.0
57.00	911.0
59.90	360.0
61.00	1608.0
62.00	1687.0
62.90	1499.0
63.90	368.0
64.90	370.0
67.90	3547.0
69.00	3346.0
69.90	227.0
71.80	173.0
73.00	1601.0
74.00	5473.0
75.00	16944.0
76.00	1571.0
76.90	236.0
77.90	154.0
78.90	1350.0
79.80	477.0
80.80	1413.0
81.70	277.0
86.90	1561.0
87.90	1303.0
90.90	110.0
91.90	1052.0
92.90	1393.0
94.00	3953.0
95.00	35272.0
95.90	2341.0
105.80	194.0
115.90	126.0
116.80	247.0
117.70	168.0
118.80	255.0
127.80	151.0
140.80	295.0
142.80	479.0
144.80	302.0
171.90	541.0
173.00	401.0
173.90	27904.0
174.90	1961.0
175.90	27080.0
176.90	1624.0

Instrument :
MSVOA_U
ClientSampleId :
BFB113

m/z	Abundance
35.80	286.0
36.90	1240.0
37.90	1067.0
39.00	653.0
39.80	188.0
43.90	556.0
44.90	308.0
46.90	333.0
47.90	292.0
48.90	1257.0
49.90	5784.0
51.00	1561.0
54.90	103.0
55.90	485.0
56.90	839.0
59.90	360.0
60.90	1504.0
62.00	1544.0
62.90	1390.0
63.90	323.0
64.90	484.0
67.90	3301.0
69.00	3221.0
69.90	157.0
71.80	122.0
72.90	1539.0
73.90	4851.0
75.00	15579.0
76.00	1412.0
76.90	186.0
77.80	141.0
78.80	1230.0
79.80	434.0
80.80	1300.0
81.70	261.0
86.80	1352.0
87.90	1180.0
91.90	1050.0
92.90	1235.0
93.90	3745.0
95.00	32936.0
96.00	2103.0
105.80	172.0
116.80	245.0
117.70	132.0
118.80	228.0
127.80	158.0
140.80	261.0
142.80	462.0
144.80	271.0
171.90	525.0
173.00	390.0
173.90	26816.0
174.90	1924.0
175.90	26328.0
176.90	1579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB113