

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082624\
 Data File : VU060544.D
 Acq On : 26 Aug 2024 12:31
 Operator : MD/SY
 Sample : P3711-07DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2499DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	107	rVB	22848	25472	8.70%	0.926%
2	1.911	184	193	207	rBV	32394	43636	14.91%	1.586%
3	2.560	383	395	410	rBV	45267	74739	25.53%	2.716%
4	3.039	531	544	555	rBV3	7840	14976	5.12%	0.544%
5	3.181	578	588	598	rVB4	1607	3333	1.14%	0.121%
6	4.634	1030	1040	1068	rBV	34743	109172	37.30%	3.967%
7	5.055	1157	1171	1199	rBV	58438	129184	44.14%	4.695%
8	5.717	1357	1377	1398	rBV3	105666	280202	95.73%	10.182%
9	6.242	1528	1540	1564	rBV	109146	214597	73.32%	7.798%
10	6.682	1664	1677	1699	rBV	68842	137566	47.00%	4.999%
11	7.560	1940	1950	1964	rBV2	28070	51136	17.47%	1.858%
12	7.891	2042	2053	2074	rBV	118733	210786	72.01%	7.660%
13	8.177	2132	2142	2158	rBV2	17185	30373	10.38%	1.104%
14	8.547	2244	2257	2273	rBV2	160729	278470	95.14%	10.120%
15	8.630	2273	2283	2316	rVV	131283	265339	90.65%	9.642%
16	9.412	2511	2526	2550	rBV	160868	280204	95.73%	10.183%
17	10.749	2931	2942	2957	rBV2	74845	122897	41.99%	4.466%
18	10.888	2974	2985	2994	rBV3	2911	4689	1.60%	0.170%
19	11.807	3260	3271	3296	rBV	176158	292698	100.00%	10.637%
20	12.187	3378	3389	3409	rBV2	106411	182337	62.30%	6.626%




Sum of corrected areas: 2751806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082624\
Data File : VU060544.D
Acq On : 26 Aug 2024 12:31
Operator : MD/SY
Sample : P3711-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2499DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

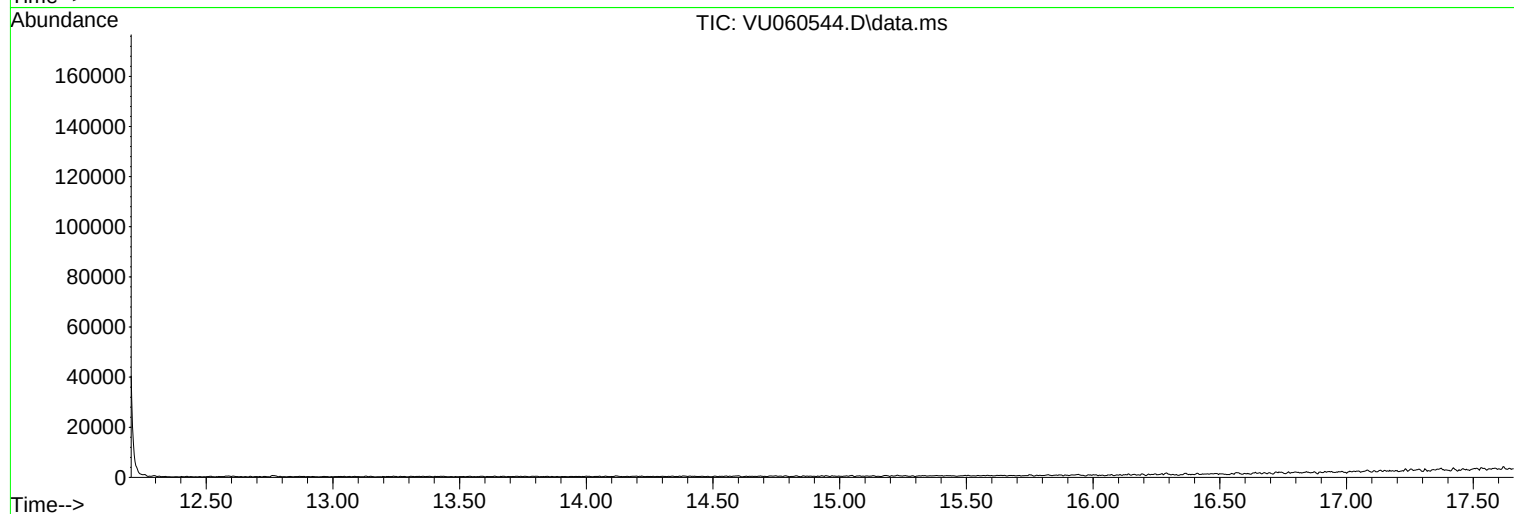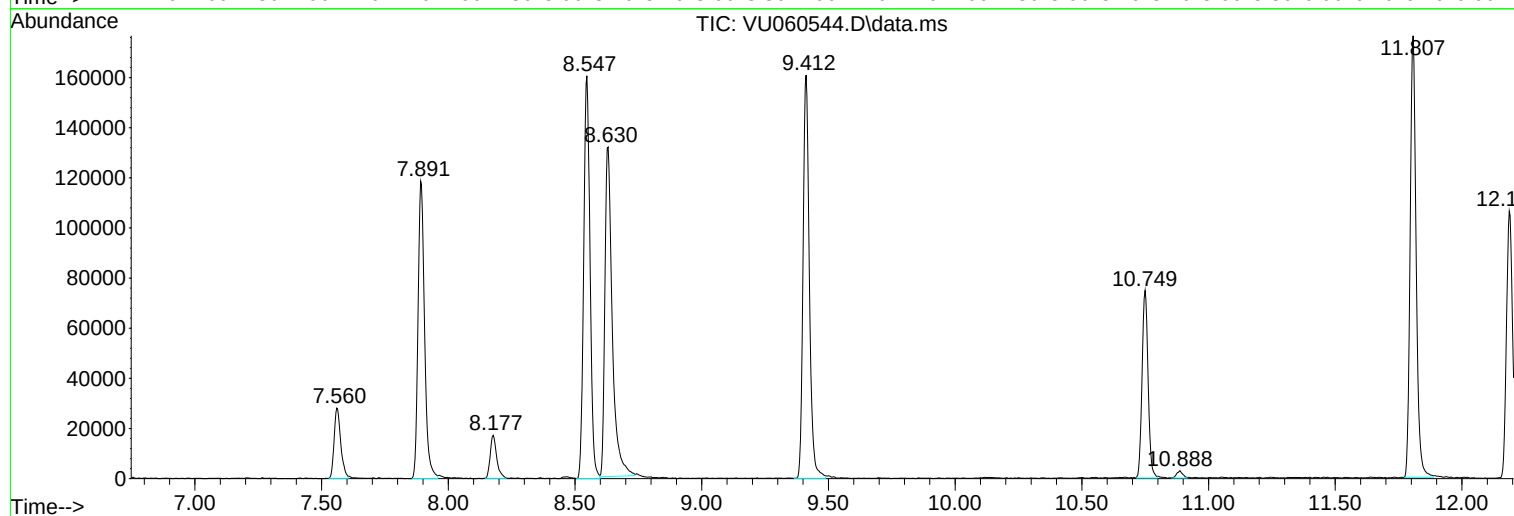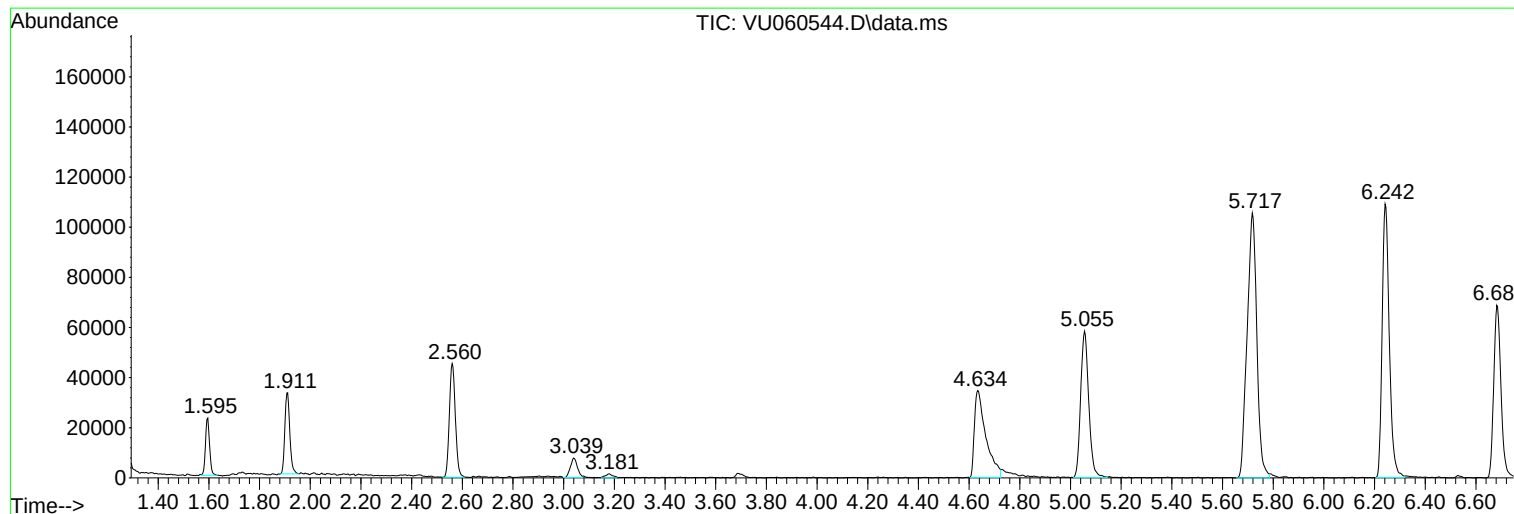

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082624\
Data File : VU060544.D
Acq On : 26 Aug 2024 12:31
Operator : MD/SY
Sample : P3711-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2499DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082624\
Data File : VU060544.D
Acq On : 26 Aug 2024 12:31
Operator : MD/SY
Sample : P3711-07DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2499DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc