


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082624\
Data File : VU060540.D
Acq On : 26 Aug 2024 09:30
Operator : MD/SY
Sample : BFB190
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB190

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Aug 27 05:49:06 2024

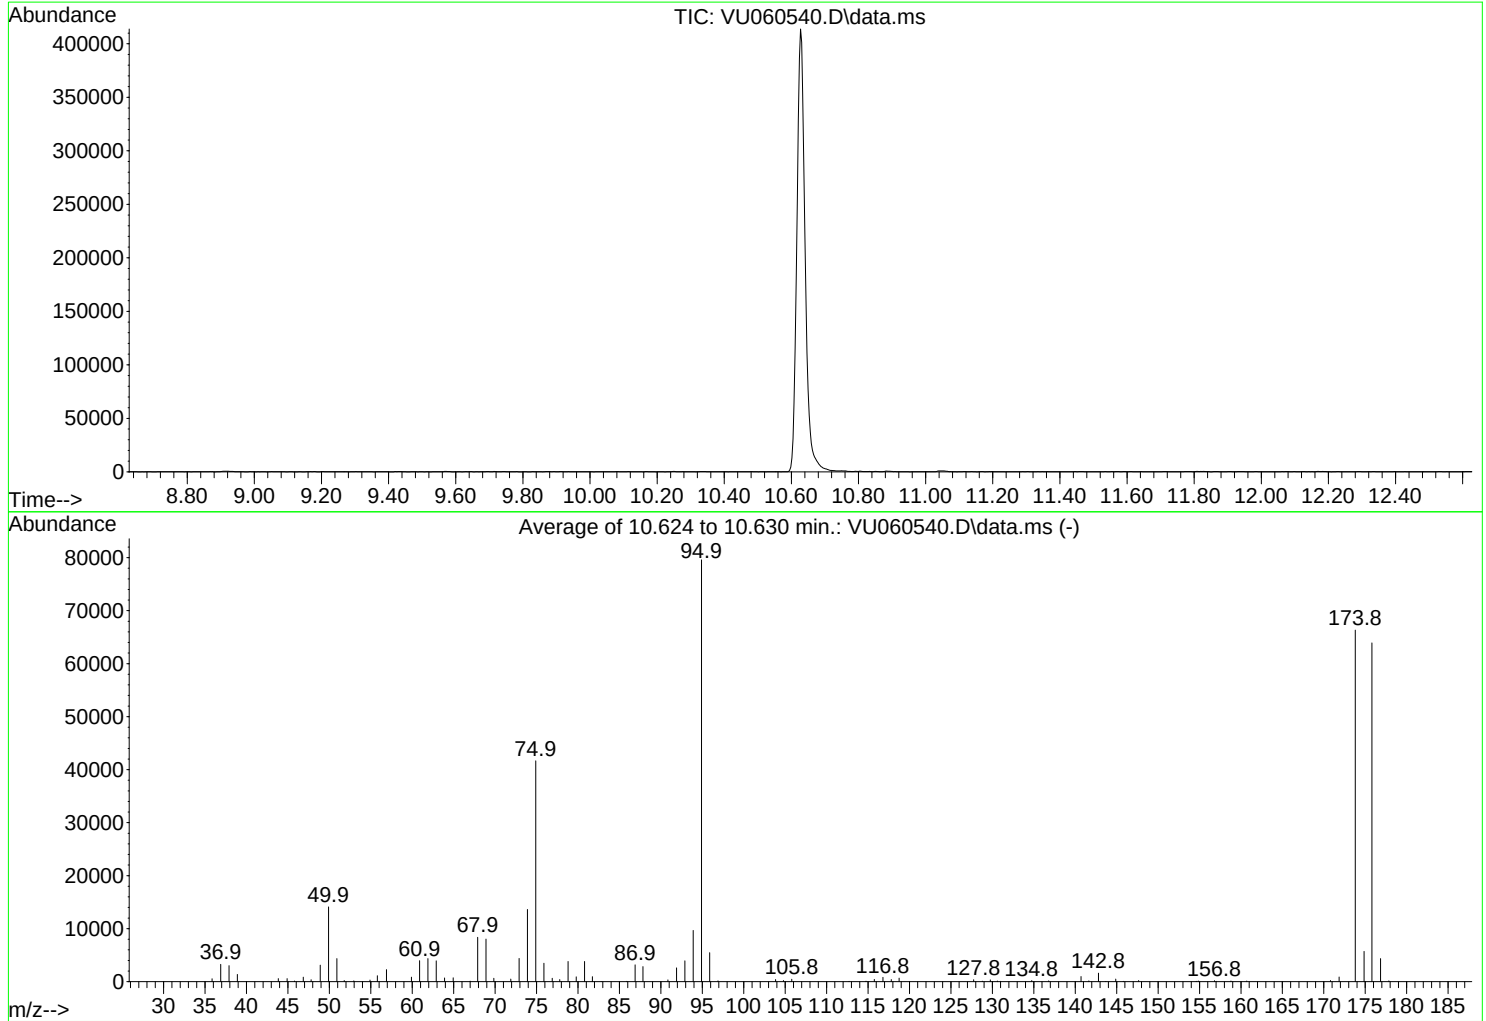

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	14113	PASS
75	95	30	80	52.3	41651	PASS
95	95	100	100	100.0	79587	PASS
96	95	5	9	6.9	5456	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.4	66336	PASS
175	174	5	9	8.6	5698	PASS
176	174	95	101	96.3	63912	PASS
177	176	5	9	6.8	4340	PASS

m/z	Abundance
43.80	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.90	531.0
36.90	3386.0
37.90	2977.0
38.90	1356.0
40.00	136.0
43.90	719.0
44.90	633.0
45.80	106.0
46.90	763.0
47.70	302.0
48.90	3027.0
49.90	13699.0
50.90	4221.0
51.80	152.0
52.90	155.0
54.90	278.0
55.80	1059.0
56.90	2174.0
59.90	868.0
60.90	3663.0
61.90	4024.0
62.90	3846.0
63.90	721.0
64.90	723.0
67.90	8316.0
68.90	7760.0
69.90	568.0
71.90	455.0
72.90	4117.0
73.90	13378.0
74.90	41024.0
75.90	3361.0
76.90	561.0
77.80	461.0
78.80	3793.0
79.80	877.0
80.80	3781.0
81.70	829.0
86.90	3136.0
87.90	2782.0
90.80	349.0
91.90	2592.0
92.90	3774.0
93.90	9471.0
94.90	76968.0
95.90	5130.0
96.90	137.0
103.90	362.0
104.80	198.0
105.80	463.0
115.80	464.0
116.80	727.0
117.80	365.0
118.70	658.0
127.80	342.0
129.80	342.0
130.60	133.0
134.70	182.0
136.80	128.0
140.70	855.0
141.80	152.0
142.80	1522.0
143.70	107.0
144.90	525.0
145.80	115.0
147.60	235.0
154.60	162.0
156.80	140.0
158.80	111.0
160.70	141.0
170.80	224.0
171.80	876.0
173.80	63152.0
174.80	5494.0
175.80	61032.0
176.80	4215.0
177.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.80	562.0
36.90	3328.0
37.90	3137.0
38.90	1412.0
43.90	740.0
44.90	579.0
45.80	135.0
46.80	861.0
47.80	325.0
48.90	3230.0
49.90	14624.0
50.90	4491.0
51.80	221.0
53.00	167.0
54.90	326.0
55.80	1150.0
56.90	2352.0
59.90	855.0
60.90	4079.0
61.90	4512.0
62.90	4054.0
63.90	717.0
64.90	723.0
67.90	8642.0
68.90	8310.0
69.90	637.0
71.90	488.0
72.90	4603.0
73.90	14037.0
74.90	42984.0
75.90	3609.0
76.90	681.0
77.80	413.0
78.80	3941.0
79.80	889.0
80.80	3925.0
81.70	1022.0
82.80	106.0
86.90	3231.0
87.80	2964.0
90.80	334.0
91.90	2727.0
92.90	4058.0
93.90	10016.0
94.90	82472.0
95.90	5634.0
96.90	168.0
103.80	395.0
104.80	239.0
105.80	474.0
112.70	114.0
114.70	121.0
115.70	433.0
116.80	855.0
117.80	408.0
118.80	690.0
127.80	374.0
128.80	130.0
129.70	363.0
130.60	127.0
131.00	118.0
134.80	234.0
136.80	159.0
140.70	985.0
141.60	167.0
142.80	1670.0
144.90	495.0
145.80	101.0
147.60	221.0
154.80	164.0
156.80	179.0
157.00	180.0
158.80	131.0
160.70	125.0
170.80	229.0
171.90	888.0
173.80	68064.0
174.90	5932.0
175.80	65928.0
176.80	4470.0
177.90	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.80	503.0
36.90	3120.0
37.90	2947.0
38.90	1344.0
43.90	671.0
44.90	475.0
45.80	153.0
46.80	926.0
47.90	448.0
48.90	3107.0
49.90	14015.0
50.90	4326.0
51.80	266.0
53.00	155.0
54.90	276.0
55.80	1109.0
56.90	2302.0
59.90	815.0
60.90	4157.0
61.90	4491.0
62.90	3881.0
63.90	673.0
65.00	698.0
67.00	268.0
67.90	8158.0
68.90	8002.0
69.80	678.0
71.90	476.0
72.90	4398.0
73.90	13412.0
74.90	40944.0
75.90	3478.0
76.90	702.0
77.80	331.0
78.80	3706.0
79.80	941.0
80.80	3746.0
81.80	988.0
85.90	149.0
86.90	3134.0
87.80	2735.0
90.90	287.0
91.90	2476.0
92.90	3904.0
93.90	9526.0
94.90	79320.0
95.90	5604.0
96.90	168.0
103.80	404.0
104.80	181.0
105.80	435.0
112.70	110.0
114.80	130.0
115.70	381.0
116.80	848.0
117.80	443.0
118.80	675.0
127.70	353.0
128.80	159.0
129.70	295.0
130.60	102.0
131.00	108.0
134.80	263.0
136.80	212.0
140.70	1075.0
141.60	152.0
142.80	1659.0
144.90	415.0
147.70	188.0
154.90	162.0
156.80	193.0
158.80	118.0
160.70	108.0
170.80	195.0
171.90	883.0
173.80	67792.0
174.90	5667.0
175.80	64776.0
176.90	4335.0
177.80	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190