


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082718\
 Data File : VU026386.D
 Acq On : 27 Aug 2018 09:41
 Operator : MD/SY
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082218WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 27 13:46:46 2018

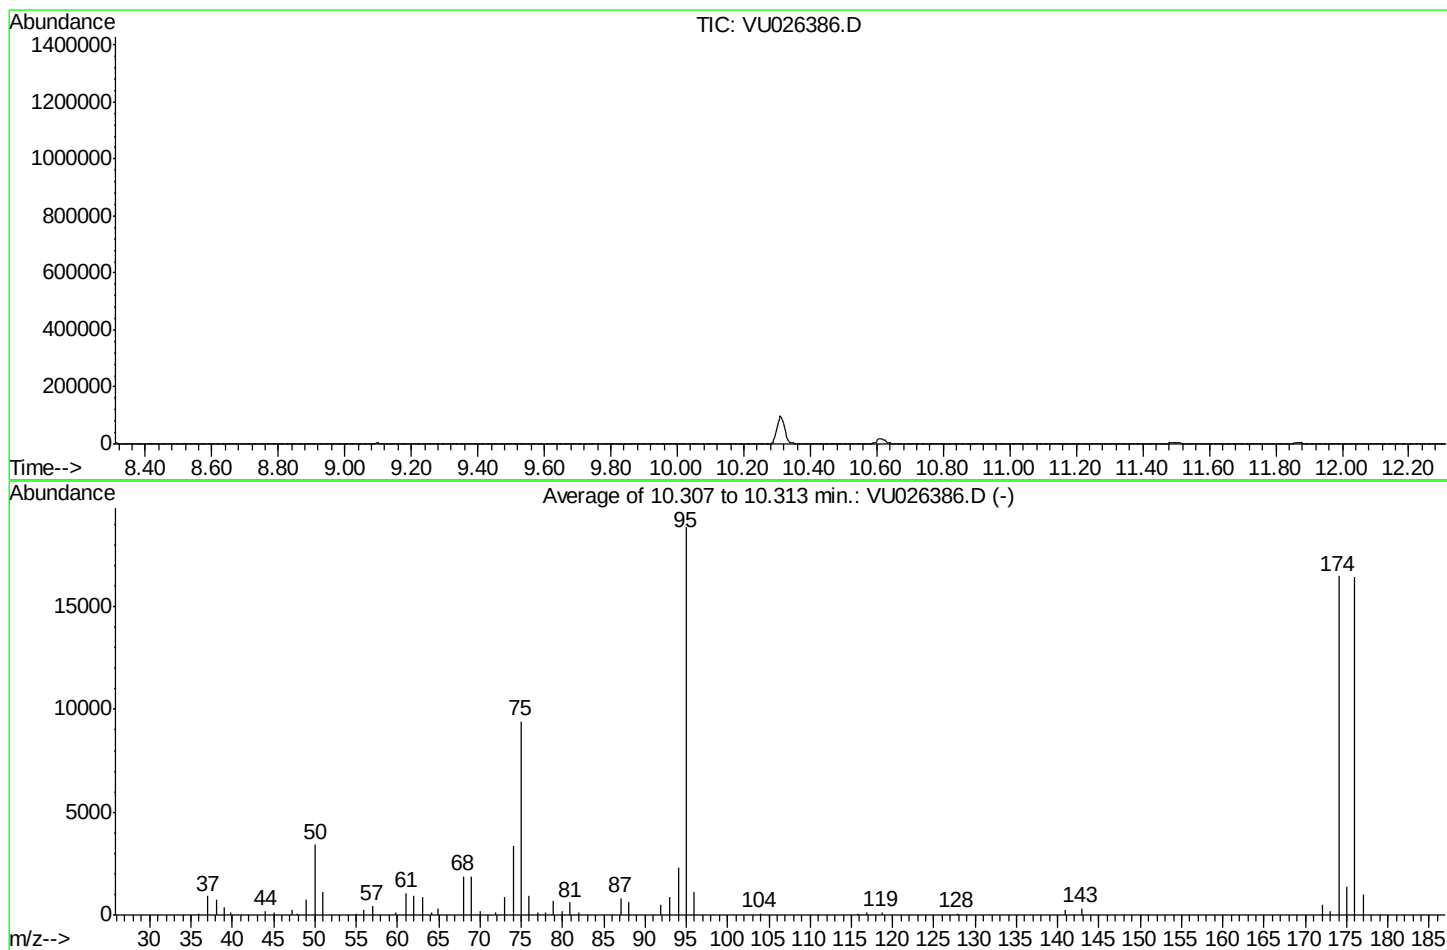

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	3400	PASS
75	95	30	80	49.9	9405	PASS
95	95	100	100	100.0	18858	PASS
96	95	5	9	5.9	1118	PASS
173	174	0.00	2	1.3	214	PASS
174	95	50	120	87.4	16486	PASS
175	174	5	9	8.4	1385	PASS
176	174	95	101	99.6	16427	PASS
177	176	5	9	5.9	977	PASS

Scan 3011 (10.271 min): VU026386.D
BFB44

m/z	Abundance
40.10	151.0
44.00	407.0
207.10	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
37.10	946.0
38.10	716.0
39.00	397.0
39.80	125.0
44.00	583.0
45.10	155.0
47.20	177.0
47.80	110.0
49.00	708.0
50.00	3383.0
51.00	1069.0
55.00	116.0
56.00	280.0
56.90	423.0
61.10	1015.0
62.00	944.0
63.00	857.0
64.20	223.0
64.90	287.0
68.00	1785.0
69.00	2044.0
70.00	186.0
72.00	113.0
73.00	921.0
74.00	3132.0
75.00	9121.0
76.00	959.0
77.00	130.0
78.90	611.0
80.00	212.0
80.90	538.0
82.00	122.0
87.00	794.0
88.00	587.0
91.90	445.0
92.90	801.0
94.00	2263.0
95.00	17824.0
96.00	1072.0
103.90	108.0
115.80	105.0
116.90	143.0
118.70	152.0
141.00	254.0
142.90	230.0
172.00	344.0
173.00	217.0
174.00	15292.0
175.00	1404.0
176.00	15833.0
176.90	1000.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	123.0
37.00	946.0
38.00	739.0
39.00	384.0
39.90	126.0
44.00	648.0
45.00	148.0
47.20	235.0
49.00	745.0
50.10	3489.0
51.00	1205.0
56.00	286.0
57.00	445.0
59.80	143.0
61.10	1162.0
62.00	936.0
63.10	952.0
64.20	178.0
65.00	329.0
68.00	1960.0
69.00	1956.0
70.00	188.0
72.00	115.0
73.00	941.0
74.00	3484.0
75.00	9660.0
76.00	945.0
77.00	154.0
78.00	143.0
78.90	722.0
80.00	213.0
80.90	629.0
82.10	129.0
87.10	872.0
88.10	651.0
92.00	488.0
92.90	890.0
94.00	2374.0
95.00	19640.0
96.00	1170.0
116.90	146.0
118.70	177.0
127.80	106.0
140.90	257.0
142.90	296.0
172.00	503.0
173.00	215.0
174.00	16984.0
175.00	1464.0
176.00	17064.0
176.90	971.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	149.0
37.00	846.0
38.00	740.0
39.00	343.0
39.90	144.0
44.00	626.0
45.00	132.0
47.20	250.0
49.00	752.0
50.10	3328.0
51.00	1130.0
56.00	273.0
57.00	501.0
59.80	173.0
61.00	1039.0
62.00	986.0
63.10	860.0
65.00	329.0
68.00	1932.0
69.00	1662.0
70.00	179.0
71.90	133.0
73.00	827.0
74.00	3453.0
75.00	9434.0
76.00	848.0
77.00	182.0
78.00	156.0
78.90	757.0
80.00	181.0
80.90	621.0
82.10	113.0
87.00	820.0
88.00	638.0
92.00	505.0
93.00	885.0
94.00	2287.0
95.00	19112.0
96.00	1113.0
104.00	104.0
116.90	158.0
118.70	143.0
127.80	103.0
140.80	258.0
142.90	425.0
172.00	623.0
173.10	212.0
174.00	17184.0
175.00	1289.0
176.00	16384.0
177.00	962.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44