


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082719\
Data File : VU033952.D
Acq On : 26 Aug 2019 15:50
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082719W.M
Title : SW846 8260
Last Update : Tue Aug 27 06:58:46 2019

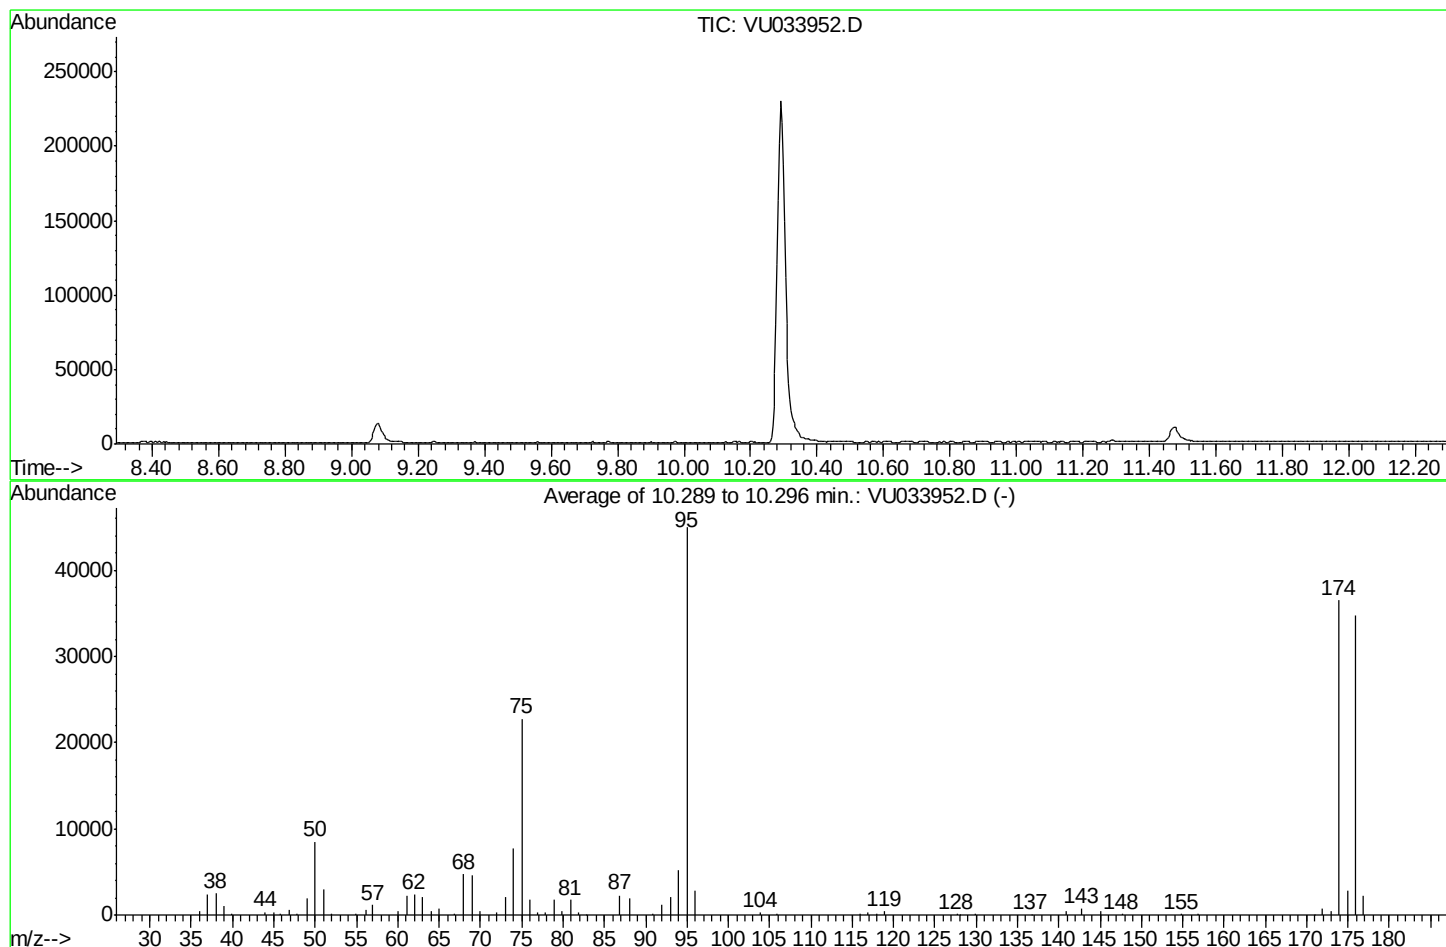

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8524	PASS
75	95	30	60	50.7	22808	PASS
95	95	100	100	100.0	45008	PASS
96	95	5	9	6.2	2784	PASS
173	174	0.00	2	1.1	409	PASS
174	95	50	100	81.1	36498	PASS
175	174	5	9	7.6	2772	PASS
176	174	95	101	95.4	34824	PASS
177	176	5	9	6.3	2180	PASS