


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082720\
Data File : VU039991.D
Acq On : 27 Aug 2020 14:34
Operator : SY/MD
Sample : L3821-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB3

Manual Integrations
APPROVED

sam
8/28/2020 3:26:44 PM

Quant Time: Aug 28 01:53:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 28 01:12:06 2020
Response via : Initial Calibration

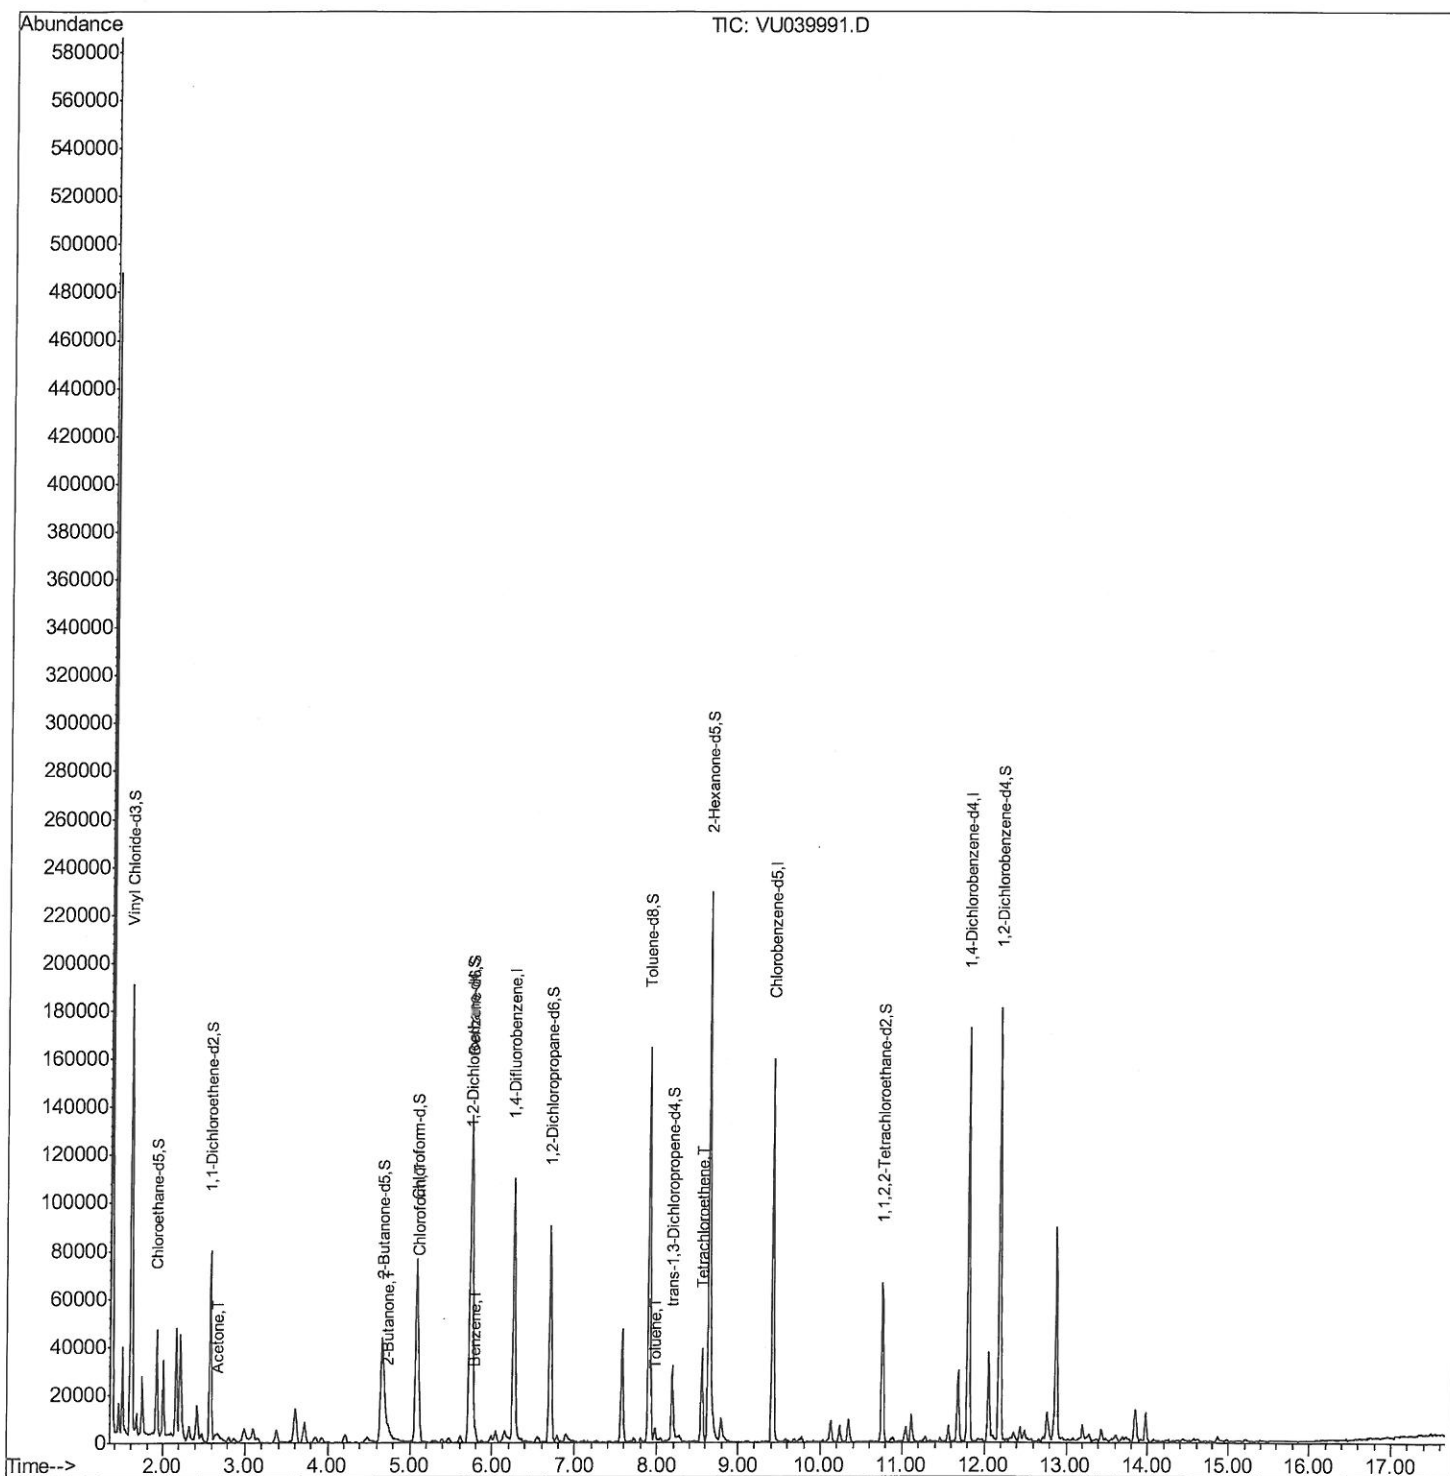

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082720\
 Data File : VU039991.D
 Acq On : 27 Aug 2020 14:34
 Operator : SY/MD
 Sample : L3821-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB3

Manual Integrations
 APPROVED

Sam
 8/28/2020 3:26:44 PM

Quant Time: Aug 28 01:14:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 28 01:12:06 2020
 Response via : Initial Calibration

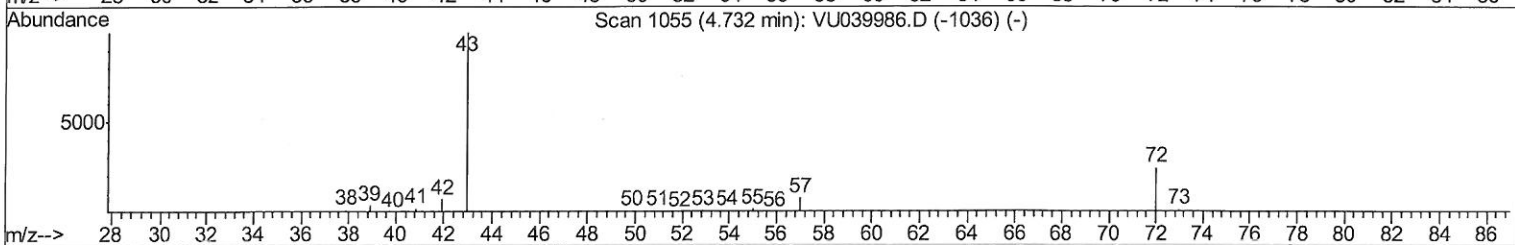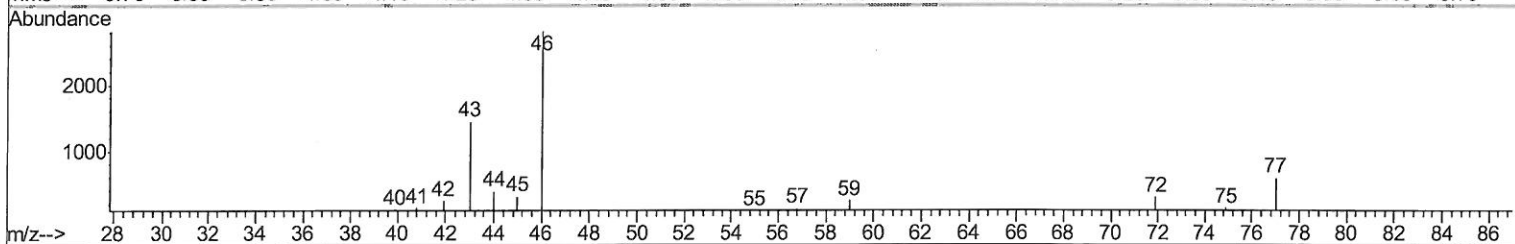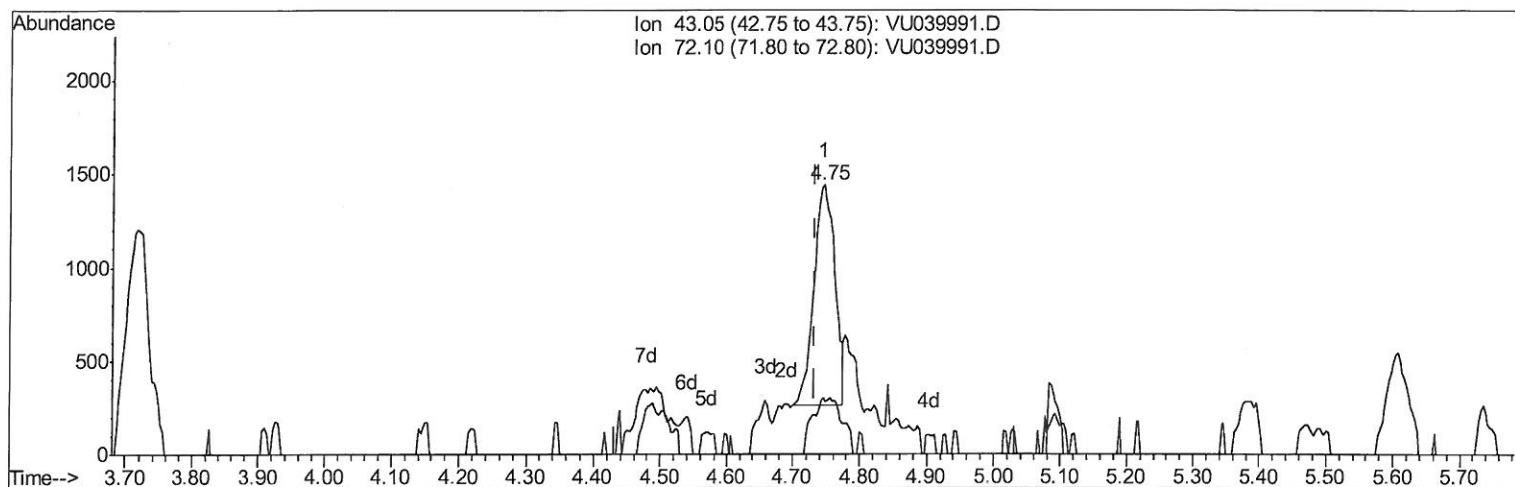

TIC: VU039991.D

(21) 2-Butanone (T)
 4.745min (+0.013) 0.93ug/L
 response 2583

Ion	Exp%	Act%
43.05	100	100
72.10	25.30	16.45
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082720\
 Data File : VU039991.D
 Acq On : 27 Aug 2020 14:34
 Operator : SY/MD
 Sample : L3821-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 H0AB3

Manual Integrations
 APPROVED

sam
 8/28/2020 3:26:44 PM

Quant Time: Aug 28 01:14:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 28 01:12:06 2020
 Response via : Initial Calibration

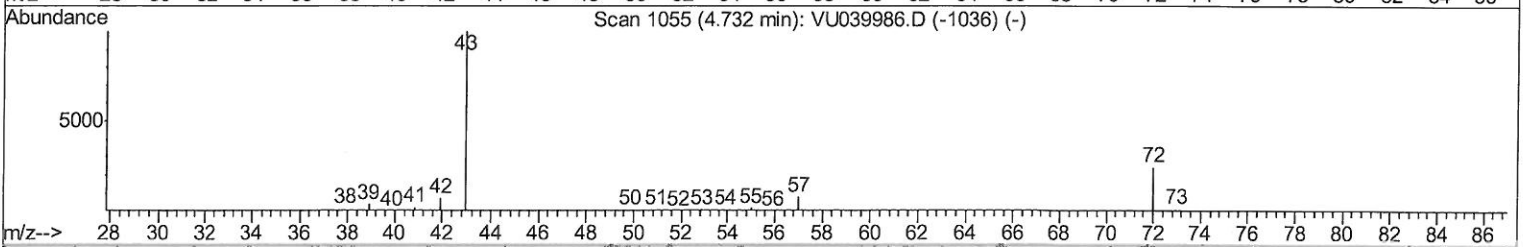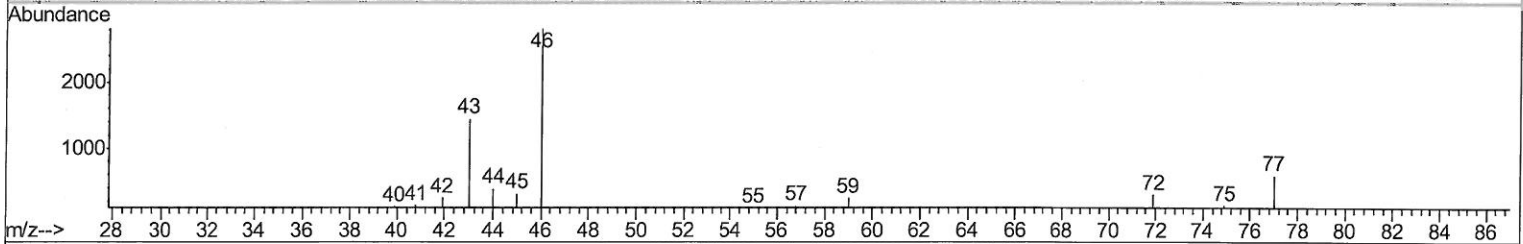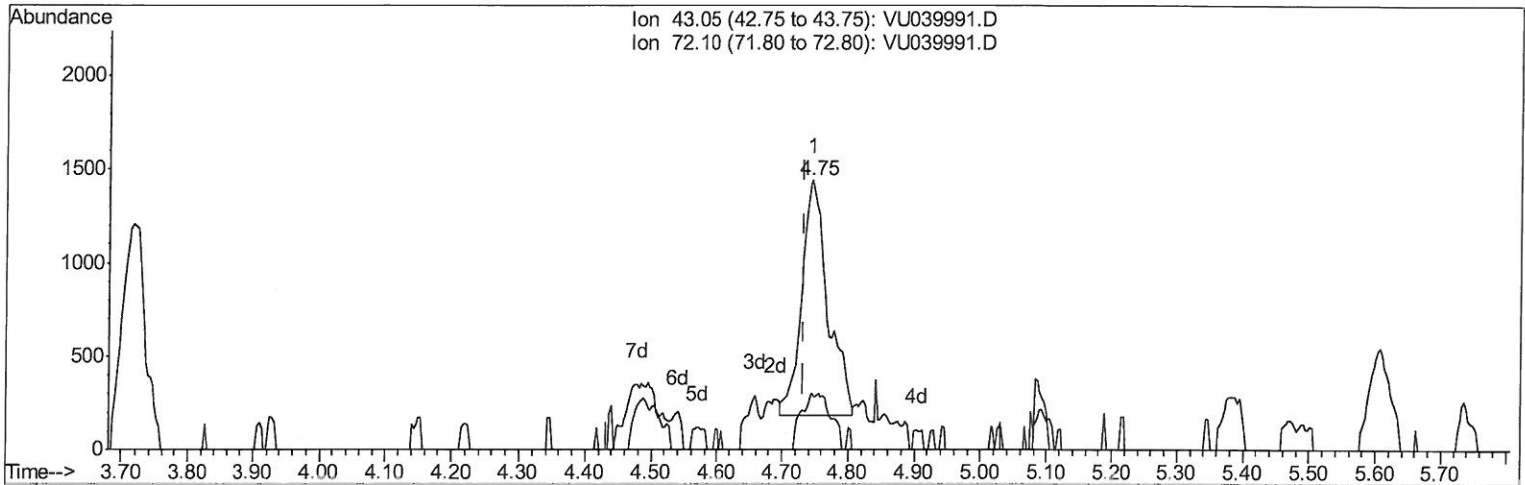

TIC: VU039991.D

(21) 2-Butanone (T)

4.745min (+0.013) 1.24ug/L m

response 3449

Ion Exp% Act%

43.05 100 100

72.10 25.30 12.32#

0.00 0.00 0.00

0.00 0.00 0.00

7 MD
8/31/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082720\
 Data File : VU039991.D
 Acq On : 27 Aug 2020 14:34
 Operator : SY/MD
 Sample : L3821-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB3

Manual Integrations
 APPROVED

sam
 8/28/2020 3:26:44 PM

Quant Time: Aug 28 01:53:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 28 01:12:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	83878	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	80336	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	41087	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	27188	3.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.20%
7) Chloroethane-d5	1.92	69	25750	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.58	63	45687	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	4.66	46	92618	39.56	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.12%
24) Chloroform-d	5.08	84	63524	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.72	65	37571	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.75	84	112998	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.70	67	38030	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.91	98	96116	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
43) trans-1,3-Dichloropropene-	8.19	79	15350	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
46) 2-Hexanone-d5	8.64	63	77486	46.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.24%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	31129	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	42523	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.68	43	8867	5.542	ug/L	80
21) 2-Butanone	4.75	43	3449m	1.241	ug/L	7
25) Chloroform	5.11	83	11270	0.787	ug/L	99
33) Benzene	5.79	78	4063	0.139	ug/L	100
42) Toluene	7.98	91	3572	0.120	ug/L	95
47) Tetrachloroethene	8.56	164	7514	1.344	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed