


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082720\
Data File : VU039985.D
Acq On : 27 Aug 2020 09:50
Operator : SY/MD
Sample : BFB23
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR081920WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 28 01:12:06 2020

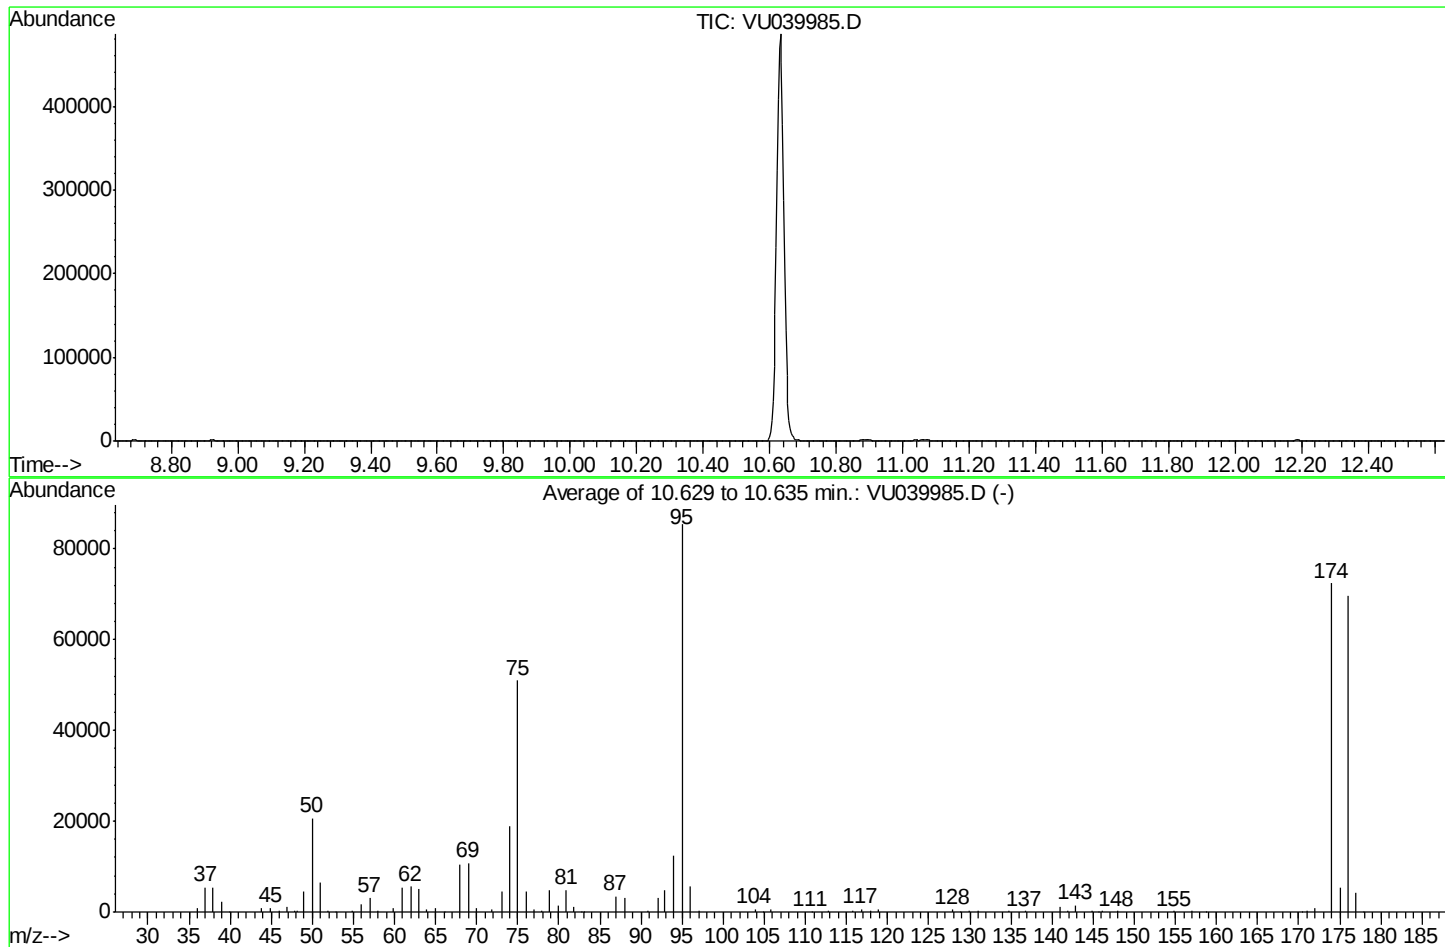

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	20597	PASS
75	95	30	80	59.7	51034	PASS
95	95	100	100	100.0	85440	PASS
96	95	5	9	6.7	5706	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	72405	PASS
175	174	5	9	7.5	5424	PASS
176	174	95	101	96.3	69701	PASS
177	176	5	9	6.2	4293	PASS

m/z	Abundance
36.00	923.0
37.00	5805.0
37.90	5622.0
38.90	2321.0
39.90	128.0
43.90	1042.0
44.90	990.0
46.00	172.0
46.80	1055.0
47.80	560.0
48.90	4451.0
49.90	21104.0
51.00	6639.0
52.00	311.0
54.90	385.0
55.90	1777.0
57.00	3128.0
57.90	174.0
59.90	921.0
60.90	5277.0
62.00	5836.0
63.00	5375.0
64.00	669.0
65.00	920.0
67.90	10659.0
69.00	10925.0
70.00	847.0
71.90	595.0
73.00	4651.0
74.00	18944.0
75.00	51536.0
76.00	4633.0
77.00	467.0
77.90	386.0
78.90	4726.0
79.90	1395.0
80.90	4891.0
81.90	1243.0
82.80	173.0
86.90	3674.0
87.90	3000.0
90.90	406.0
92.00	3175.0
92.90	4991.0
94.00	12363.0
95.00	85480.0
96.00	5760.0
97.00	189.0
103.90	607.0
104.90	148.0
105.80	557.0
110.70	144.0
112.80	145.0
115.80	373.0
116.80	723.0
118.00	392.0
118.90	607.0
127.90	445.0
128.90	144.0
129.90	333.0
130.90	160.0
134.80	209.0
136.70	210.0
140.90	1296.0
141.80	175.0
142.90	1533.0
144.90	204.0
146.10	169.0
148.00	216.0
154.90	191.0
157.00	155.0
158.80	113.0
170.90	206.0
171.90	943.0
174.00	71144.0
175.00	5398.0
176.00	67544.0
177.00	4259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.10	896.0
37.00	5672.0
37.90	5542.0
38.90	2319.0
39.80	108.0
43.90	1015.0
44.90	944.0
45.90	154.0
46.80	1067.0
47.80	518.0
48.90	4542.0
50.00	21304.0
51.00	6882.0
52.00	380.0
52.90	108.0
54.90	389.0
56.00	1879.0
57.00	3277.0
57.90	224.0
59.90	1017.0
60.90	5553.0
61.90	5785.0
63.00	5283.0
63.90	646.0
65.00	845.0
66.10	108.0
68.00	10920.0
69.00	11058.0
70.00	953.0
71.90	636.0
73.00	4570.0
74.00	19672.0
75.00	53024.0
76.00	4640.0
77.00	538.0
77.90	351.0
78.90	4863.0
79.90	1421.0
80.90	4979.0
81.80	1155.0
82.80	179.0
86.90	3632.0
88.00	3065.0
91.00	375.0
92.00	3159.0
92.90	5138.0
94.00	12862.0
95.00	88608.0
96.00	5892.0
97.00	208.0
103.90	613.0
104.90	149.0
105.80	562.0
110.70	153.0
112.70	186.0
115.80	373.0
116.80	723.0
117.90	396.0
118.90	578.0
127.90	506.0
128.90	143.0
129.90	305.0
130.90	181.0
134.80	200.0
136.70	214.0
140.90	1312.0
141.90	184.0
142.90	1593.0
144.90	211.0
146.00	185.0
148.00	206.0
154.90	202.0
157.00	160.0
158.80	119.0
170.40	127.0
171.00	196.0
172.00	910.0
174.00	74976.0
175.00	5593.0
176.00	72272.0
177.00	4425.0
177.80	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.10	738.0
37.00	4986.0
37.90	4891.0
38.90	2141.0
43.90	897.0
45.00	943.0
45.90	133.0
46.90	920.0
48.10	506.0
49.00	4244.0
50.00	19384.0
51.00	6252.0
51.90	415.0
52.90	117.0
54.90	342.0
56.00	1810.0
57.00	3050.0
57.90	217.0
59.90	926.0
60.90	5271.0
61.90	5069.0
63.00	4656.0
64.00	537.0
65.00	718.0
68.00	10088.0
69.00	10298.0
70.00	880.0
71.90	580.0
73.00	4043.0
74.00	18064.0
75.00	48544.0
76.00	4204.0
77.00	527.0
77.90	295.0
78.90	4435.0
79.90	1283.0
80.90	4566.0
81.80	1049.0
83.00	161.0
86.90	3141.0
88.00	2924.0
90.80	353.0
92.00	2893.0
92.90	4624.0
94.00	12263.0
95.00	82232.0
96.00	5467.0
97.00	178.0
103.90	544.0
104.90	128.0
105.90	517.0
110.80	151.0
112.70	182.0
115.80	370.0
116.80	668.0
117.80	387.0
118.90	570.0
127.90	498.0
128.90	118.0
129.80	264.0
131.00	159.0
134.80	166.0
136.80	207.0
141.00	1193.0
142.00	177.0
142.90	1448.0
144.90	232.0
145.60	125.0
146.00	144.0
147.80	206.0
154.80	198.0
157.00	148.0
158.80	123.0
170.30	129.0
171.10	178.0
172.00	870.0
174.00	71096.0
175.00	5283.0
176.00	69288.0
177.00	4196.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
43.80	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23