
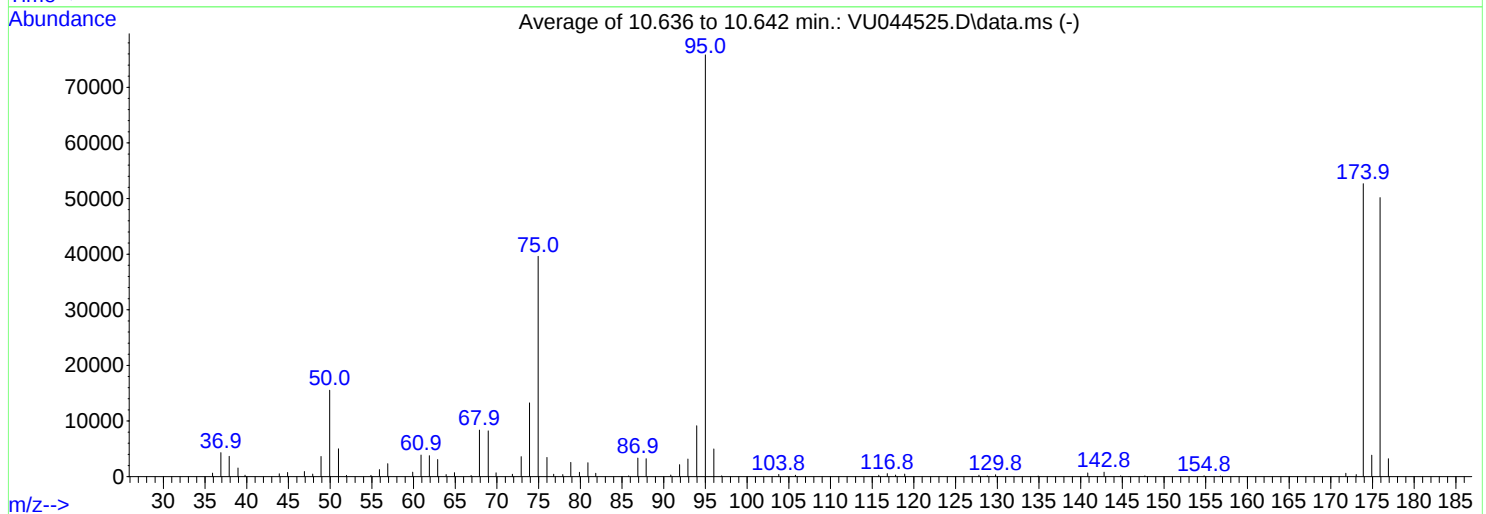


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082721\
 Data File : VU044525.D
 Acq On : 27 Aug 2021 09:35
 Operator : SY/MD
 Sample : BFB011
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB011

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 28 01:19:29 2021

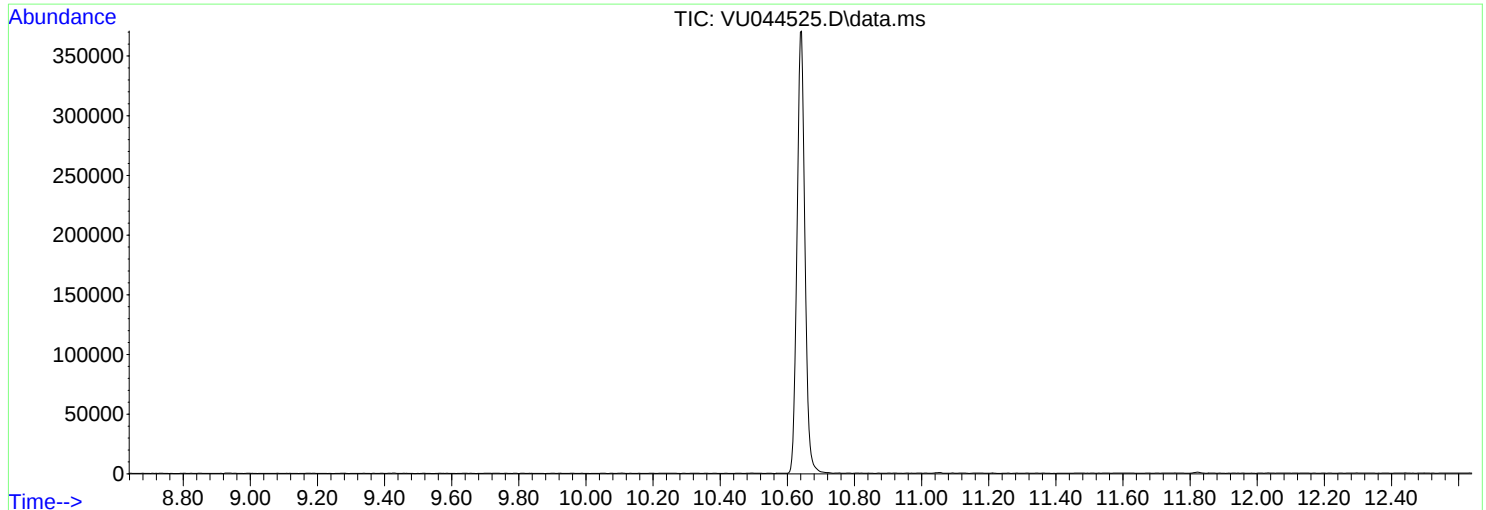

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	15550	PASS
75	95	30	80	52.2	39600	PASS
95	95	100	100	100.0	75837	PASS
96	95	5	9	6.6	4976	PASS
173	174	0.00	2	0.7	385	PASS
174	95	50	120	69.5	52675	PASS
175	174	5	9	7.3	3855	PASS
176	174	95	101	95.2	50171	PASS
177	176	5	9	6.4	3216	PASS

m/z	Abundance
35.90	670.0
36.90	4455.0
37.90	3637.0
38.90	1614.0
39.80	431.0
43.90	904.0
44.90	690.0
46.90	949.0
47.90	482.0
48.90	3642.0
49.90	15614.0
51.00	5115.0
51.90	223.0
54.90	235.0
55.90	1315.0
56.90	2476.0
59.90	856.0
60.90	3991.0
61.90	3731.0
62.90	3040.0
63.90	380.0
64.90	696.0
66.90	195.0
67.90	8620.0
68.90	8487.0
69.90	735.0
71.90	470.0
72.90	3811.0
73.90	13876.0
74.90	40672.0
76.00	3467.0
76.80	433.0
77.90	375.0
78.80	2650.0
79.90	848.0
80.90	2533.0
81.90	641.0
85.70	156.0
86.90	3490.0
87.90	3447.0
90.80	284.0
91.90	2291.0
92.90	3231.0
93.90	9397.0
95.00	77840.0
96.00	5003.0
96.90	161.0
103.80	443.0
105.80	294.0
115.80	265.0
116.80	572.0
117.80	302.0
118.90	444.0
127.80	263.0
128.80	114.0
129.80	328.0
134.90	151.0
140.80	678.0
142.80	854.0
144.80	155.0
147.70	147.0
154.80	161.0
156.80	116.0
171.80	631.0
173.00	606.0
173.90	55400.0
174.90	4078.0
175.90	53312.0
176.90	3349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

Scan 2878 (10.594 min): VU044525.D\data.ms
BFB011

m/z	Abundance
39.80	201.0
44.00	377.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	596.0
36.90	4020.0
37.90	3540.0
39.00	1455.0
39.90	503.0
43.90	907.0
44.90	781.0
46.90	893.0
47.90	443.0
48.90	3477.0
50.00	14919.0
51.00	4714.0
52.00	223.0
54.90	213.0
55.90	1170.0
56.90	2072.0
59.90	760.0
60.90	3654.0
61.90	3718.0
62.90	3039.0
63.90	357.0
64.90	752.0
66.90	215.0
67.90	7904.0
69.00	7751.0
69.90	647.0
71.80	399.0
72.90	3283.0
73.90	12202.0
75.00	37208.0
76.00	3370.0
76.80	419.0
77.90	373.0
78.90	2357.0
79.90	693.0
80.90	2373.0
81.80	555.0
85.90	120.0
86.90	3138.0
87.90	2928.0
90.90	276.0
91.90	1996.0
92.90	3059.0
93.90	8614.0
95.00	71128.0
96.00	4808.0
97.00	153.0
103.80	329.0
104.80	103.0
105.80	228.0
115.80	232.0
116.80	495.0
117.80	264.0
118.90	449.0
127.80	221.0
128.80	153.0
129.80	321.0
134.90	100.0
140.90	622.0
142.80	740.0
144.80	143.0
147.70	126.0
154.80	173.0
156.70	111.0
171.80	537.0
173.90	48368.0
174.90	3525.0
175.90	45496.0
176.90	3009.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	655.0
36.90	4452.0
37.90	3776.0
39.00	1625.0
39.80	451.0
43.90	893.0
44.90	757.0
46.90	939.0
47.90	474.0
48.90	3763.0
49.90	16116.0
51.00	5170.0
51.90	221.0
54.90	218.0
55.90	1300.0
56.90	2431.0
59.90	849.0
60.90	3982.0
61.90	3880.0
62.90	3170.0
63.90	394.0
64.90	751.0
66.90	226.0
67.90	8597.0
69.00	8491.0
69.90	734.0
71.90	449.0
72.90	3727.0
73.90	13689.0
74.90	40920.0
76.00	3563.0
76.80	437.0
77.90	395.0
78.90	2670.0
79.90	820.0
80.90	2580.0
81.90	641.0
85.80	138.0
86.90	3380.0
87.90	3332.0
90.90	297.0
91.90	2226.0
92.90	3245.0
94.00	9401.0
95.00	78544.0
96.00	5116.0
97.00	157.0
103.80	409.0
104.80	101.0
105.80	270.0
115.80	259.0
116.80	551.0
117.80	305.0
118.90	481.0
127.80	259.0
128.80	150.0
129.80	357.0
134.90	136.0
140.90	693.0
142.80	840.0
144.80	164.0
145.80	103.0
147.70	140.0
154.80	175.0
156.80	134.0
171.80	615.0
173.10	548.0
173.90	54256.0
174.90	3961.0
175.90	51704.0
176.90	3291.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011