

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
 Data File : VU026409.D
 Acq On : 28 Aug 2018 20:07
 Operator : MD/SY
 Sample : J4633-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB3K2

Quant Time: Aug 29 02:07:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 00:08:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	63595	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	63547	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	28396	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	22216	2.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.40%
7) Chloroethane-d5	1.68	69	19814	3.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	62.20%#
11) 1,1-Dichloroethene-d2	2.27	63	33495	2.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	46.80%#
20) 2-Butanone-d5	4.20	46	62389	39.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.64%
24) Chloroform-d	4.65	84	37504	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.20%
26) 1,2-Dichloroethane-d4	5.31	65	21880	3.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.80%
32) Benzene-d6	5.34	84	74126	3.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.20%#
36) 1,2-Dichloropropane-d6	6.34	67	25821	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.60%
41) Toluene-d8	7.57	98	63669	3.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	62.60%#
43) trans-1,3-Dichloropropene-	7.85	79	7648	2.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.20%
46) 2-Hexanone-d5	8.32	63	43740	37.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.06%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	20188	3.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	25244	3.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	76.20%#


Target Compounds					Ovalue
13) Acetone	2.33	43	3613	3.12 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
Data File : VU026409.D
Acq On : 28 Aug 2018 20:07
Operator : MD/SY
Sample : J4633-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB3K2

Quant Time: Aug 29 02:07:55 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 00:08:04 2018
Response via : Initial Calibration

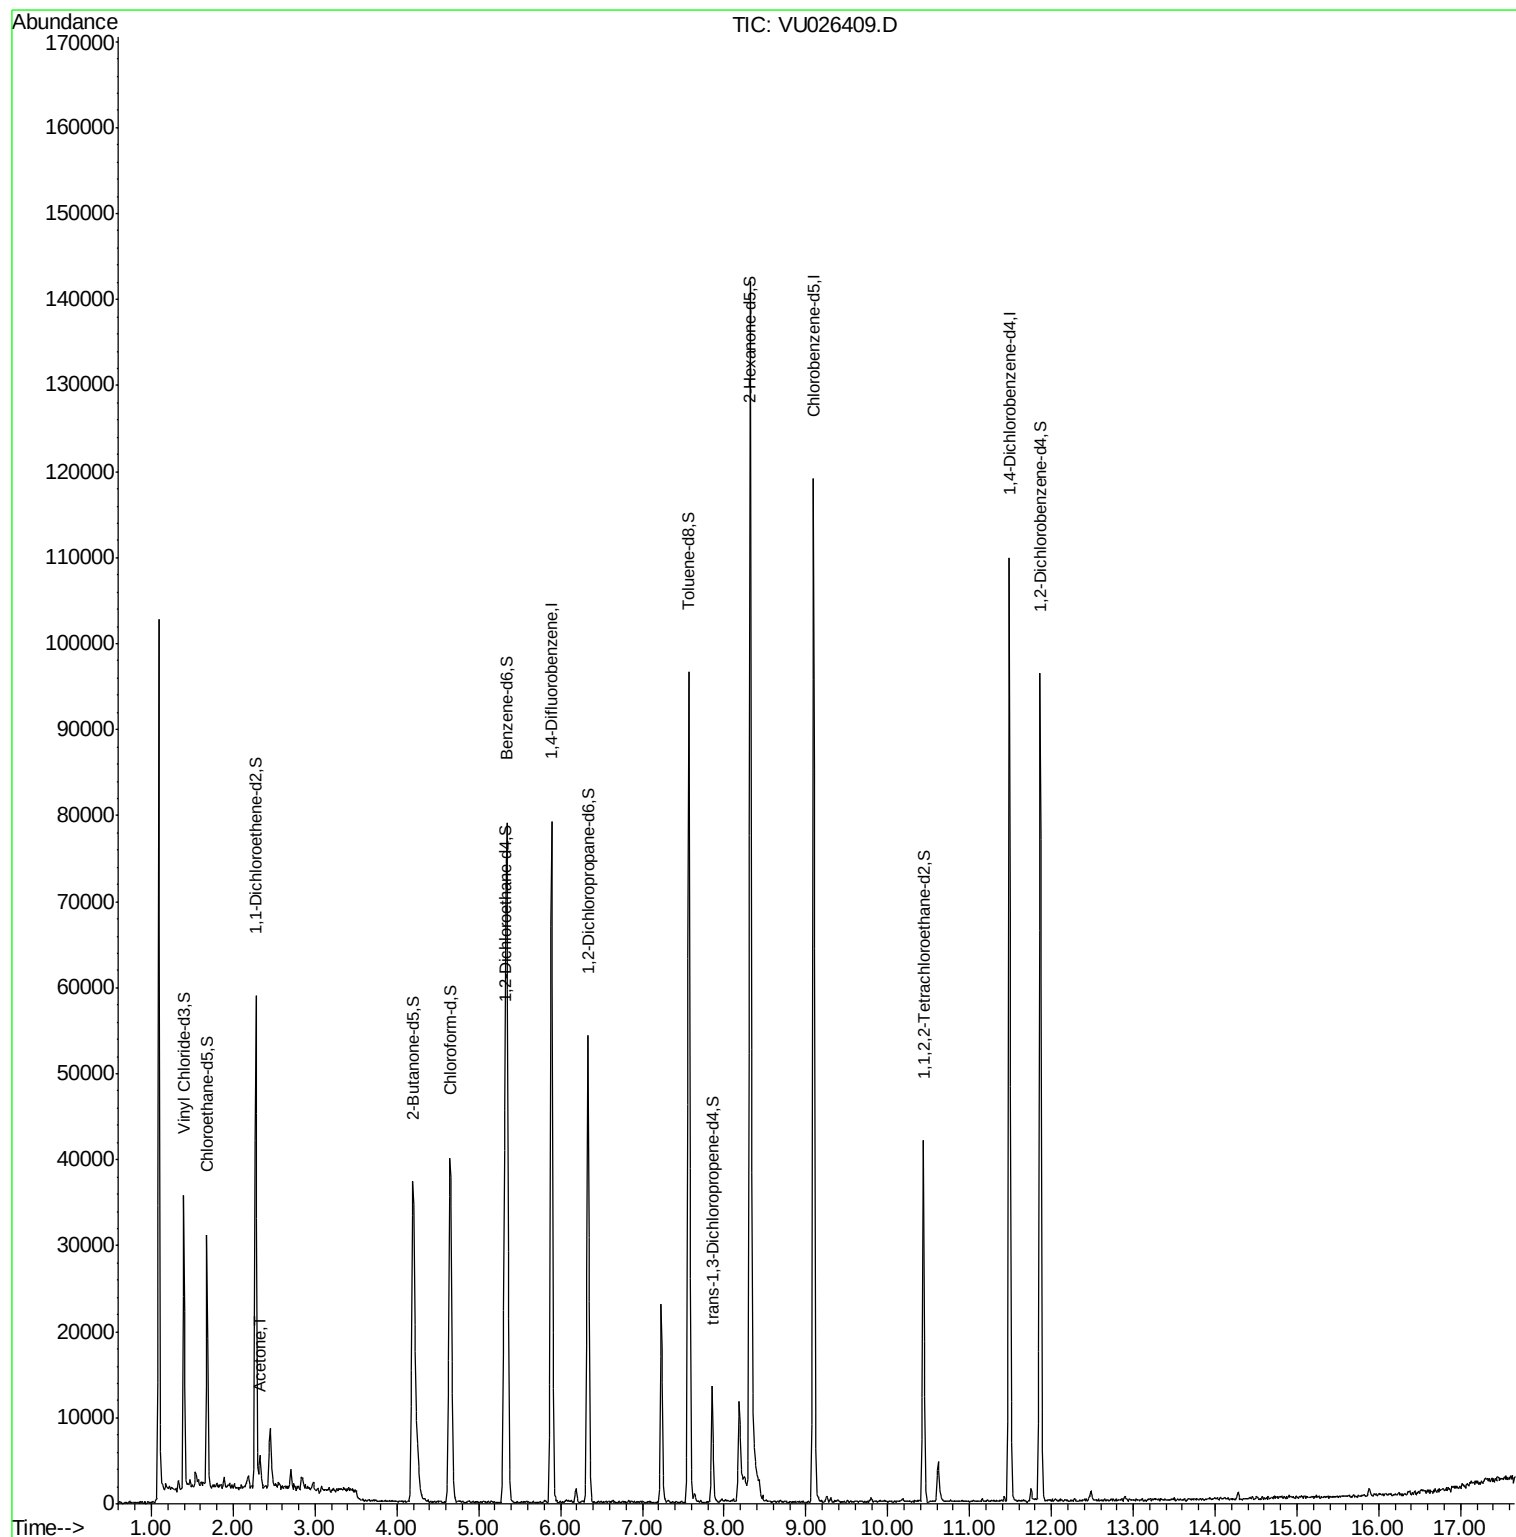

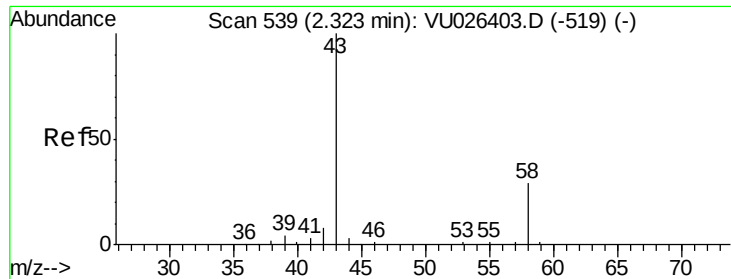

#13

Acetone

Concen: 3.12 ug/L

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU026409.D

Acq: 28 Aug 2018 20:07

Instrument :
MSVOA_U
ClientSampleId :
DB3K2

Tot Ion: 43 Resp: 3613

Ion Ratio Lower Upper

43 100

58 24.9 0.0 60.6

