

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
 Data File : VU026410.D
 Acq On : 28 Aug 2018 20:32
 Operator : MD/SY
 Sample : J4633-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB3K0

Quant Time: Aug 29 02:06:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 00:08:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	61247	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	61050	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	27283	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	20696	2.53	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	50.60%
7) Chloroethane-d5	1.68	69	19222	3.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	62.60%#
11) 1,1-Dichloroethene-d2	2.27	63	32921	2.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.60%#
20) 2-Butanone-d5	4.20	46	59609	39.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.02%
24) Chloroform-d	4.65	84	34264	3.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.20%
26) 1,2-Dichloroethane-d4	5.31	65	21722	3.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.00%
32) Benzene-d6	5.34	84	72837	3.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.80%#
36) 1,2-Dichloropropane-d6	6.34	67	24755	3.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.40%
41) Toluene-d8	7.57	98	62264	3.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.60%#
43) trans-1,3-Dichloropropene-	7.85	79	7462	2.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	59.20%
46) 2-Hexanone-d5	8.32	63	43826	39.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.28%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	19723	3.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	73.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	24654	3.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	77.40%#


Target Compounds					Ovalue
13) Acetone	2.33	43	4763	4.28 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU082818\
Data File : VU026410.D
Acq On : 28 Aug 2018 20:32
Operator : MD/SY
Sample : J4633-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB3K0

Quant Time: Aug 29 02:06:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 00:08:04 2018
Response via : Initial Calibration

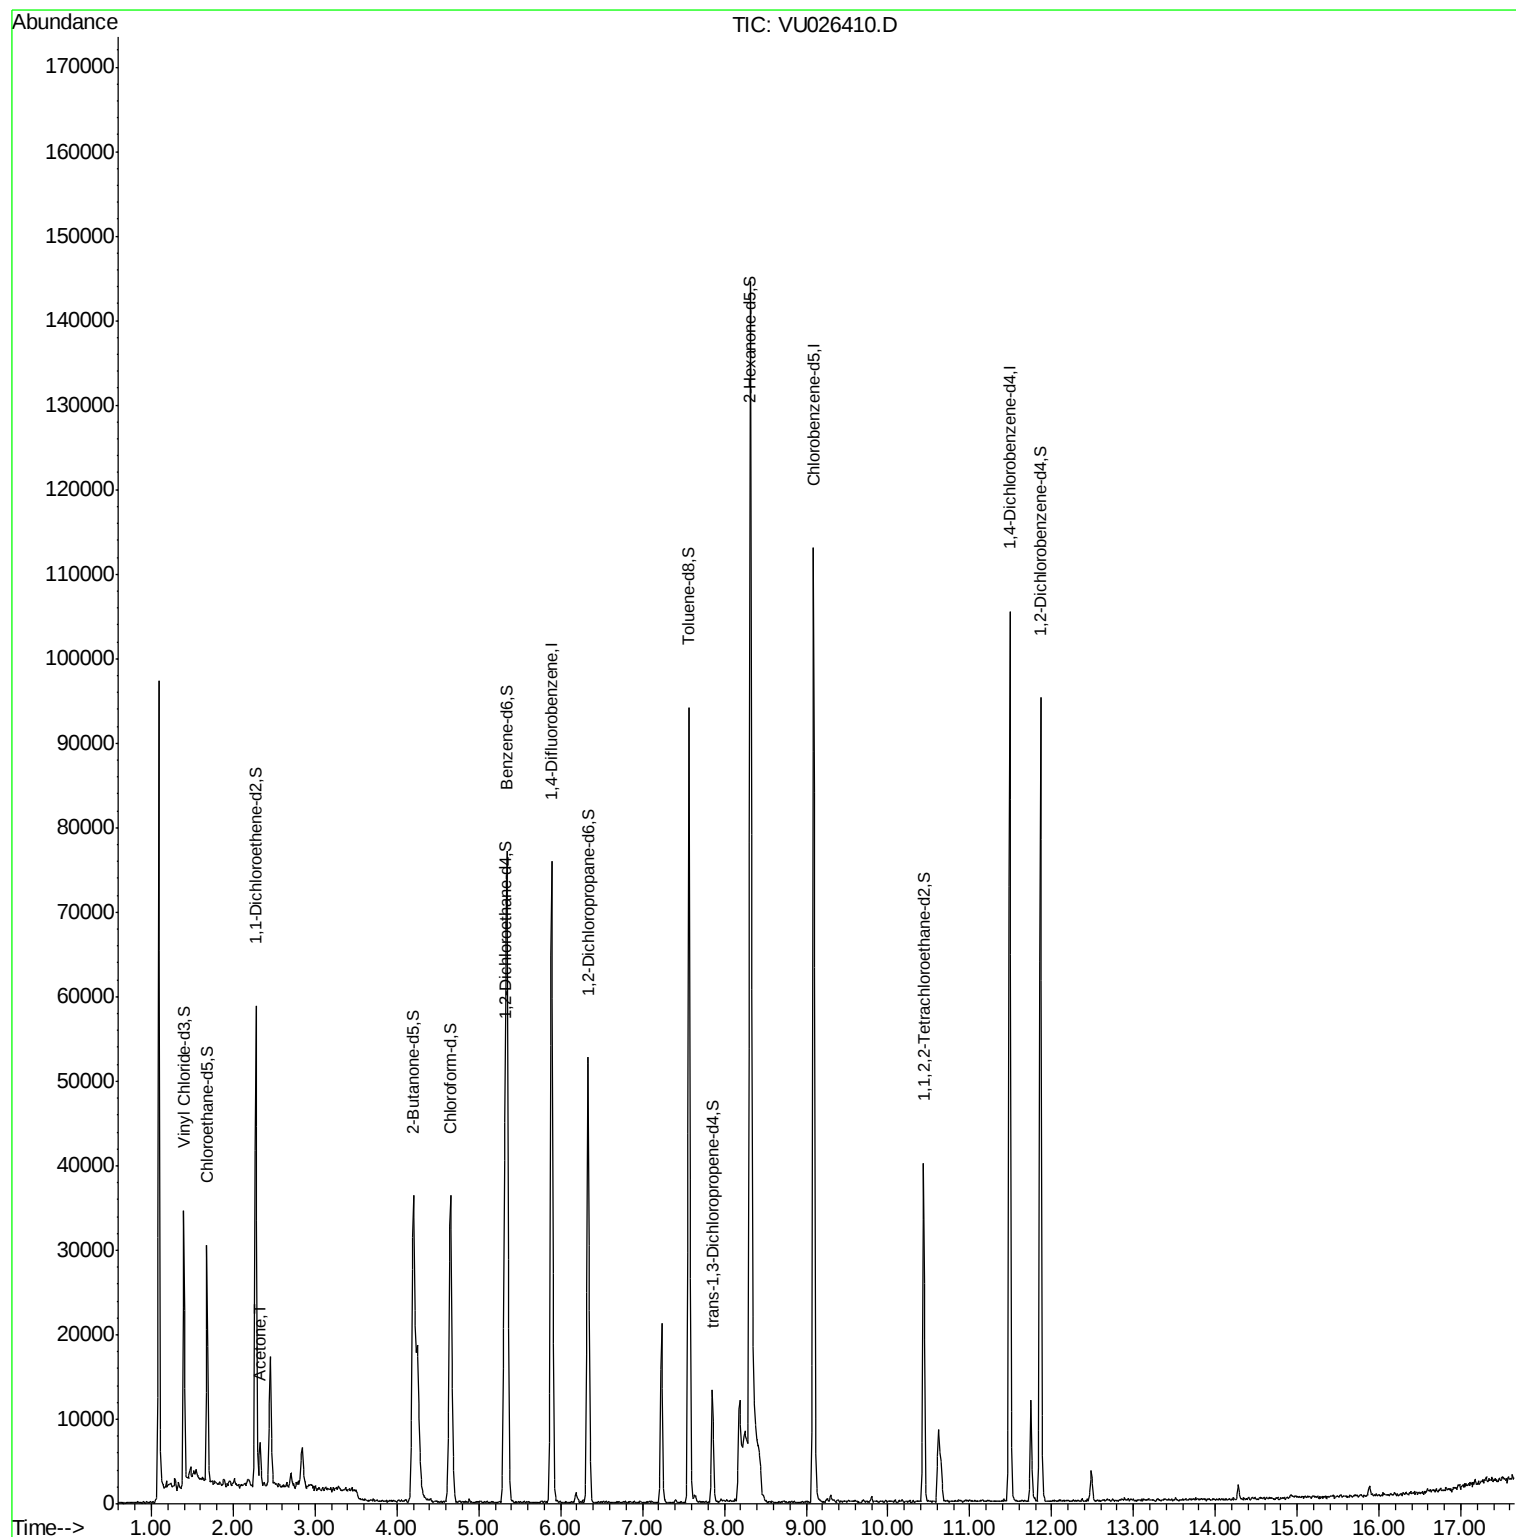

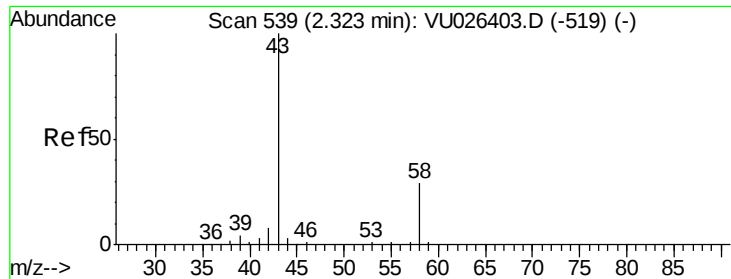

#13

Acetone

Concen: 4.28 ug/L

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU026410.D

Acq: 28 Aug 2018 20:32

Instrument :
MSVOA_U
ClientSampleId :
DB3K0

Tot Ion: 43 Resp: 4763

Ion Ratio Lower Upper

43 100

58 29.1 0.0 60.6

