

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
 Data File : VU026413.D
 Acq On : 28 Aug 2018 21:44
 Operator : MD/SY
 Sample : J4633-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB3J6

Quant Time: Aug 29 02:16:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 00:08:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	57406	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	58169	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	25615	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	20129	2.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.60%
7) Chloroethane-d5	1.68	69	18726	3.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	65.20%
11) 1,1-Dichloroethene-d2	2.27	63	31981	2.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.40%#
20) 2-Butanone-d5	4.20	46	57122	40.39	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.78%
24) Chloroform-d	4.65	84	35518	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.00%
26) 1,2-Dichloroethane-d4	5.31	65	20746	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.40%
32) Benzene-d6	5.34	84	69950	3.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.20%
36) 1,2-Dichloropropane-d6	6.33	67	24607	3.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	74.60%
41) Toluene-d8	7.57	98	59343	3.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.60%#
43) trans-1,3-Dichloropropene-	7.85	79	7322	3.05	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.00%
46) 2-Hexanone-d5	8.32	63	40448	37.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.82%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	19385	3.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	25718	4.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.00%


Target Compounds					Ovalue
13) Acetone	2.33	43	5692	5.45 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
Data File : VU026413.D
Acq On : 28 Aug 2018 21:44
Operator : MD/SY
Sample : J4633-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB3J6

Quant Time: Aug 29 02:16:49 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 00:08:04 2018
Response via : Initial Calibration

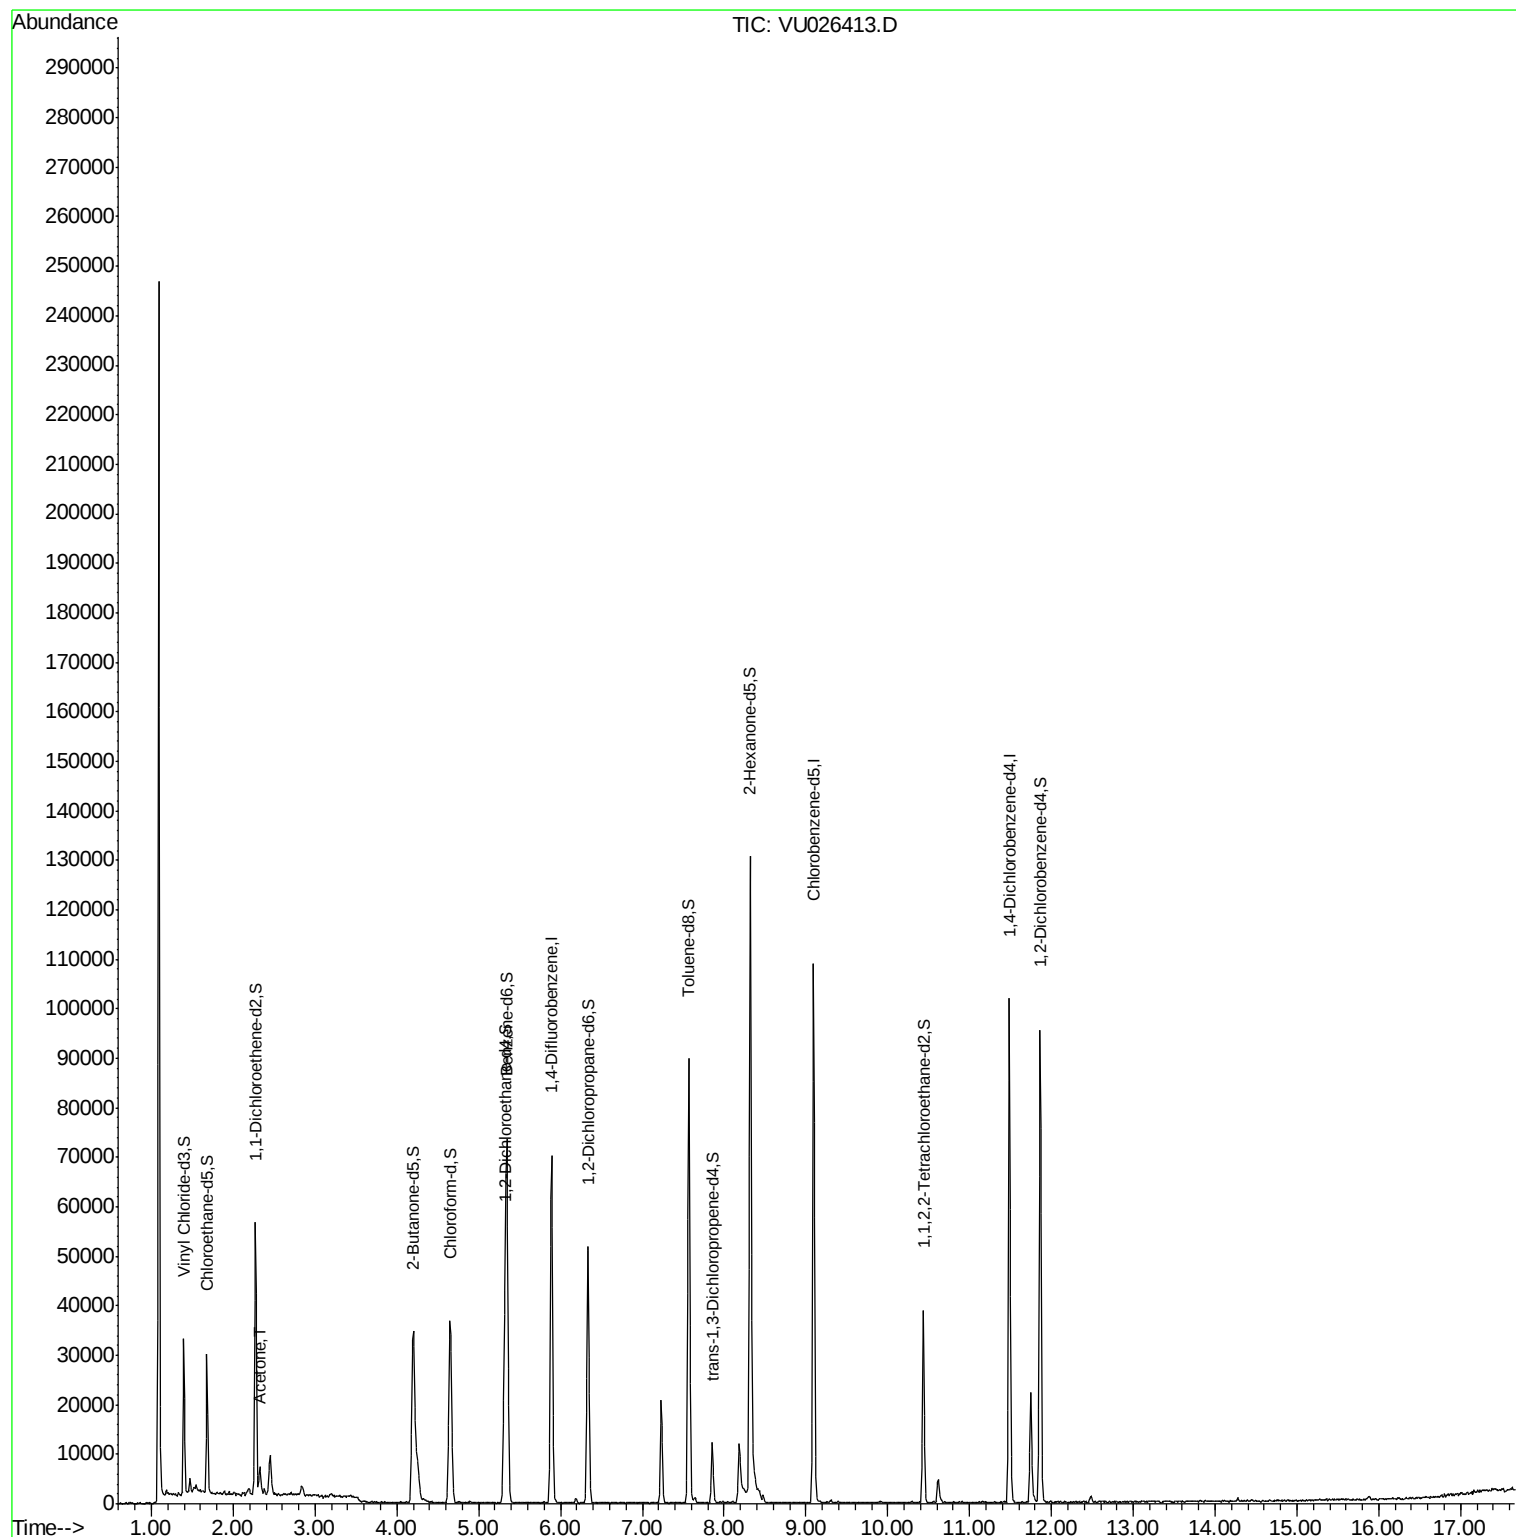

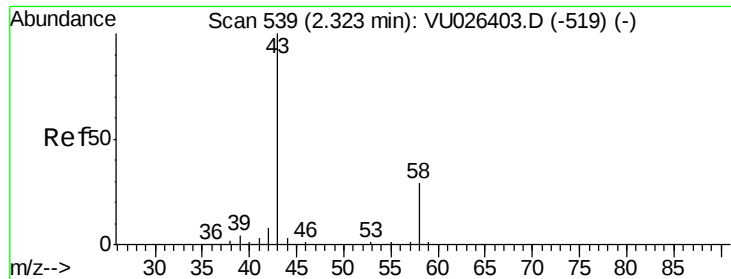

#13

Acetone

Concen: 5.45 ug/L

RT: 2.33 min Scan# 540

Delta R.T. 0.00 min

Lab File: VU026413.D

Acq: 28 Aug 2018 21:44

Instrument :
MSVOA_U
ClientSampleId :
DB3J6

Tot Ion: 43 Resp: 5692

Ion Ratio Lower Upper

43 100

58 27.1 0.0 60.6

