


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU082818\
 Data File : VU026400.D
 Acq On : 28 Aug 2018 15:31
 Operator : MD/SY
 Sample : BFB42
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR082818WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 29 00:08:04 2018

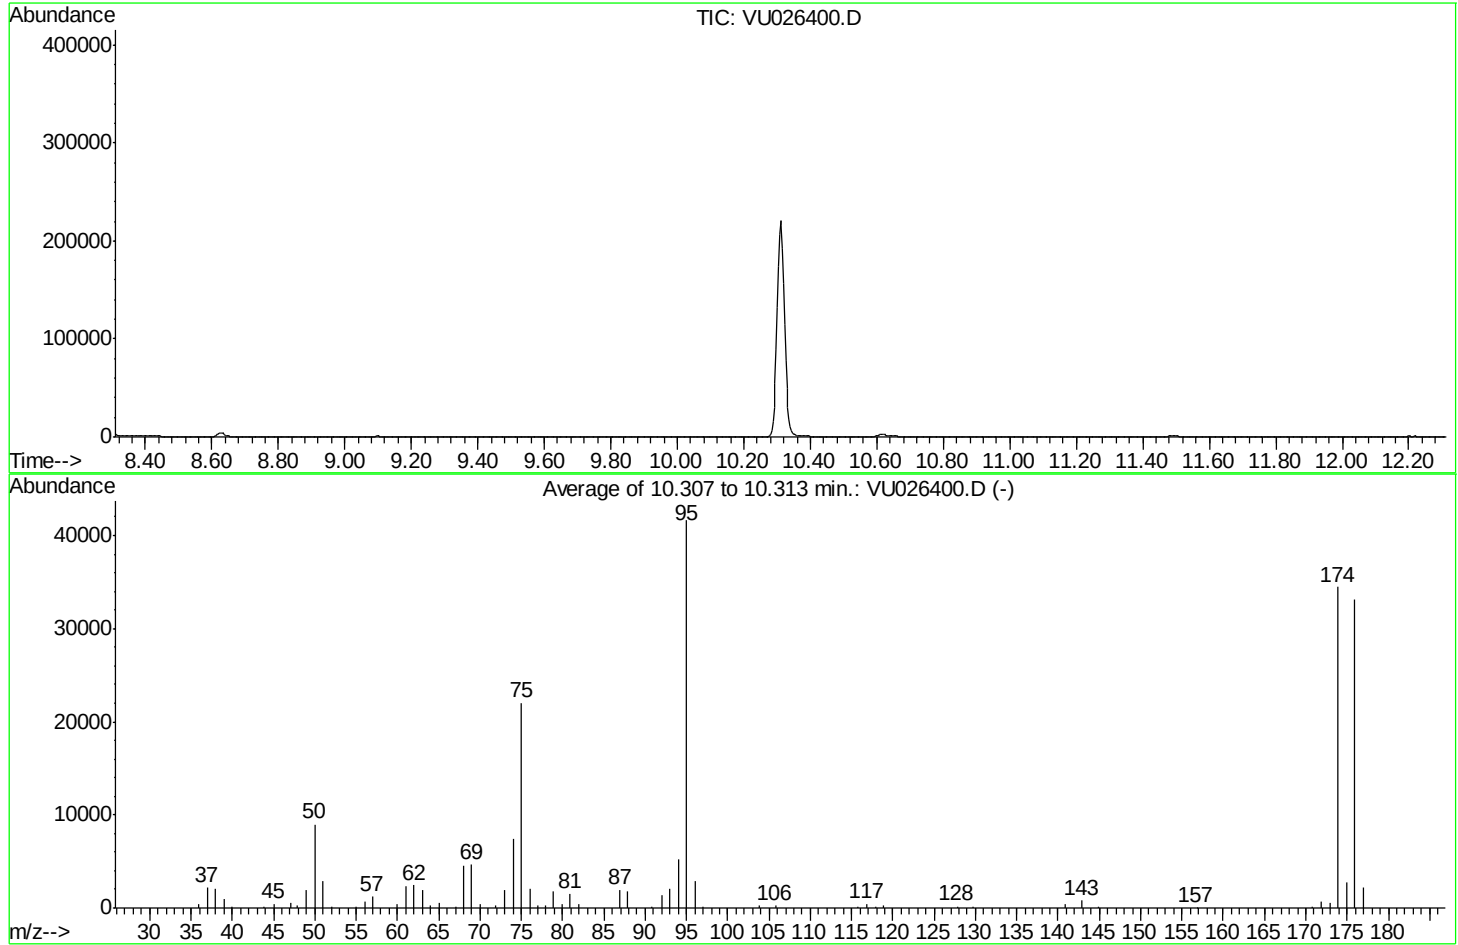

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	8999	PASS
75	95	30	80	52.9	22016	PASS
95	95	100	100	100.0	41632	PASS
96	95	5	9	6.9	2874	PASS
173	174	0.00	2	1.7	579	PASS
174	95	50	120	82.8	34490	PASS
175	174	5	9	7.8	2699	PASS
176	174	95	101	96.2	33173	PASS
177	176	5	9	6.8	2246	PASS

m/z	Abundance
43.90	337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	428.0
37.00	2086.0
38.00	2076.0
39.00	938.0
39.90	136.0
43.90	493.0
45.00	408.0
47.00	495.0
47.90	331.0
49.00	1874.0
50.00	8770.0
51.00	2817.0
52.00	118.0
55.00	167.0
56.00	658.0
57.00	1256.0
60.00	425.0
61.00	2328.0
62.00	2386.0
63.00	1804.0
64.00	364.0
65.00	468.0
67.00	138.0
68.00	4468.0
69.00	4578.0
70.00	329.0
72.00	189.0
73.00	1879.0
74.00	7286.0
75.00	21632.0
76.00	2054.0
76.90	216.0
77.80	157.0
78.90	1757.0
79.90	469.0
80.90	1477.0
81.90	361.0
87.00	2004.0
87.90	1792.0
90.80	172.0
92.00	1363.0
93.00	1896.0
94.00	5030.0
95.00	40184.0
96.00	2814.0
97.00	106.0
103.90	194.0
105.80	198.0
115.80	155.0
116.90	389.0
117.90	160.0
118.90	248.0
127.80	140.0
129.80	147.0
140.90	416.0
142.90	750.0
144.80	187.0
170.80	115.0
171.90	574.0
172.90	546.0
173.90	32672.0
174.90	2614.0
175.90	31400.0
176.90	2134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	444.0
37.00	2184.0
38.00	2178.0
39.00	1016.0
39.90	142.0
44.00	558.0
45.00	440.0
47.10	576.0
47.90	327.0
49.00	1956.0
50.00	9278.0
51.00	3038.0
52.00	151.0
55.00	179.0
56.00	712.0
57.00	1227.0
60.00	423.0
61.00	2437.0
62.00	2486.0
63.00	1920.0
64.00	336.0
65.00	507.0
67.00	134.0
68.00	4610.0
69.00	4765.0
70.00	384.0
71.90	208.0
73.00	2001.0
74.00	7745.0
75.00	22576.0
76.00	2174.0
77.00	244.0
77.90	210.0
78.90	1895.0
79.90	477.0
80.90	1614.0
81.90	394.0
87.00	2034.0
87.90	1848.0
90.90	195.0
92.00	1397.0
93.00	2065.0
94.00	5428.0
95.00	43016.0
96.00	2940.0
97.00	112.0
103.90	222.0
105.80	228.0
115.80	156.0
116.90	455.0
117.90	167.0
118.90	271.0
127.80	149.0
129.70	139.0
140.90	486.0
142.90	855.0
144.80	210.0
170.80	128.0
171.90	631.0
173.00	585.0
173.90	35480.0
174.90	2800.0
175.90	34120.0
176.90	2336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	454.0
37.00	2139.0
38.00	2040.0
39.00	961.0
39.90	137.0
44.00	593.0
45.00	422.0
47.00	652.0
47.90	282.0
49.00	1785.0
50.00	8949.0
51.00	2900.0
52.00	162.0
55.00	152.0
56.00	694.0
57.00	1181.0
59.90	381.0
61.00	2411.0
62.00	2406.0
63.00	1871.0
64.00	277.0
65.00	562.0
67.00	118.0
68.00	4409.0
69.00	4552.0
70.00	383.0
71.90	247.0
73.00	1971.0
74.00	7453.0
75.00	21840.0
76.00	2017.0
77.00	258.0
77.90	279.0
78.90	1797.0
79.90	447.0
80.90	1613.0
82.00	352.0
86.90	1873.0
87.90	1657.0
90.90	173.0
92.00	1291.0
93.00	2104.0
94.00	5148.0
95.00	41696.0
96.00	2868.0
97.00	115.0
103.80	224.0
105.80	228.0
115.80	161.0
116.90	412.0
117.90	182.0
118.80	290.0
127.80	155.0
129.70	130.0
140.90	491.0
142.90	774.0
144.90	199.0
156.80	106.0
170.80	112.0
171.90	738.0
173.00	608.0
173.90	35320.0
174.90	2685.0
175.90	34000.0
176.90	2270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42