

Data File : VU033985.D
Acq On : 27 Aug 2019 20:17
Operator : JC/SP
Sample : K4516-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)

Quant Time: Aug 28 04:06:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 28 02:42:03 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	395813	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.86	114	572347	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	545162	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.47	152	254261	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	205857	46.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.62%	
35) Dibromofluoromethane	4.86	113	181763	47.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.48%	
50) Toluene-d8	7.55	98	706288	49.77	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.54%	
62) 4-Bromofluorobenzene	10.29	95	235032	43.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.36%	


Target Compounds						Qvalue
3) Chloromethane	1.32	50	1677	1.294	ug/l	93
5) Bromomethane	1.62	94	1218	0.504	ug/l #	54
8) Diethyl Ether	2.09	74	528	0.266	ug/l #	38
11) Tert butyl alcohol	2.82	59	3588	3.150	ug/l #	85
16) Acetone	2.31	43	7447	3.538	ug/l	99
18) Methyl Acetate	2.61	43	3108	0.600	ug/l	97
20) Methylene Chloride	2.69	84	13021	2.916	ug/l	99
31) Cyclohexane	4.96	56	6391	0.986	ug/l #	1
36) 1,1-Dichloropropene	4.96	75	24898	4.750	ug/l #	48
38) Carbon Tetrachloride	4.96	117	33623	6.294	ug/l #	17
43) Isopropyl Acetate	5.53	43	56786	7.044	ug/l	99
48) Methyl methacrylate	6.68	41	87447	22.814	ug/l #	35
49) 1,4-Dioxane	6.68	88	65	0.618	ug/l #	1
51) 4-Methyl-2-Pentanone	7.40	43	51118	9.196	ug/l #	45
54) cis-1,3-Dichloropropene	7.40	75	29092	4.506	ug/l #	57
56) Ethyl methacrylate	8.01	69	65	2.524	ug/l #	29
57) 1,3-Dichloropropane	8.40	76	4668	0.690	ug/l #	43
59) 2-Hexanone	8.40	43	59436	13.911	ug/l #	52
74) N-amyl acetate	9.92	43	2614	0.426	ug/l #	40
76) 1,2,3-Trichloropropane	10.29	75	109771	21.668	ug/l #	36
81) trans-1,4-Dichloro-2-buten	10.29	75	109771	62.061	ug/l #	100
93) 1,2,4-Trichlorobenzene	13.55	180	277	1.788	ug/l #	41
95) Naphthalene	13.76	128	301	2.101	ug/l #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU033985.D
Acq On : 27 Aug 2019 20:17
Operator : JC/SP
Sample : K4516-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)

Quant Time: Aug 28 04:06:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 28 02:42:03 2019
Response via : Initial Calibration

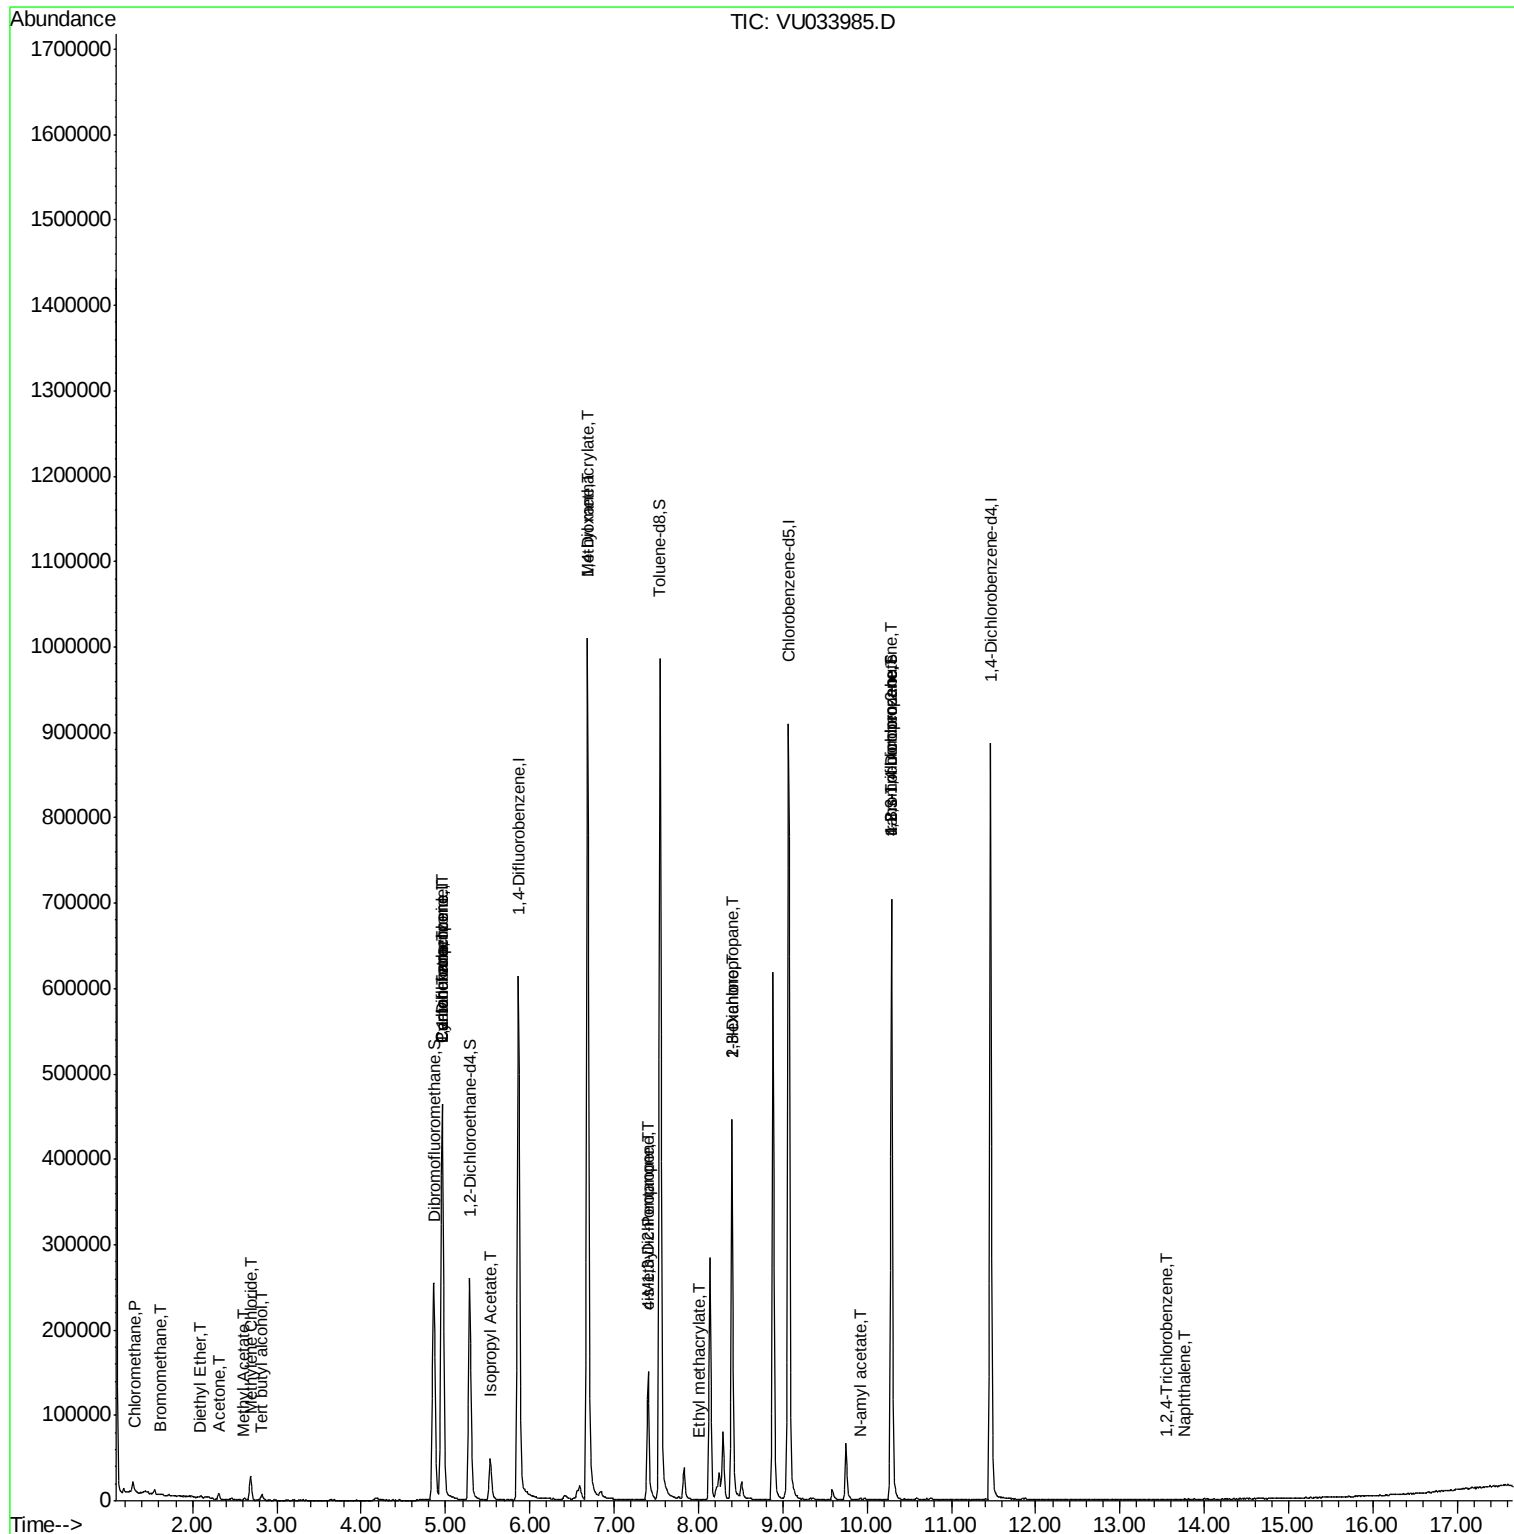

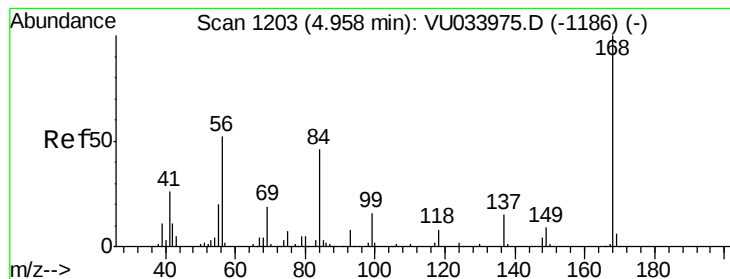

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :


T1-S-B2-(0)

Tgt Ion:168 Resp: 395813

Ion Ratio Lower Upper

168 100

99 49.6 39.4 59.2



Abundance Ion 167.90 (167.60 to 168.60): VU033975.D (-1186) (-)

Ion 98.90 (98.60 to 99.60): VU033975.D (-1186) (-)

4.96



150000

100000

50000

0

Time-->

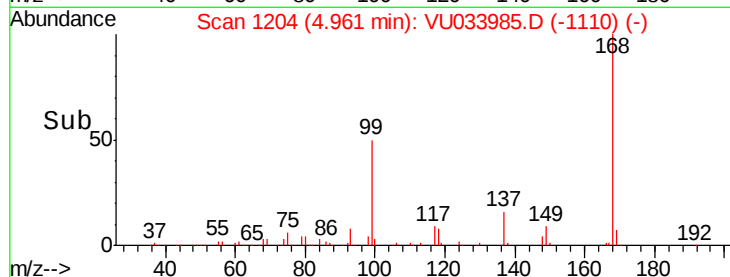

#3

Chloromethane

Concen: 1.294 ug/l

RT: 1.32 min Scan# 73

Delta R.T. 0.01 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 50 Resp: 1677

Ion Ratio Lower Upper

50 100

52 36.7 26.2 39.2



Abundance Ion 49.90 (49.60 to 50.60): VU033975.D (-63) (-)

Ion 51.90 (51.60 to 52.60): VU033975.D (-63) (-)

1.32


1500


1000

500

0

Time-->

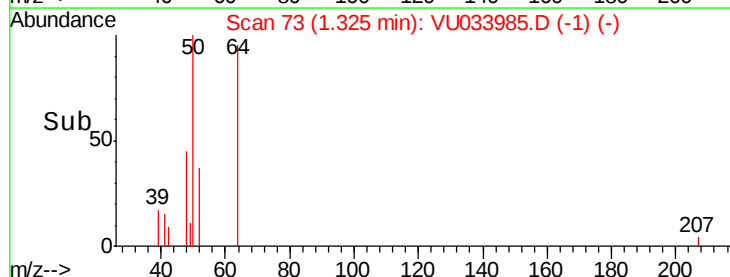



#5

Bromomethane

Concen: 0.504 ug/l

RT: 1.62 min Scan# 166

Delta R.T. 0.00 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :


T1-S-B2-(0)

Tgt Ion: 94 Resp: 1218




Ion Ratio Lower Upper

94 100

96 50.1 76.3 114.5#



Abundance Ion 93.90 (93.60 to 94.60): VU033975.D (-156) (-)

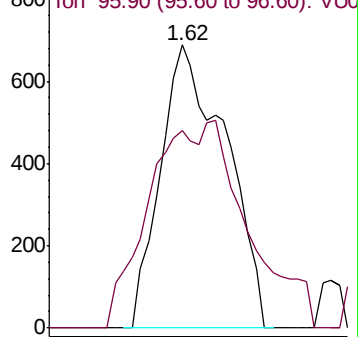

#8

Diethyl Ether

Concen: 0.266 ug/l

RT: 2.09 min Scan# 312

Delta R.T. 0.00 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 74 Resp: 528



Ion Ratio Lower Upper


74 100

45 142.4 42.8 128.4#



Abundance Ion 74.00 (73.70 to 74.70): VU033975.D (-301) (-)

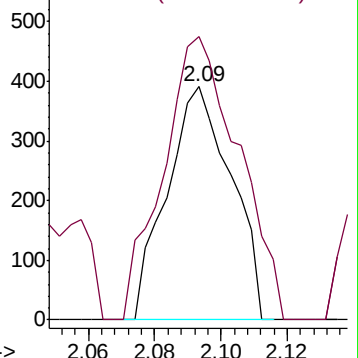

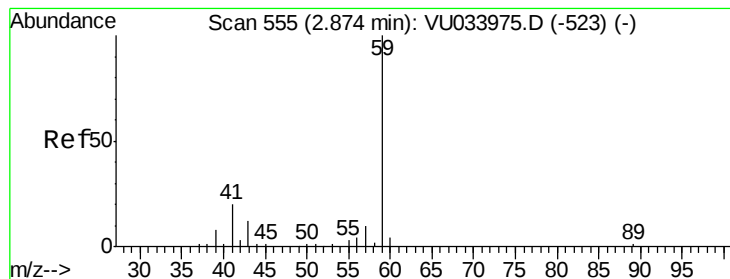

#11

Tert butyl alcohol

Concen: 3.150 ug/l

RT: 2.82 min Scan# 539

Delta R.T. -0.05 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :


T1-S-B2-(0)

Tgt Ion: 59 Resp: 3588

Ion Ratio Lower Upper

59 100

57 0.0 3.9 5.9#



Abundance Ion 59.00 (58.70 to 59.70): VU033975.D (-523) (-)

Ion 57.00 (56.70 to 57.70): VU033975.D (-523) (-)

2.82



1500

1000

500

0

Time-->

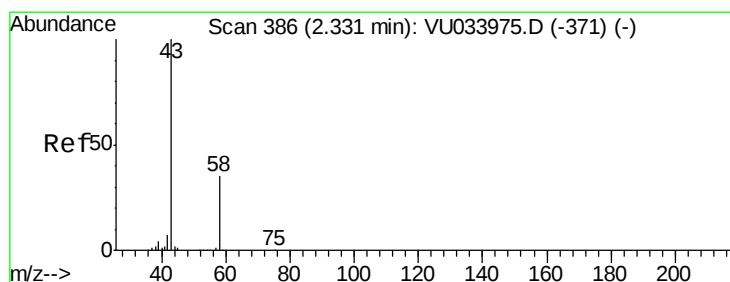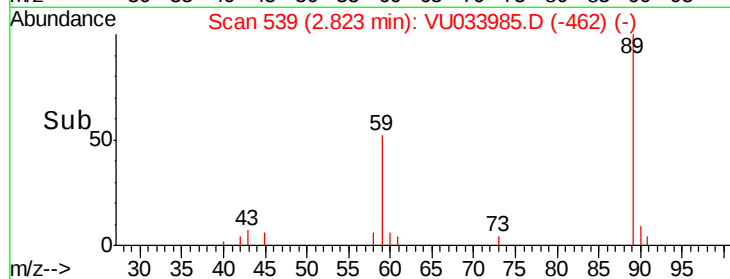

#16

Acetone

Concen: 3.538 ug/l

RT: 2.31 min Scan# 379

Delta R.T. -0.02 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 43 Resp: 7447

Ion Ratio Lower Upper

43 100

58 34.4 28.0 42.0

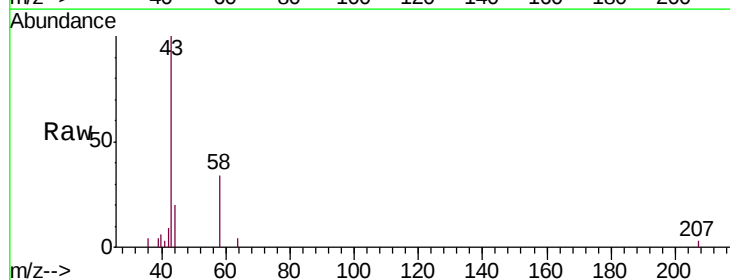

Abundance Ion 43.00 (42.70 to 43.70): VU033975.D (-371) (-)

Ion 58.00 (57.70 to 58.70): VU033975.D (-371) (-)

2.31

5000

4000


3000


2000

1000

0

Time-->




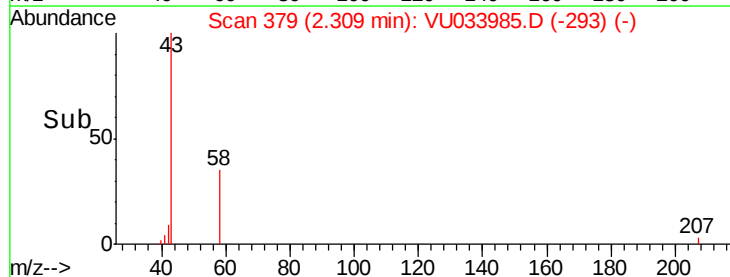


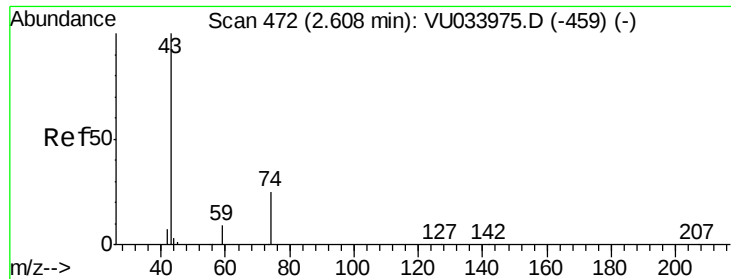

#18
Methyl Acetate
Concen: 0.600 ug/l
RT: 2.61 min Scan# 473
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17




Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)


Tgt Ion: 43 Resp: 3108
Ion Ratio Lower Upper
43 100
74 24.0 20.5 30.7

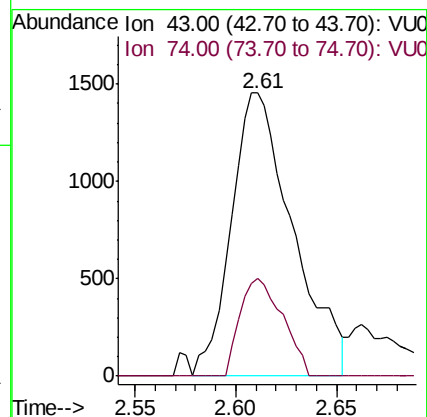

#20
Methylene Chloride
Concen: 2.916 ug/l
RT: 2.69 min Scan# 497
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Tgt Ion: 84 Resp: 13021
Ion Ratio Lower Upper
84 100
49 114.2 91.3 136.9
51 33.1 28.9 43.3
86 63.1 50.9 76.3

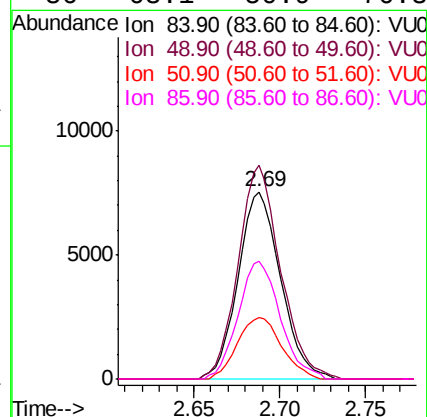

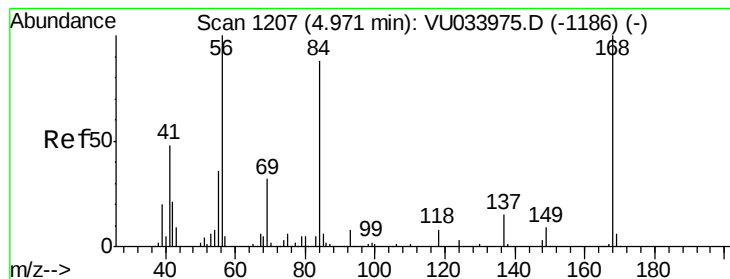

#31

Cyclohexane

Concen: 0.986 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. -0.01 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :

T1-S-B2-(0)


Tgt Ion: 56 Resp: 6391

Ion Ratio Lower Upper

56 100

69 192.4 25.9 38.9#




84 171.4 70.4 105.6#



Abundance Ion 56.00 (55.70 to 56.70): VU033975.D (-1186) (-)

Ion 69.00 (68.70 to 69.70): VU033975.D (-1186) (-)

Ion 84.00 (83.70 to 84.70): VU033975.D (-1186) (-)

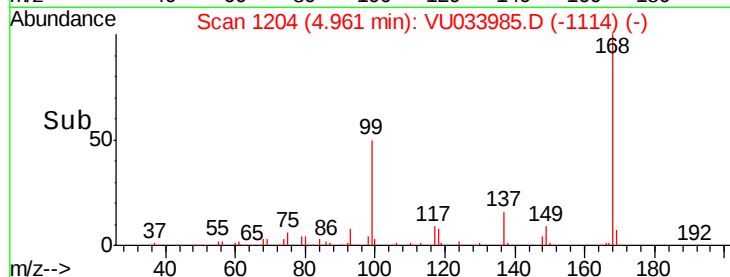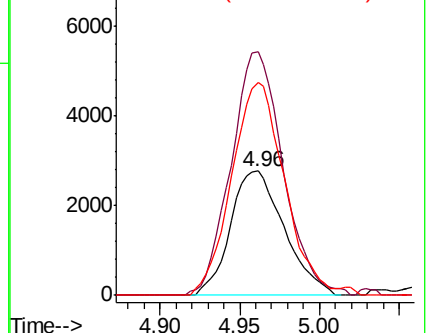

#33

1,2-Dichloroethane-d4

Concen: 46.814 ug/l

RT: 5.29 min Scan# 1305

Delta R.T. 0.00 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 65 Resp: 205857

Ion Ratio Lower Upper



65 100


67 54.2 0.0 111.0



Abundance Ion 64.90 (64.60 to 65.60): VU033975.D (-1289) (-)

Ion 66.90 (66.60 to 67.60): VU033975.D (-1289) (-)

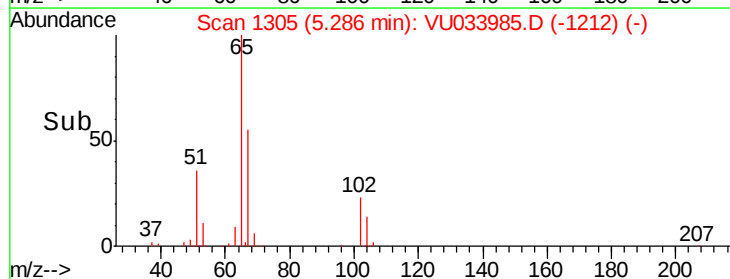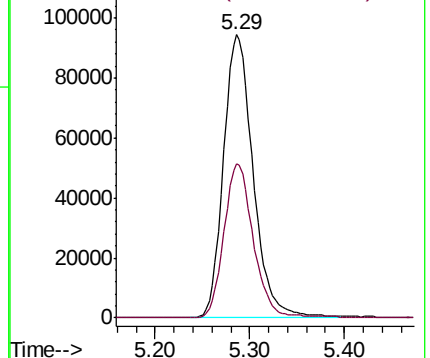

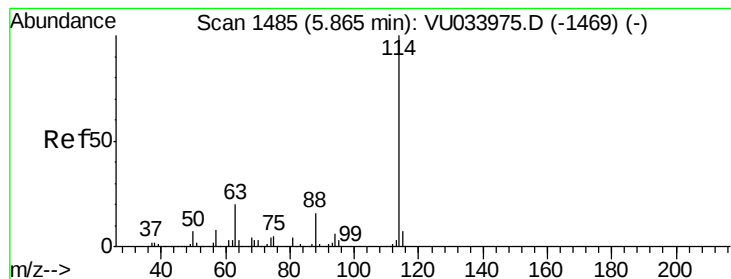

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.86 min Scan# 1485

Delta R.T. 0.00 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :

T1-S-B2-(0)


Tgt Ion:114 Resp: 572347

Ion Ratio Lower Upper

114 100

63 19.3 0.0 39.0




88 15.7 0.0 31.2



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

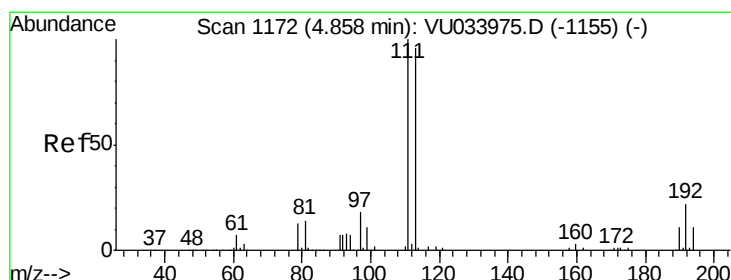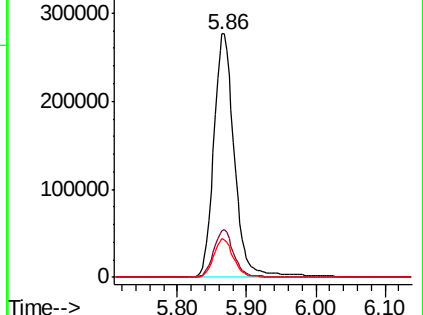

#35

Dibromofluoromethane

Concen: 47.245 ug/l

RT: 4.86 min Scan# 1172

Delta R.T. 0.00 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17


Tgt Ion:113 Resp: 181763

Ion Ratio Lower Upper

113 100

111 101.8 81.7 122.5



192 23.3 18.6 27.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

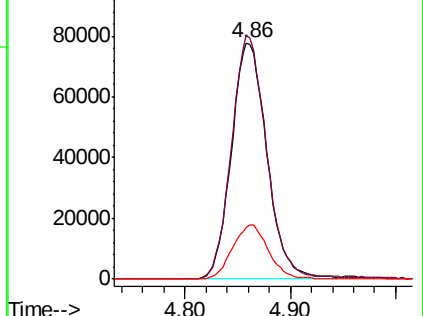


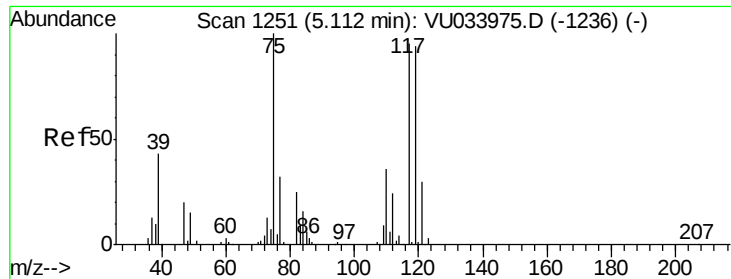




#36
 1,1-Dichloropropene
 Concen: 4.750 ug/l
 RT: 4.96 min Scan# 1203
 Delta R.T. -0.15 min
 Lab File: VU033985.D
 Acq: 27 Aug 2019 20:17

Instrument :
 MSVOA_U
 ClientSampleId :
 T1-S-B2-(0)

Tgt Ion: 75 Resp: 24898
 Ion Ratio Lower Upper
 75 100
 110 8.4 18.2 54.6#
 77 0.0 24.8 37.2#

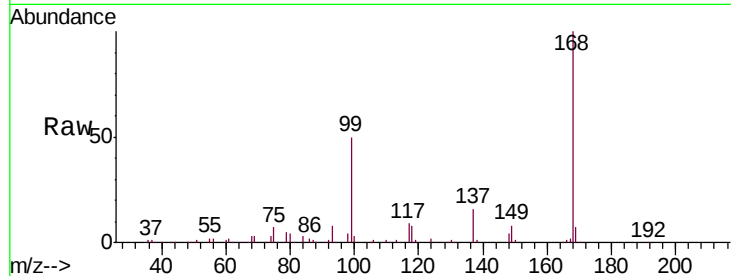


Abundance Ion 74.90 (74.60 to 75.60): VU0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VU0

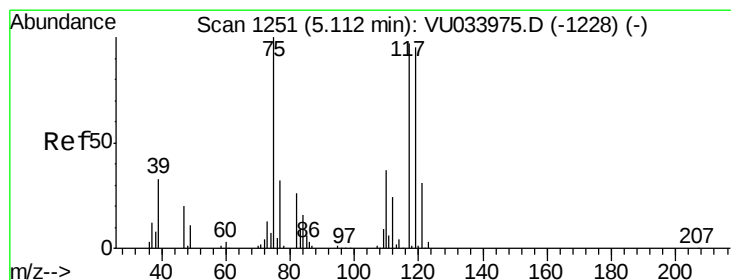
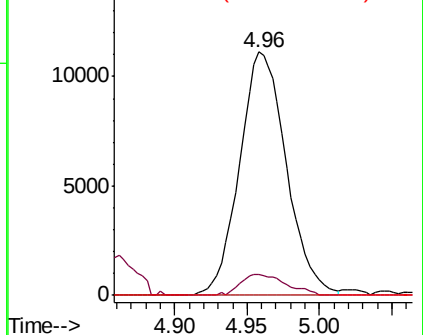



#38
 Carbon Tetrachloride
 Concen: 6.294 ug/l
 RT: 4.96 min Scan# 1204
 Delta R.T. -0.15 min
 Lab File: VU033985.D
 Acq: 27 Aug 2019 20:17

Tgt Ion: 117 Resp: 33623
 Ion Ratio Lower Upper
 117 100
 119 7.5 78.4 117.6#
 121 0.0 25.4 38.2#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V




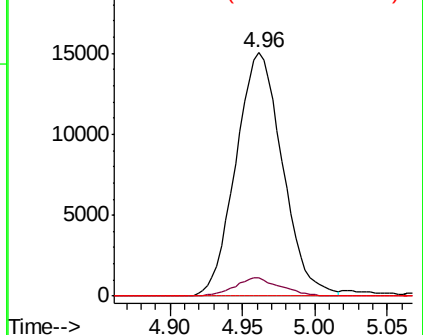




#43
Isopropyl Acetate
Concen: 7.044 ug/l
RT: 5.53 min Scan# 1381
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17




Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)


Tgt Ion: 43 Resp: 56786
Ion Ratio Lower Upper
43 100
61 22.0 17.8 26.8
87 14.5 11.9 17.9

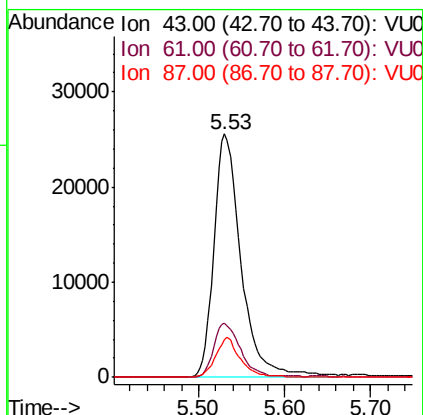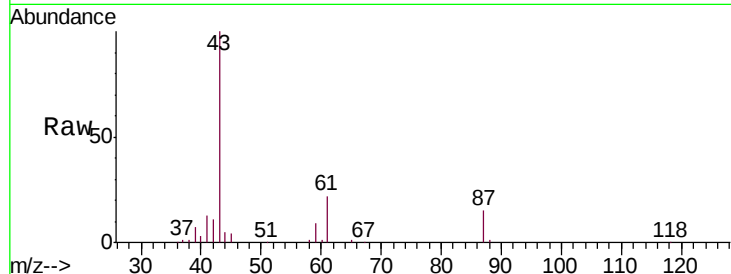

#48
Methyl methacrylate
Concen: 22.814 ug/l
RT: 6.68 min Scan# 1740
Delta R.T. 0.08 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Tgt Ion: 41 Resp: 87447
Ion Ratio Lower Upper
41 100
69 0.1 76.3 114.5#
39 48.4 41.1 61.7

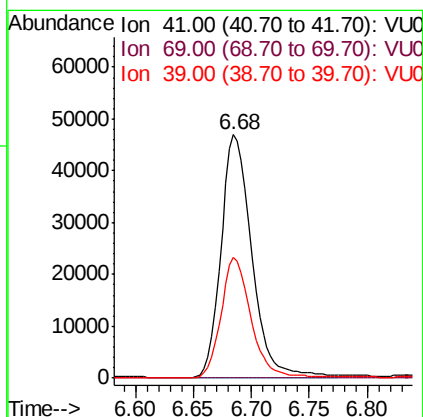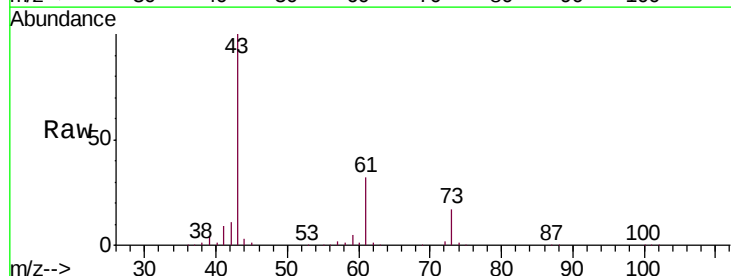



#49

1,4-Dioxane

Concen: 0.618 ug/l

RT: 6.68 min Scan# 1739

Delta R.T. 0.03 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :

T1-S-B2-(0)


Tgt Ion: 88 Resp: 65

Ion Ratio Lower Upper

88 100

43 1479866.2 0.0 0.0#




58 7723.1 56.6 85.0#



Abundance Ion 88.00 (87.70 to 88.70): VU033985.D (-1637) (-)

Ion 43.00 (42.70 to 43.70): VU033985.D (-1637) (-)

Ion 58.00 (57.70 to 58.70): VU033985.D (-1637) (-)

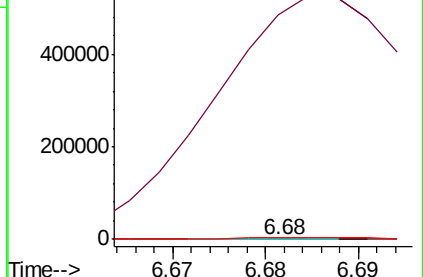

#50

Toluene-d8

Concen: 49.772 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. 0.00 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 98 Resp: 706288

Ion Ratio Lower Upper



98 100


100 64.9 51.5 77.3



Abundance Ion 98.00 (97.70 to 98.70): VU033985.D (-1915) (-)

Ion 100.00 (99.70 to 100.70): VU033985.D (-1915) (-)



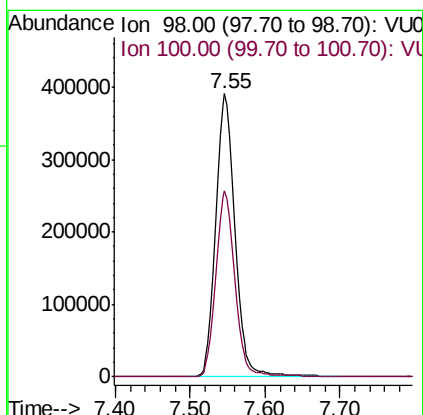



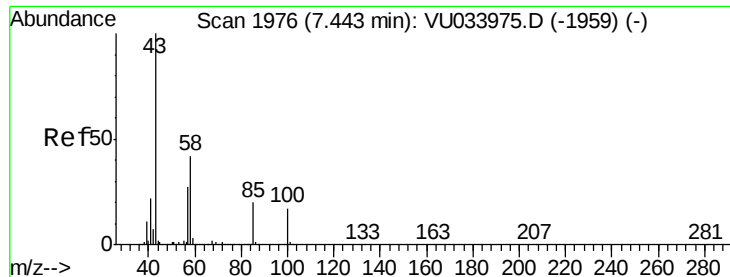

#51
 4-Methyl-2-Pentanone
 Concen: 9.196 ug/l
 RT: 7.40 min Scan# 1963
 Delta R.T. -0.04 min
 Lab File: VU033985.D
 Acq: 27 Aug 2019 20:17




Instrument :
 MSVOA_U
 ClientSampleId :
 T1-S-B2-(0)


Tgt Ion: 43 Resp: 51118
 Ion Ratio Lower Upper
 43 100
 58 7.4 33.6 50.4#

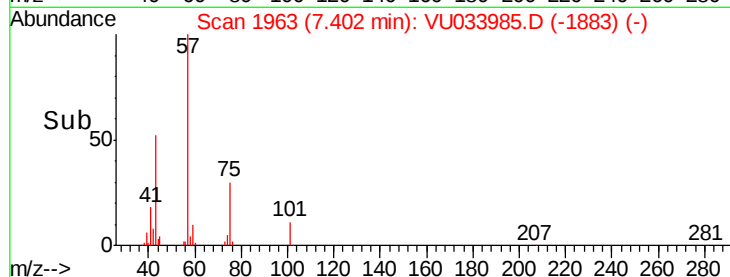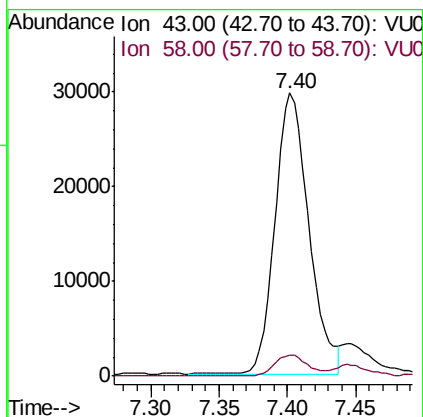

#54
 cis-1,3-Dichloropropene
 Concen: 4.506 ug/l
 RT: 7.40 min Scan# 1964
 Delta R.T. 0.15 min
 Lab File: VU033985.D
 Acq: 27 Aug 2019 20:17

Tgt Ion: 75 Resp: 29092
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.6 38.4#
 39 20.0 30.7 46.1#

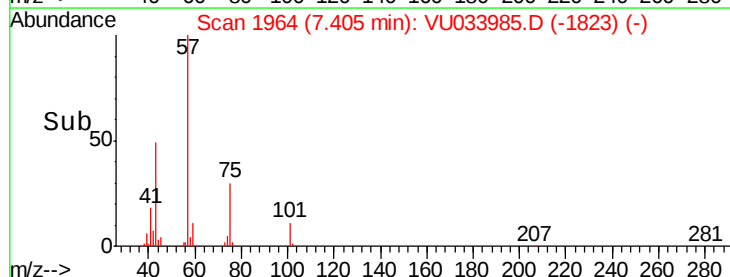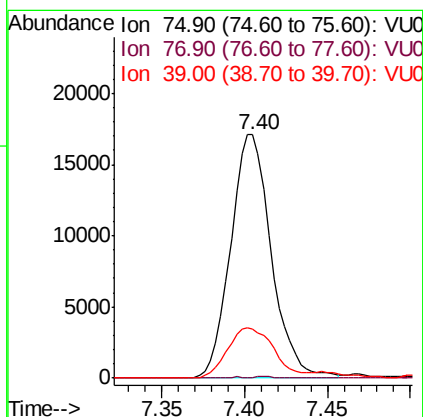


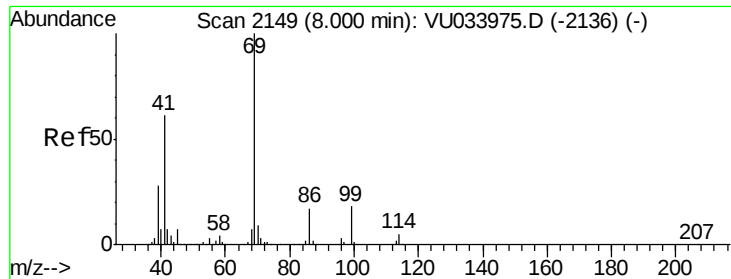




#56
Ethyl methacrylate
Concen: 2.524 ug/l
RT: 8.01 min Scan# 2153
Delta R.T. 0.01 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)

Tgt Ion: 69 Resp: 65
Ion Ratio Lower Upper
69 100
41 0.0 48.6 72.8#
39 0.0 22.4 33.6#




Abundance Ion 69.00 (68.70 to 69.70): VU0
Ion 41.00 (40.70 to 41.70): VU0
Ion 39.00 (38.70 to 39.70): VU0

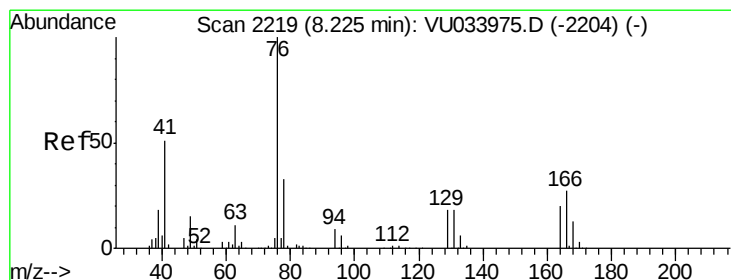
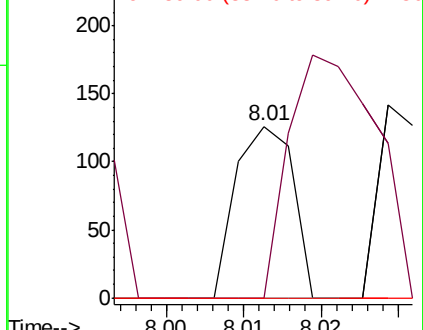



#57
1,3-Dichloropropane
Concen: 0.690 ug/l
RT: 8.40 min Scan# 2273
Delta R.T. 0.17 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Tgt Ion: 76 Resp: 4668
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#



Abundance Ion 75.90 (75.60 to 76.60): VU0
Ion 77.90 (77.60 to 78.60): VU0




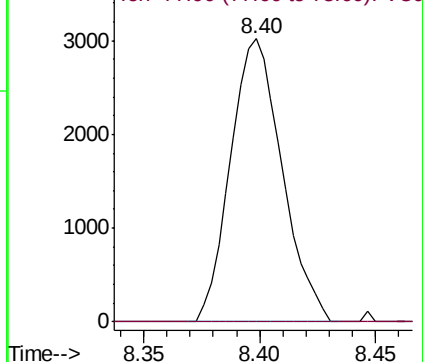


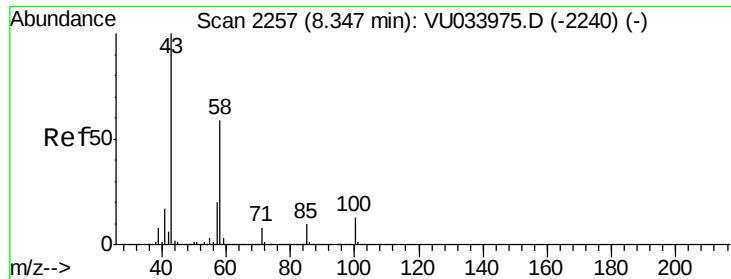

#59
2-Hexanone
Concen: 13.911 ug/l
RT: 8.40 min Scan# 2273
Delta R.T. 0.05 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17




Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)


Tgt Ion: 43 Resp: 59436
Ion Ratio Lower Upper
43 100
58 23.1 29.5 88.6#

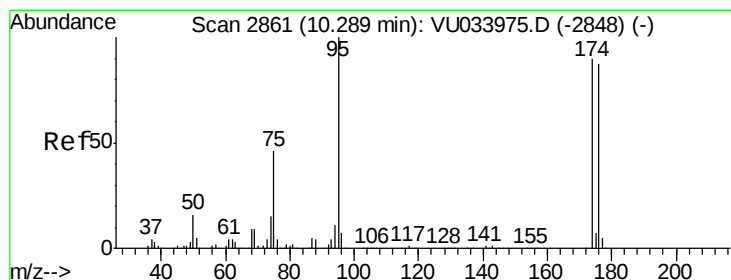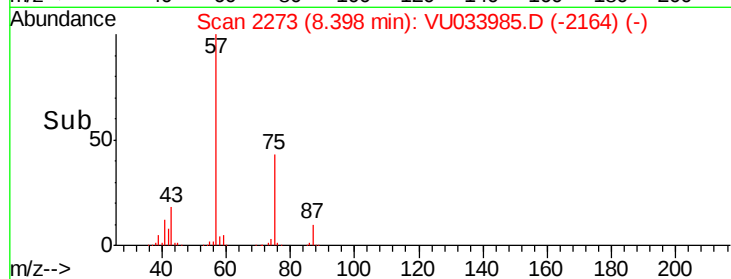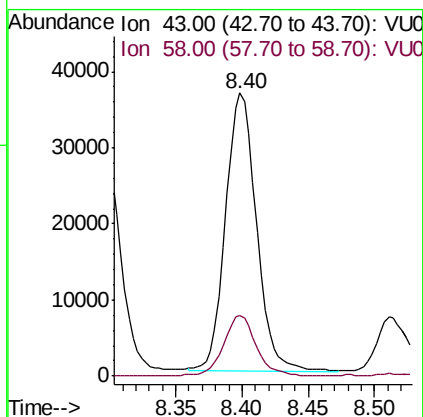

#62
4-Bromofluorobenzene
Concen: 43.177 ug/l
RT: 10.29 min Scan# 2861
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Tgt Ion: 95 Resp: 235032
Ion Ratio Lower Upper
95 100
174 94.4 0.0 183.8
176 89.4 0.0 176.4


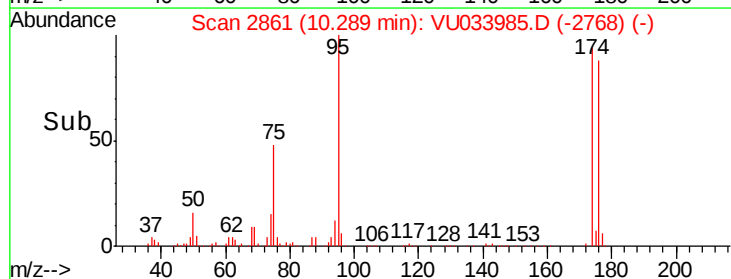
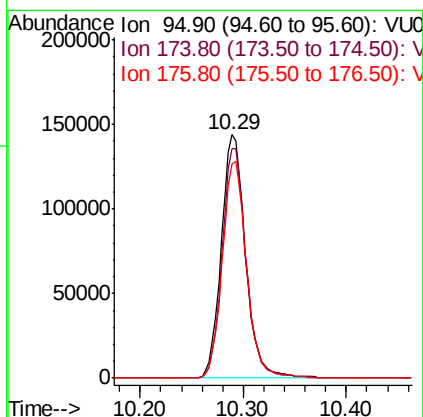
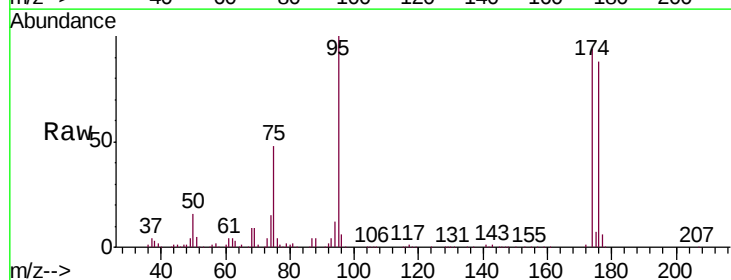




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.07 min Scan# 2482
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17




Instrument :
MSVOA_U
ClientSampleId :
T1-S-B2-(0)


Tgt Ion:117 Resp: 545162
Ion Ratio Lower Upper
117 100
82 54.1 43.8 65.8
119 32.2 25.7 38.5

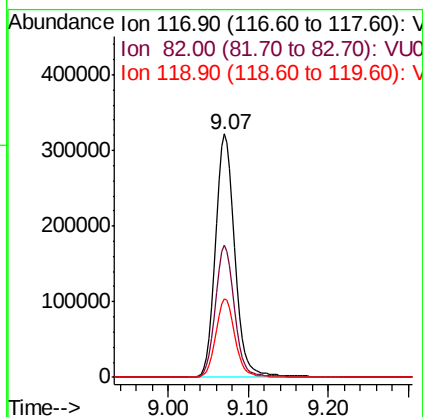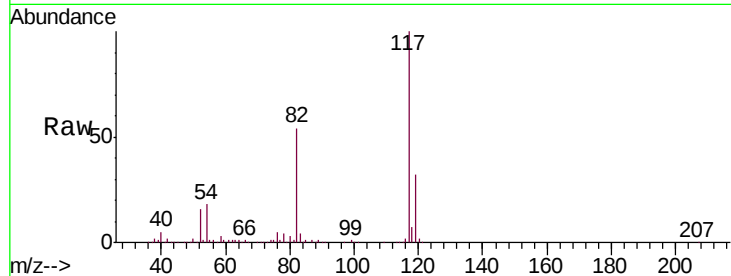

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.47 min Scan# 3227
Delta R.T. 0.00 min
Lab File: VU033985.D
Acq: 27 Aug 2019 20:17

Tgt Ion:152 Resp: 254261
Ion Ratio Lower Upper
152 100
115 54.6 38.6 115.7
150 155.0 0.0 343.8

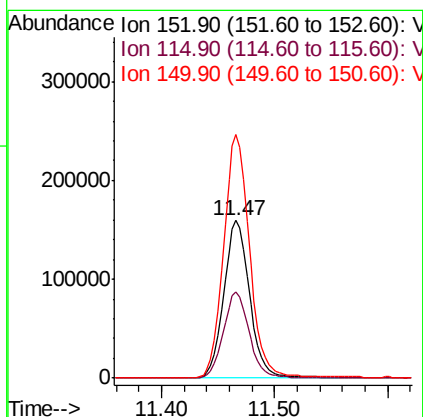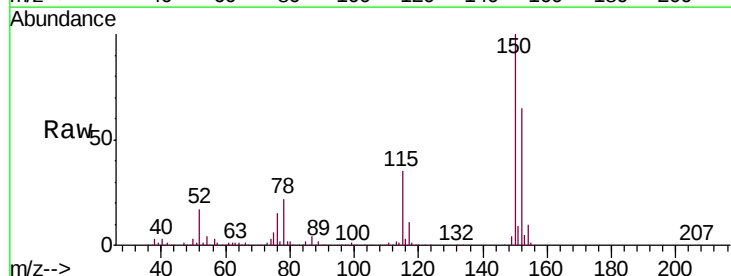



#74

N-ethyl acetate

Concen: 0.426 ug/l

RT: 9.92 min Scan# 2747

Delta R.T. -0.07 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :

T1-S-B2-(0)

Tgt Ion: 43 Resp: 2614


Ion Ratio Lower Upper

43 100

70 0.0 37.4 56.0#

55 0.0 21.0 31.4#

61 0.0 20.9 31.3#



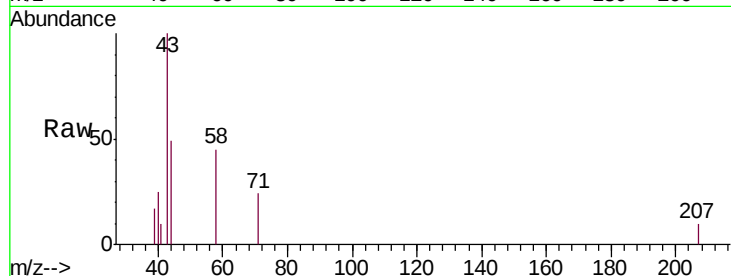


Abundance Ion 43.00 (42.70 to 43.70): VU033975.D (-2757) (-)

Ion 70.00 (69.70 to 70.70): VU033975.D (-2757) (-)

Ion 55.00 (54.70 to 55.70): VU033975.D (-2757) (-)

Ion 61.00 (60.70 to 61.70): VU033975.D (-2757) (-)

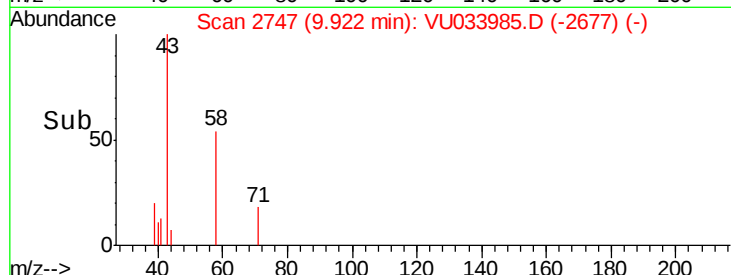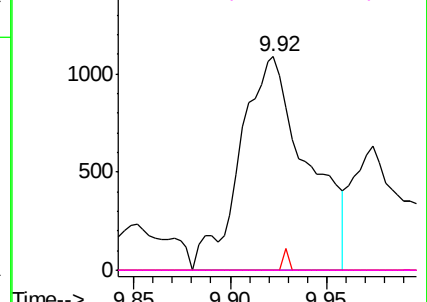

#76

1,2,3-Trichloropropane

Concen: 21.668 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.19 min

Lab File: VU033985.D


Acq: 27 Aug 2019 20:17

Tgt Ion: 75 Resp: 109771

Ion Ratio Lower Upper



75 100


77 1.3 21.0 63.0#



Abundance Ion 74.90 (74.60 to 75.60): VU033975.D (-2910) (-)

Ion 77.00 (76.70 to 77.70): VU033975.D (-2910) (-)

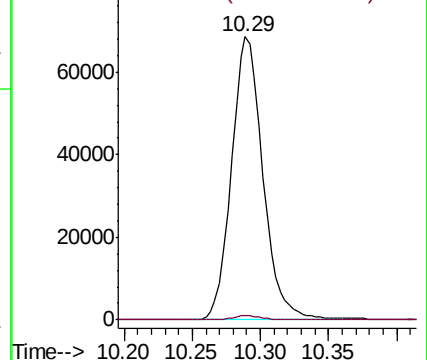



#81

trans-1,4-Dichloro-2-butene

Concen: 62.061 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.20 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17

Instrument :

MSVOA_U

ClientSampleId :

T1-S-B2-(0)


Tgt Ion: 75 Resp: 109771

Ion Ratio Lower Upper

75 100

53 0.1 0.0 0.0#




89 0.0 0.0 0.0

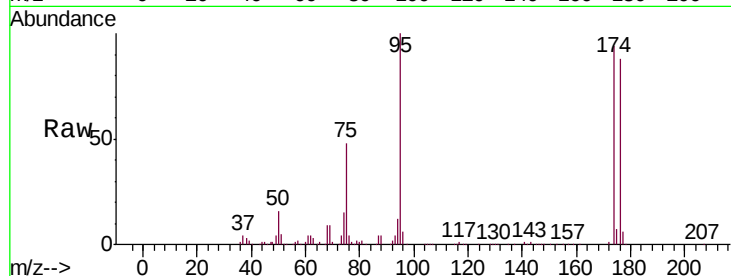

Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 53.00 (52.70 to 53.70): VU0

Ion 88.90 (88.60 to 89.60): VU0

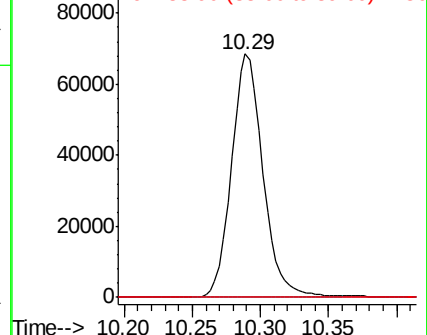

#93

1,2,4-Trichlorobenzene

Concen: 1.788 ug/l

RT: 13.55 min Scan# 3875

Delta R.T. 0.06 min

Lab File: VU033985.D

Acq: 27 Aug 2019 20:17


Tgt Ion: 180 Resp: 277

Ion Ratio Lower Upper

180 100

182 36.1 47.4 142.2#



145 0.0 14.4 43.2#




Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

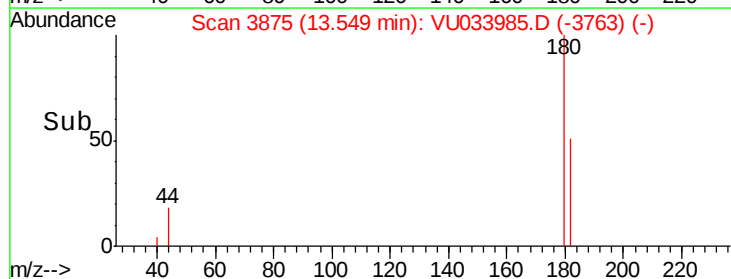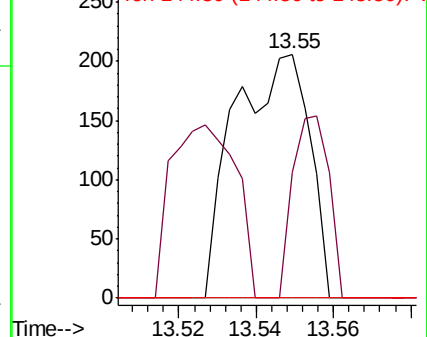



#95
 Naphthalene
 Concen: 2.101 ug/l
 RT: 13.76 min Scan# 3941
 Delta R.T. 0.04 min
 Lab File: VU033985.D
 Acq: 27 Aug 2019 20:17

Instrument :
 MSVOA_U
 ClientSampleId :
 T1-S-B2-(0)

Tgt Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.2	15.4#
129	0.0	8.5	12.7#

