



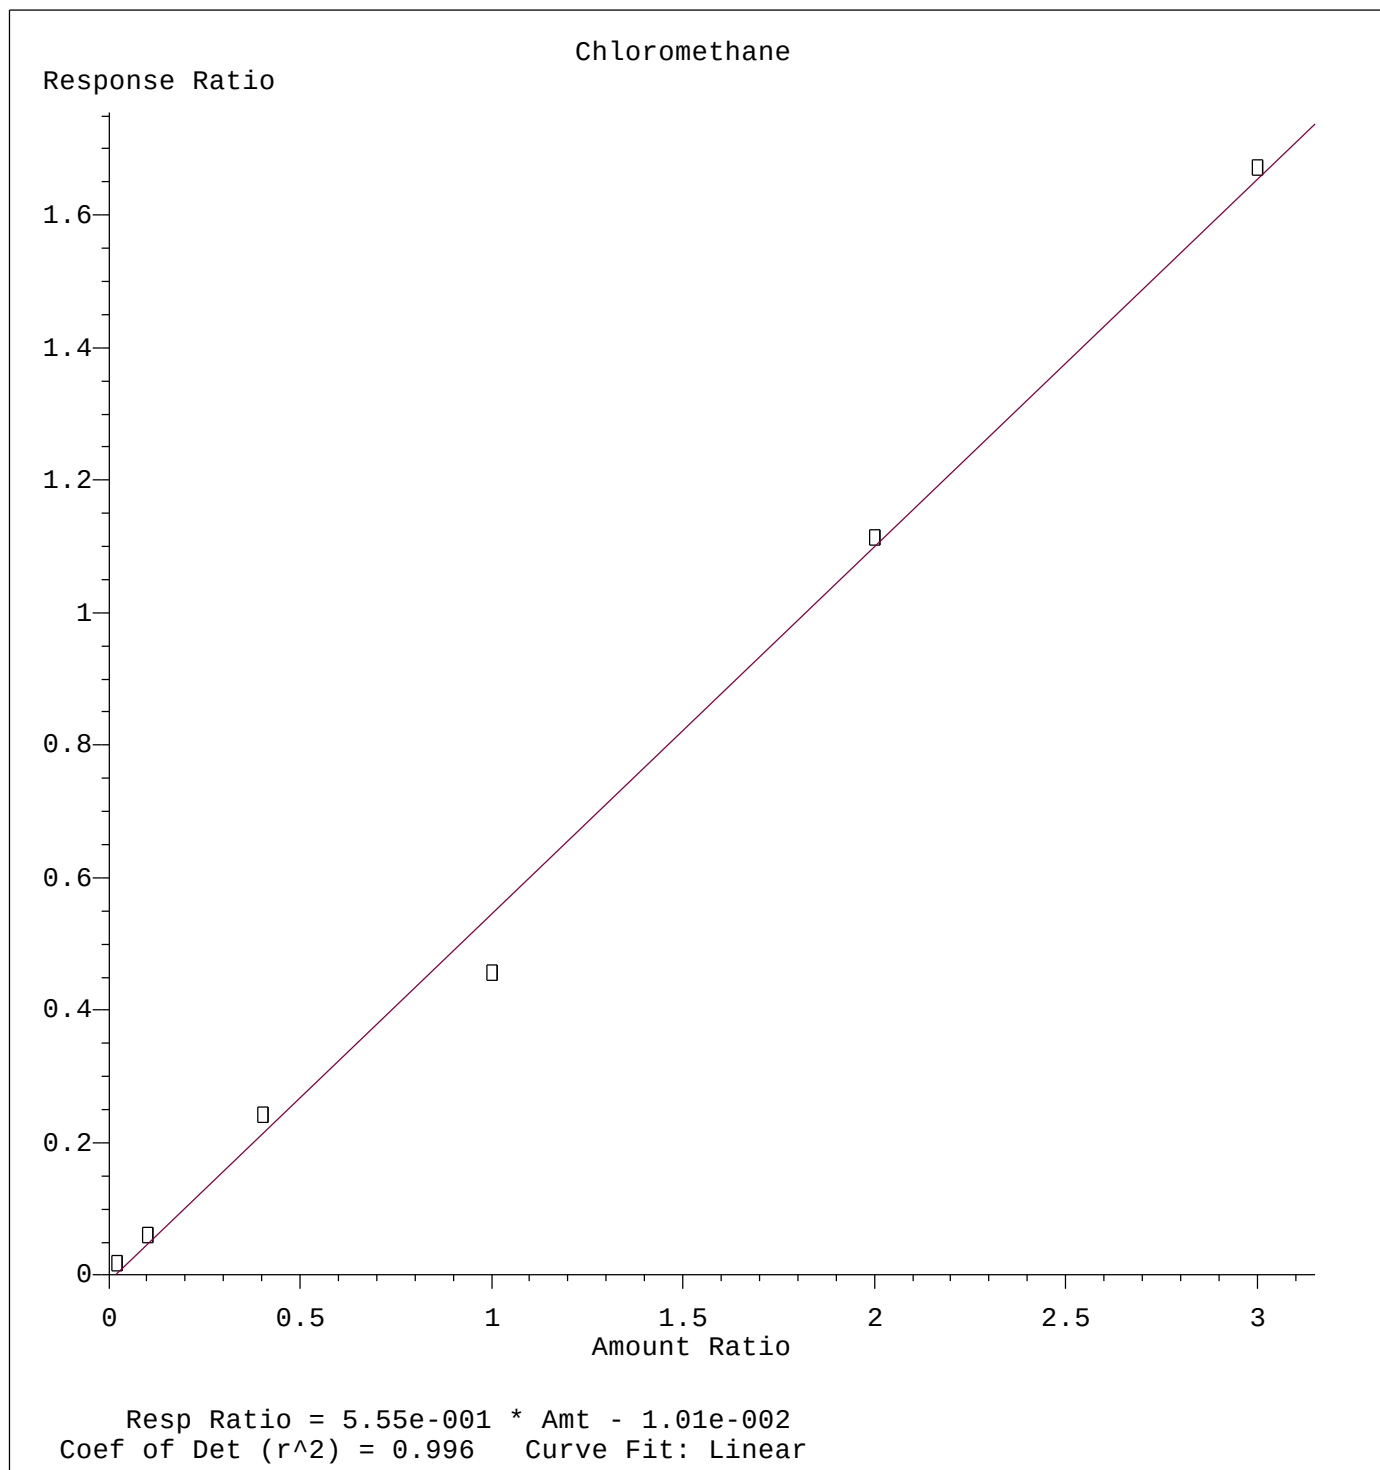

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Calibration Table Last Updated: Wed Aug 28 02:42:03 2019

Ethyl methacrylate

Response Ratio

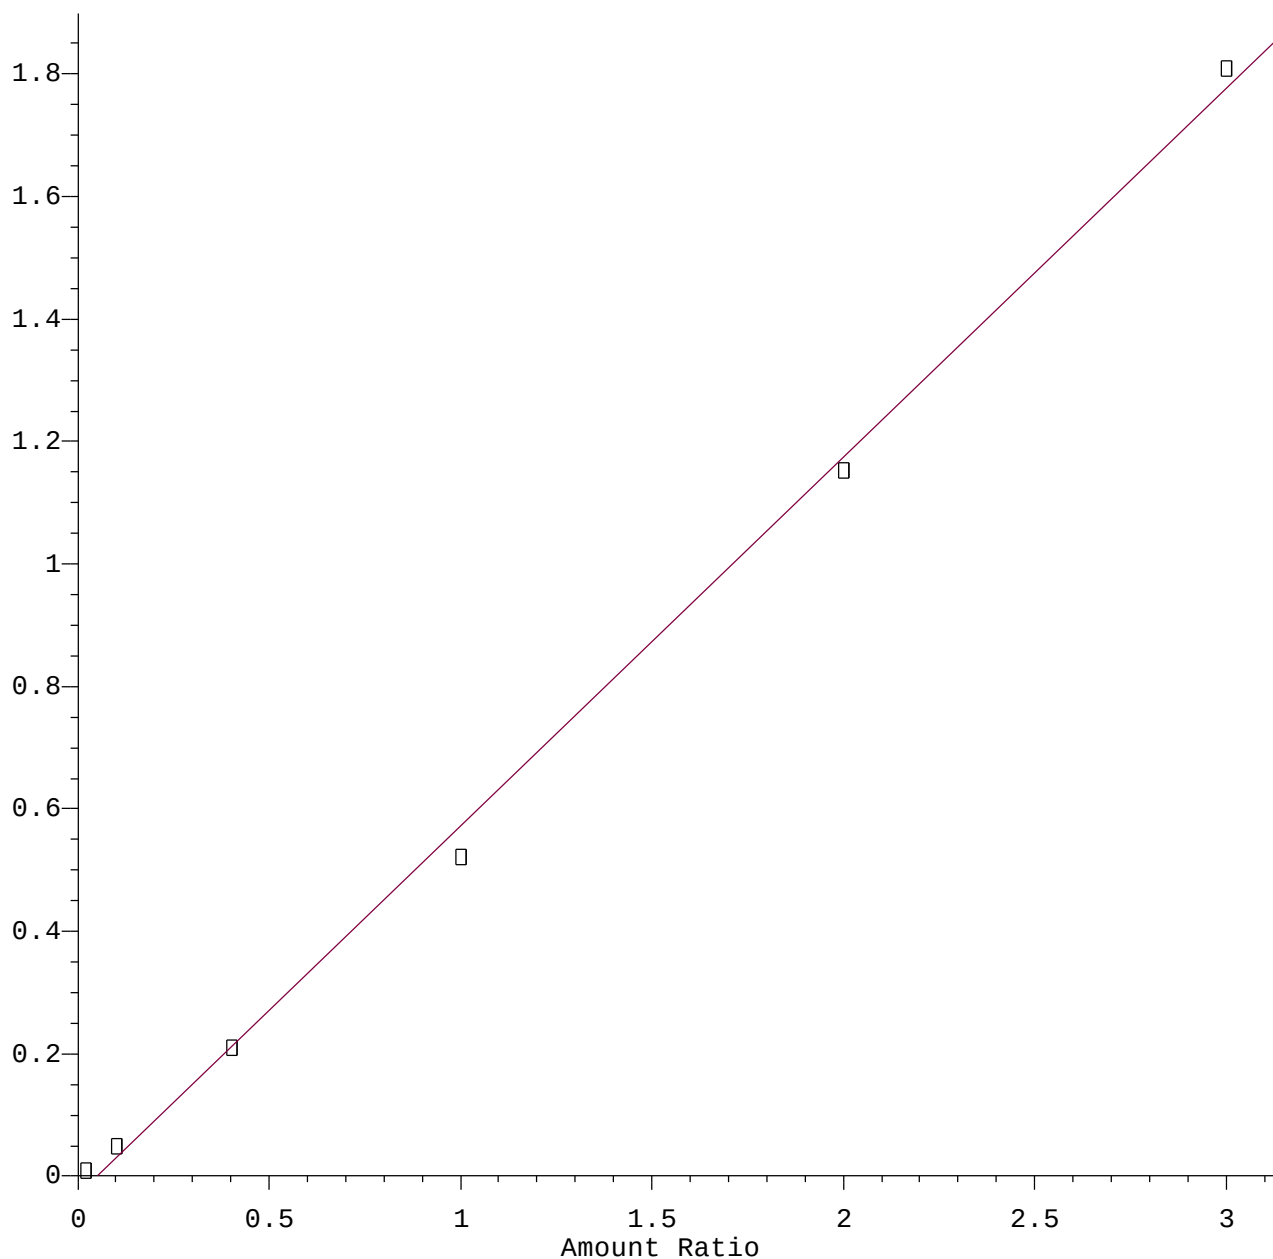


Resp Ratio = $6.02 \times 10^{-1} \times \text{Amt} - 3.03 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Calibration Table Last Updated: Wed Aug 28 02:42:03 2019

2-Chloroethyl Vinyl ether

Response Ratio

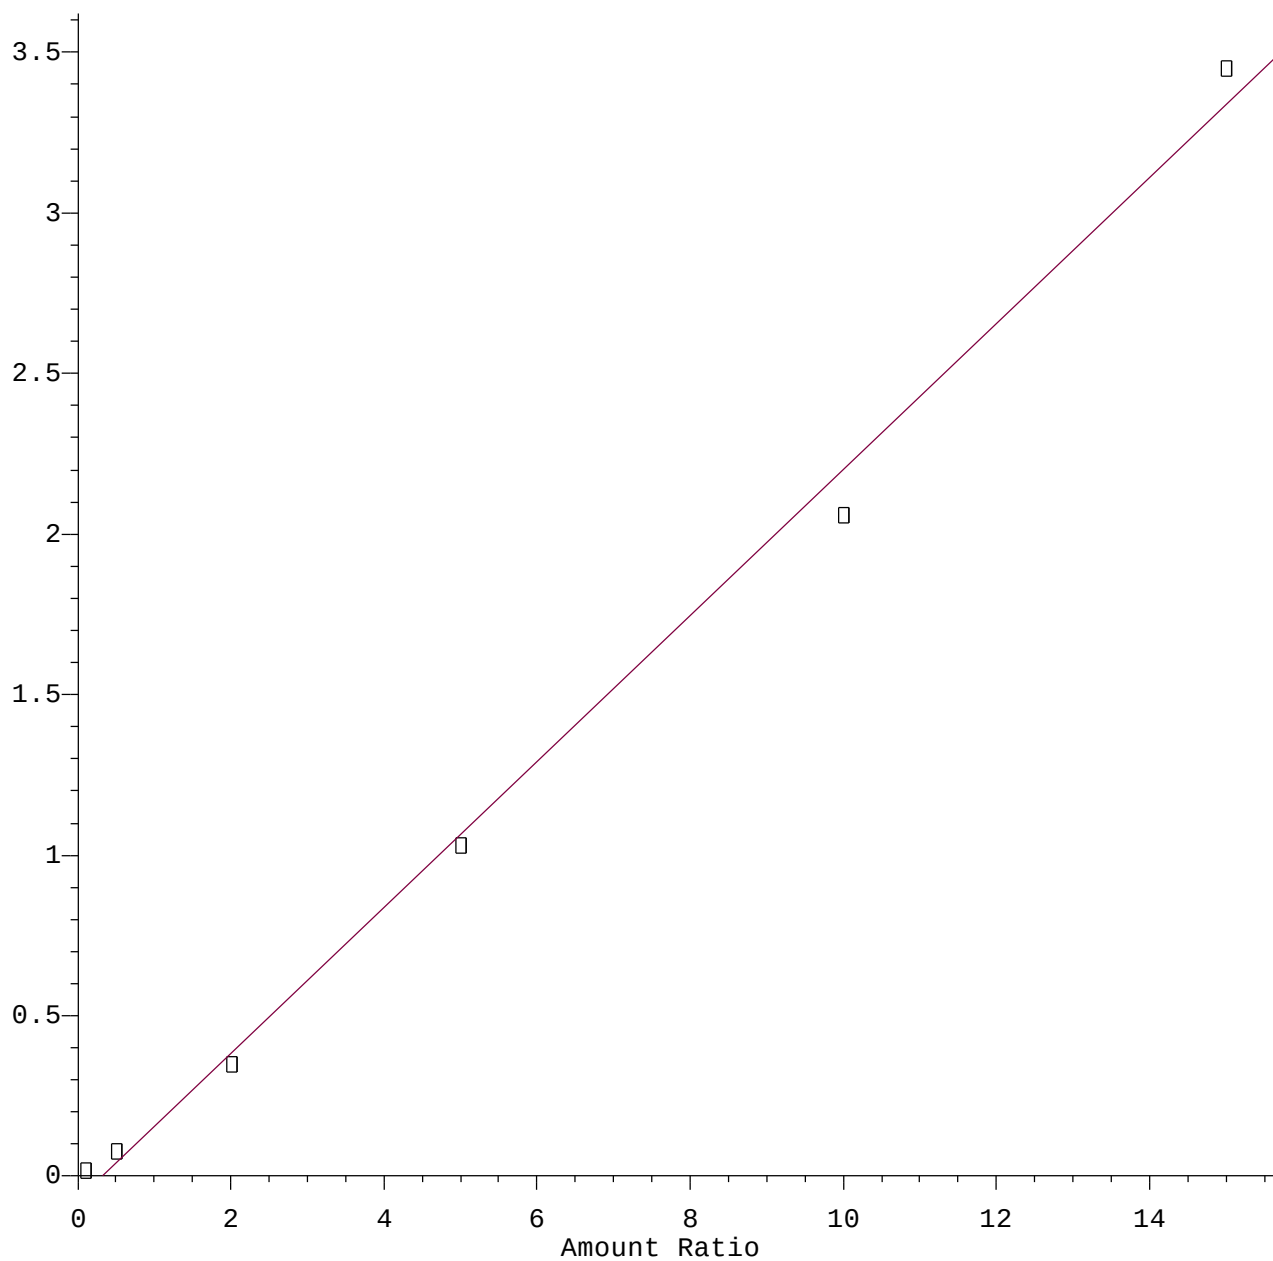


Resp Ratio = $2.27 \times 10^{-1} \times \text{Amt} - 7.37 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Calibration Table Last Updated: Wed Aug 28 02:42:03 2019

1,2,4-Trichlorobenzene

Response Ratio

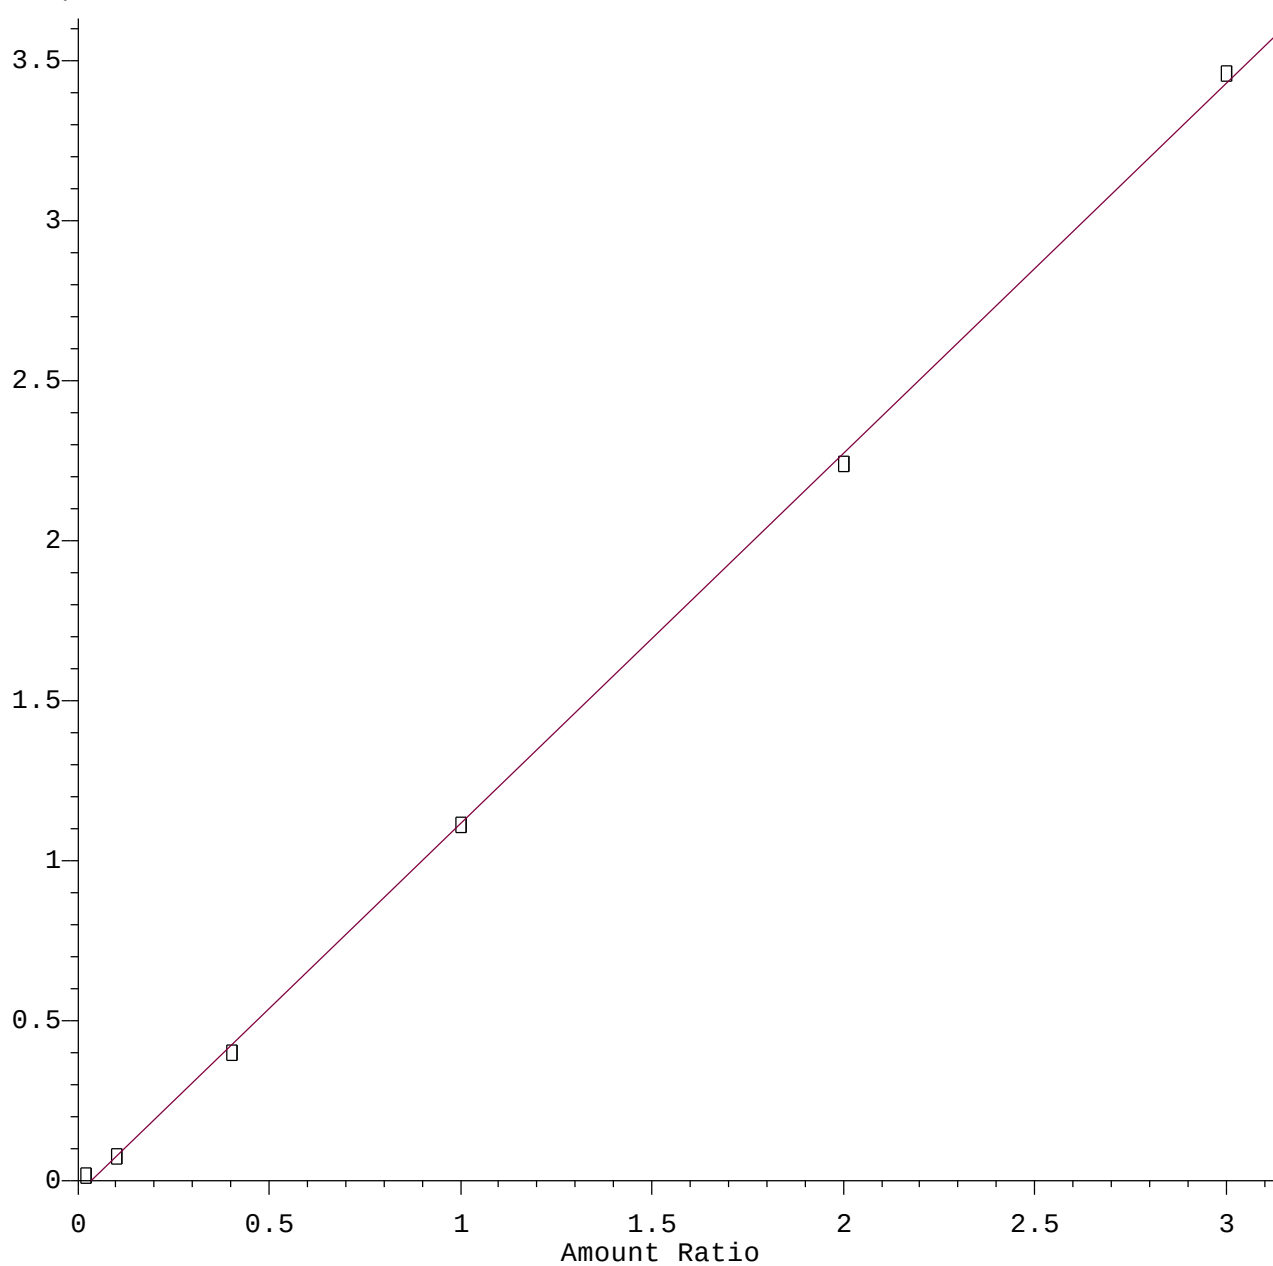


Resp Ratio = 1.16e+000 * Amt - 4.03e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Calibration Table Last Updated: Wed Aug 28 02:42:03 2019

Naphthalene

Response Ratio

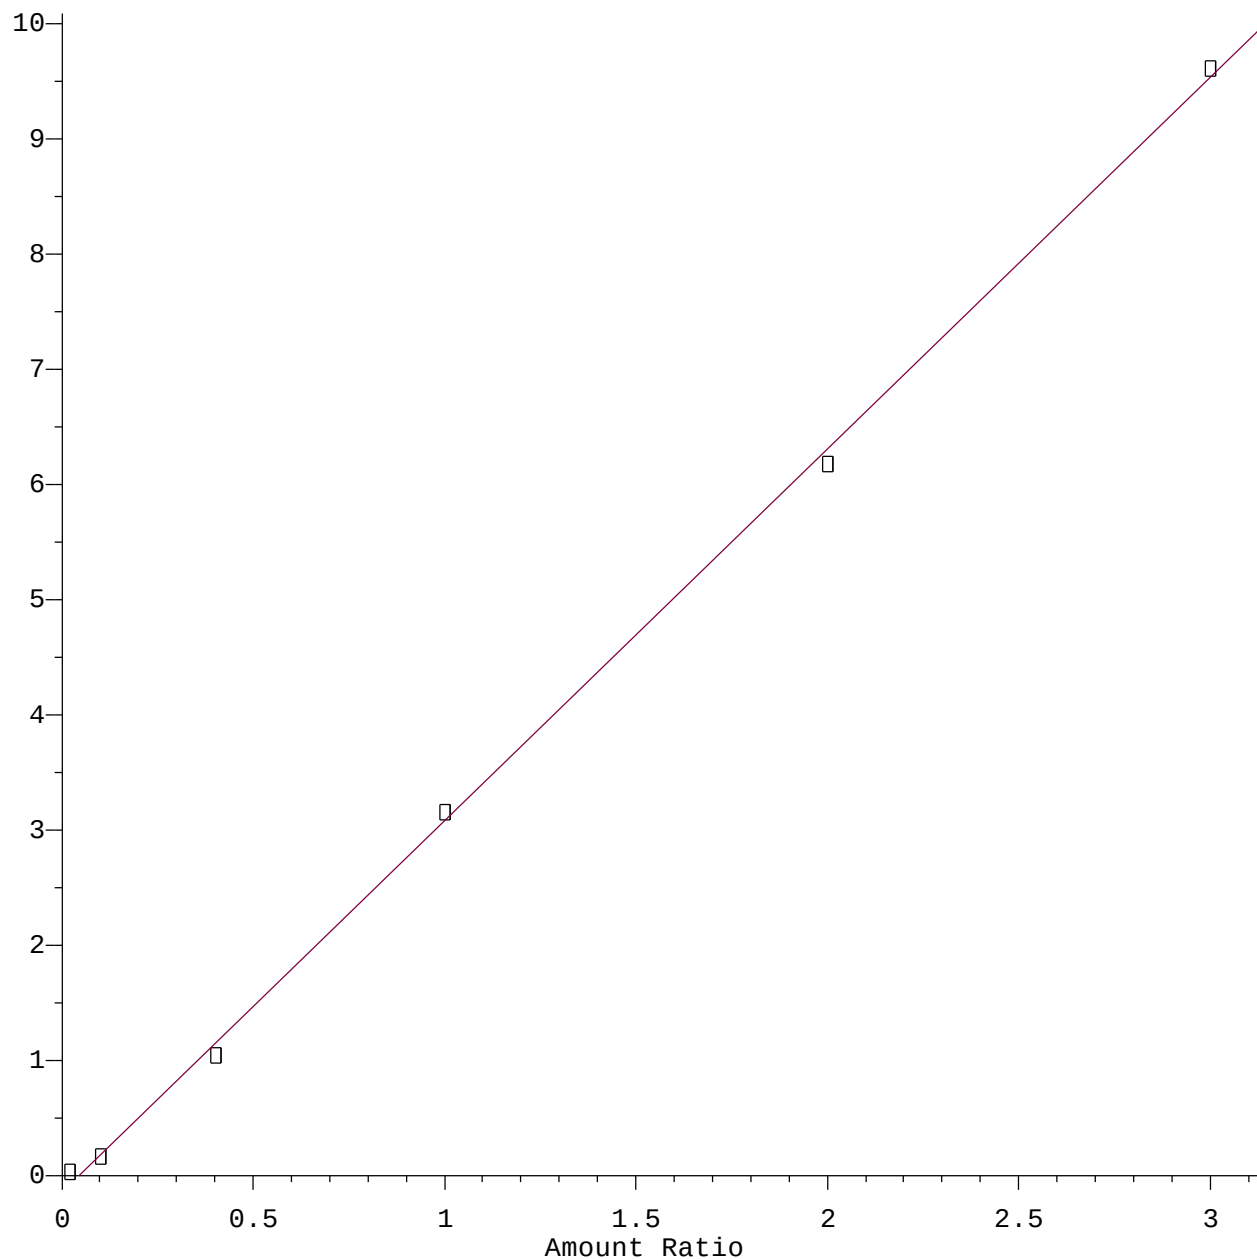

Resp Ratio = 3.22×10^0 * Amt - 1.34×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Calibration Table Last Updated: Wed Aug 28 02:42:03 2019