


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082819\
Data File : VU033971.D
Acq On : 27 Aug 2019 13:48
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
Title : SW846 8260
Last Update : Wed Aug 28 02:42:03 2019

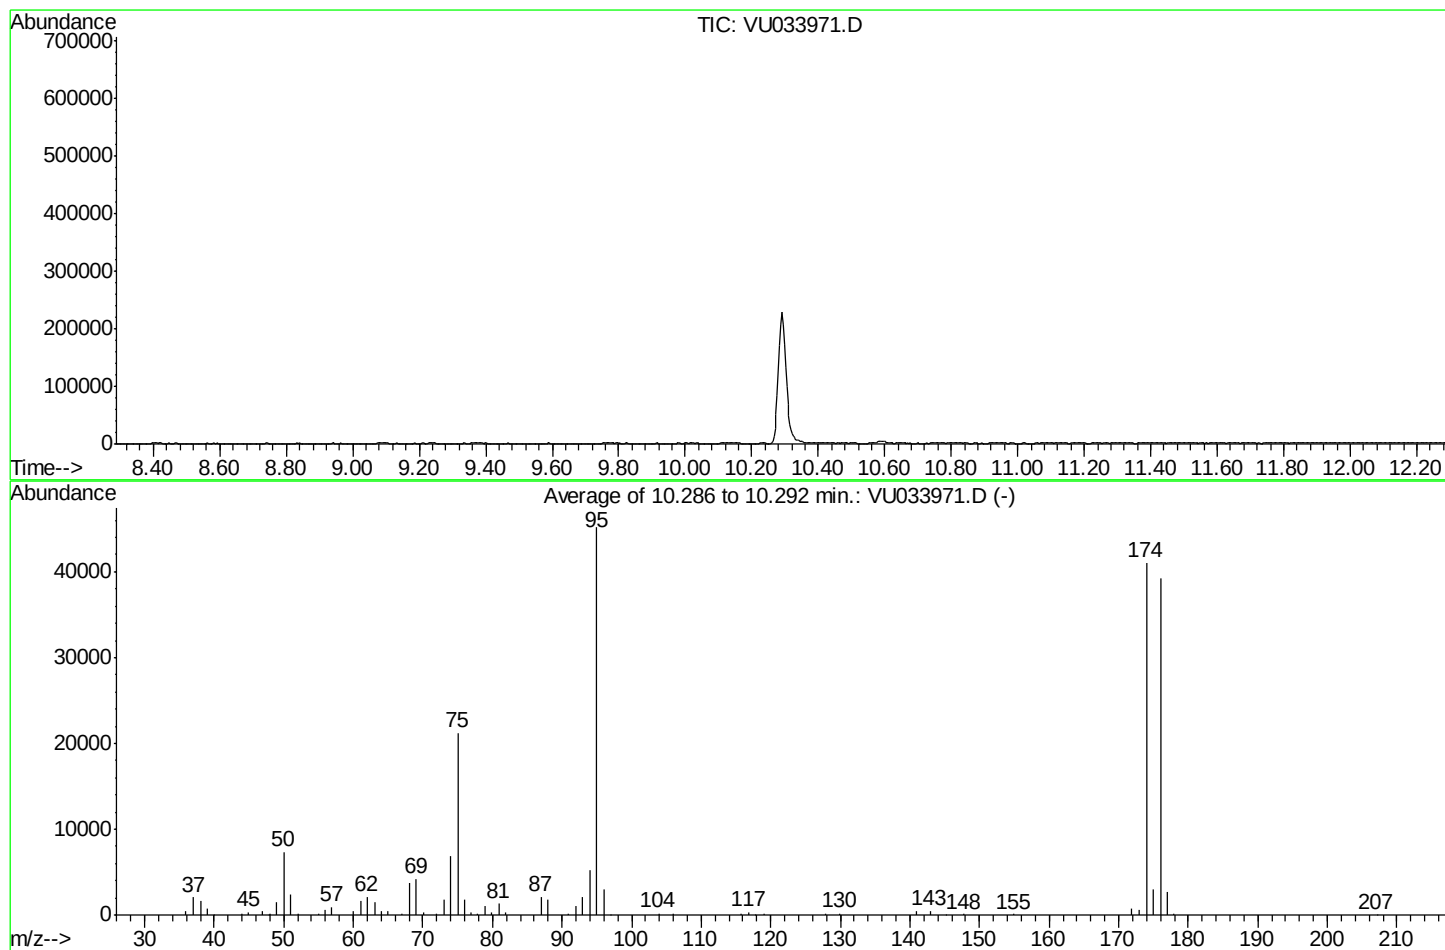

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7336	PASS
75	95	30	60	46.9	21210	PASS
95	95	100	100	100.0	45178	PASS
96	95	5	9	6.6	2980	PASS
173	174	0.00	2	1.3	549	PASS
174	95	50	100	90.8	41034	PASS
175	174	5	9	7.4	3053	PASS
176	174	95	101	95.6	39245	PASS
177	176	5	9	6.8	2672	PASS