


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082819\
 Data File : VU033995.D
 Acq On : 28 Aug 2019 00:16
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082819W.M
 Title : SW846 8260
 Last Update : Wed Aug 28 02:42:03 2019

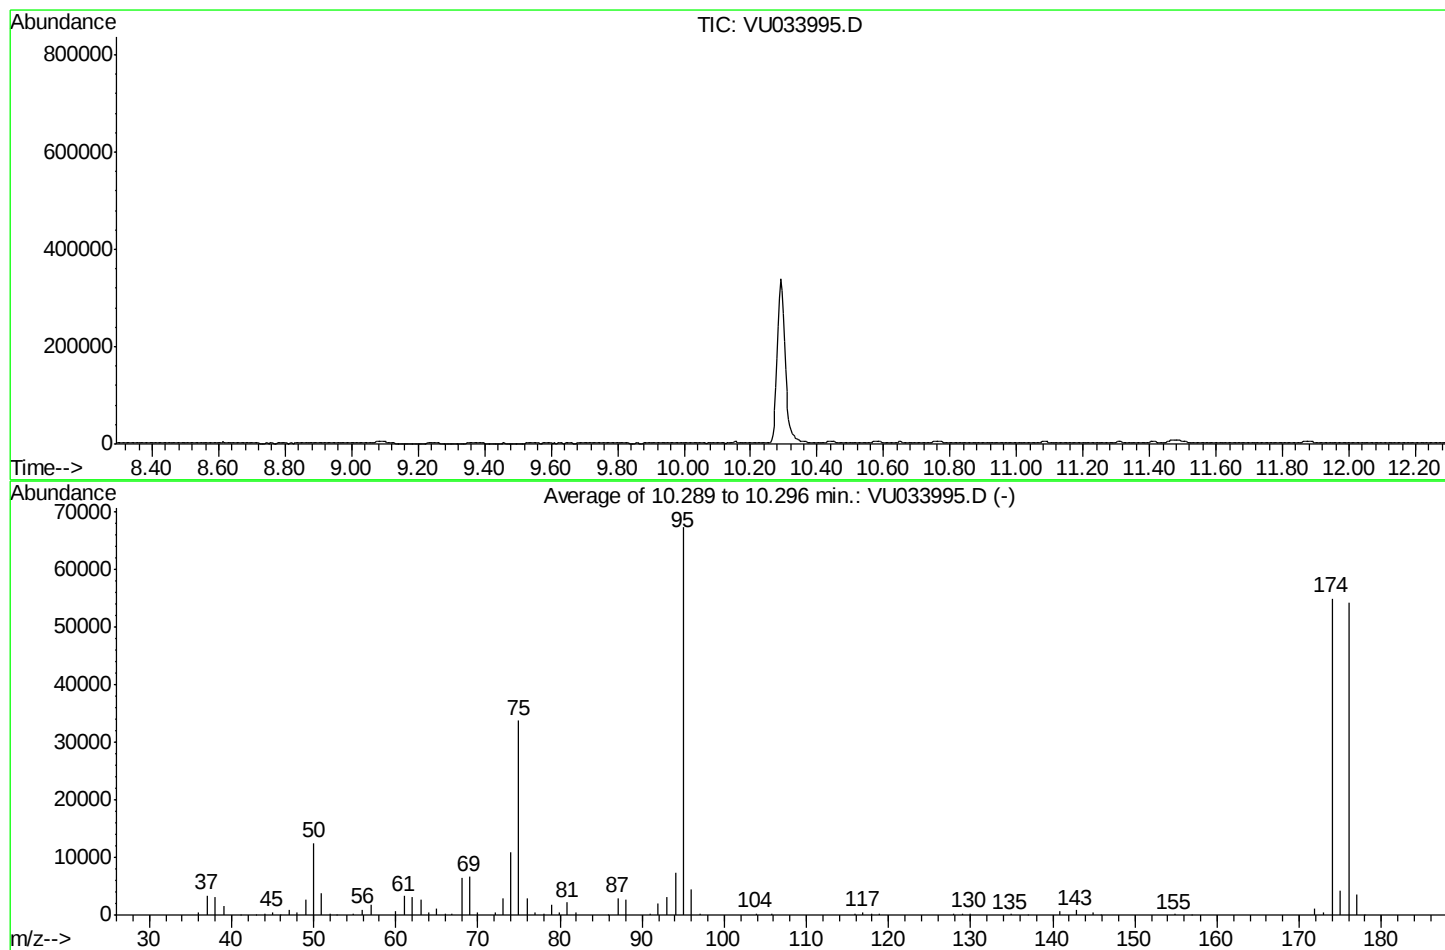

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	12559	PASS
75	95	30	60	50.2	33757	PASS
95	95	100	100	100.0	67301	PASS
96	95	5	9	6.8	4546	PASS
173	174	0.00	2	0.8	448	PASS
174	95	50	100	81.6	54896	PASS
175	174	5	9	7.8	4305	PASS
176	174	95	101	98.8	54245	PASS
177	176	5	9	6.7	3621	PASS