

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
 Data File : VU054921.D
 Acq On : 28 Aug 2023 14:06
 Operator : MD/SY
 Sample : VU0828WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK018

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	106	rVB	42601	49286	6.31%	0.890%
2	1.911	185	193	207	rVB	56779	75274	9.64%	1.360%
3	2.563	384	396	414	rVB	85991	141579	18.13%	2.558%
4	3.043	534	545	561	rBV3	11354	22120	2.83%	0.400%
5	4.628	1028	1038	1074	rBV	107725	308204	39.47%	5.568%
6	5.062	1155	1173	1199	rBV	113738	260645	33.38%	4.709%
7	5.724	1359	1379	1404	rBV2	215071	586481	75.11%	10.595%
8	6.248	1529	1542	1559	rBV	227376	443257	56.77%	8.008%
9	6.538	1620	1632	1641	rBV8	5042	10508	1.35%	0.190%
10	6.689	1666	1679	1699	rBV	148486	296827	38.02%	5.362%
11	7.563	1940	1951	1968	rBV2	62709	118939	15.23%	2.149%
12	7.898	2041	2055	2086	rBV	266842	488455	62.56%	8.824%
13	8.181	2132	2143	2161	rBV2	39788	72320	9.26%	1.307%
14	8.634	2270	2284	2319	rBV2	341461	780782	100.00%	14.105%
15	9.415	2514	2527	2555	rBV	329214	573066	73.40%	10.353%
16	10.756	2930	2944	2962	rBV	130354	211614	27.10%	3.823%
17	11.811	3260	3272	3300	rVV	349810	579222	74.18%	10.464%
18	12.193	3379	3391	3413	rBV	285808	482187	61.76%	8.711%
19	13.843	3898	3904	3918	rVB7	6706	11481	1.47%	0.207%
20	14.100	3973	3984	3992	rBV4	7334	13032	1.67%	0.235%
21	14.338	4048	4058	4069	rVB5	6214	10088	1.29%	0.182%




Sum of corrected areas: 5535367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054921.D
Acq On : 28 Aug 2023 14:06
Operator : MD/SY
Sample : VU0828WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

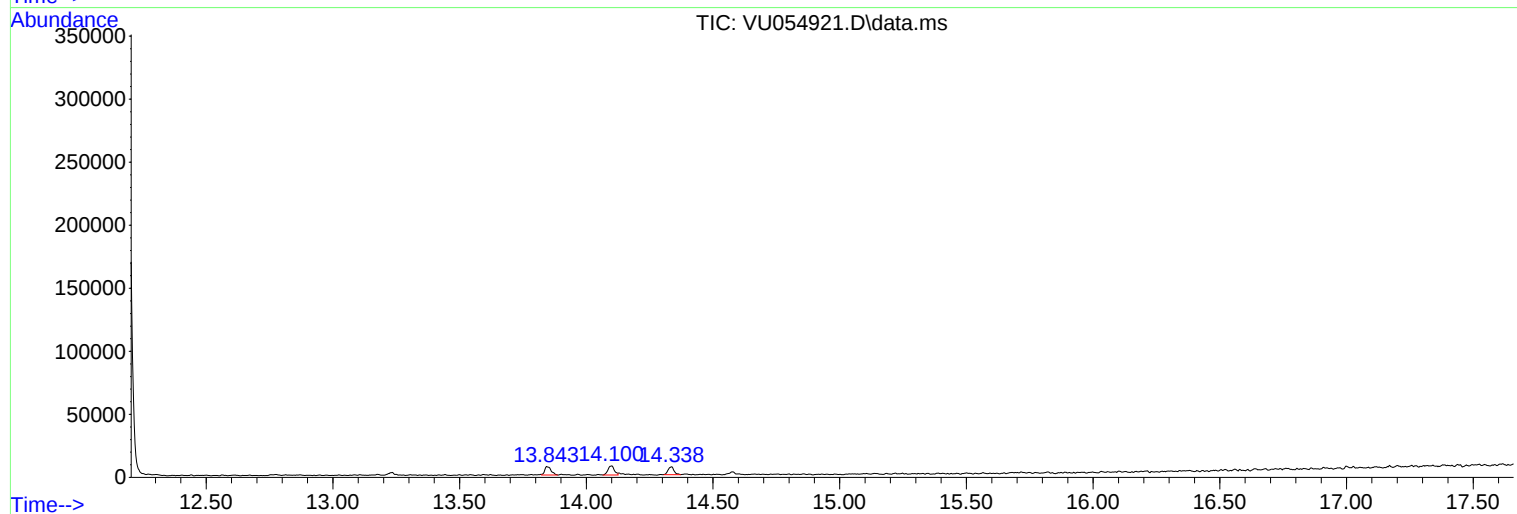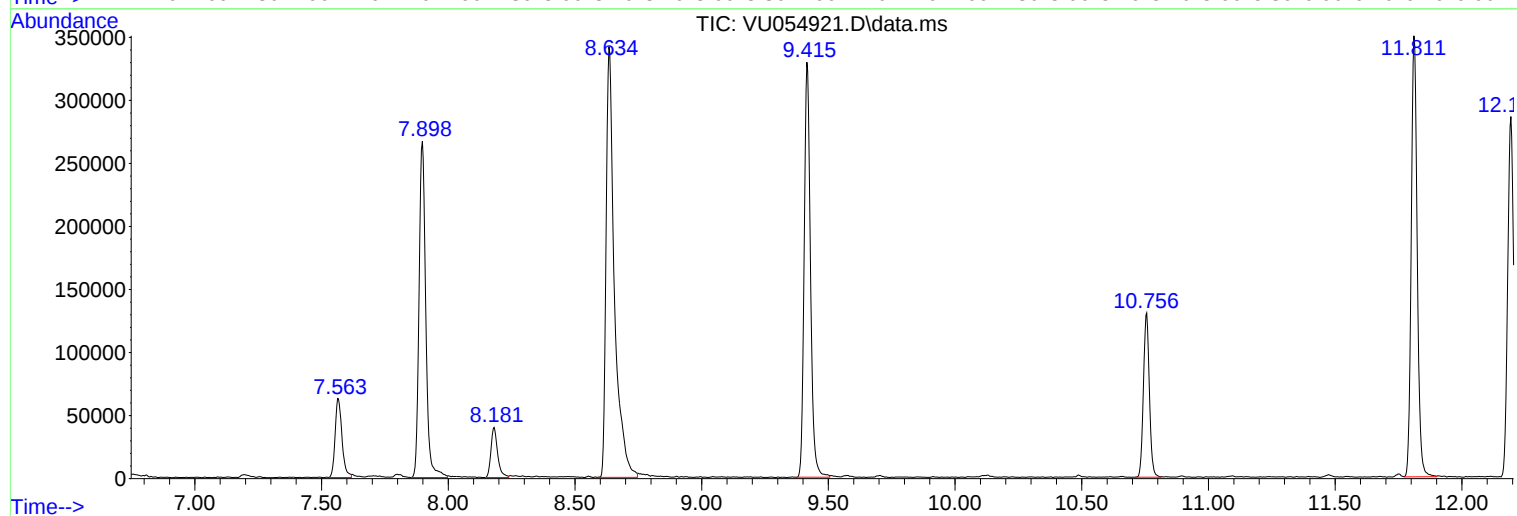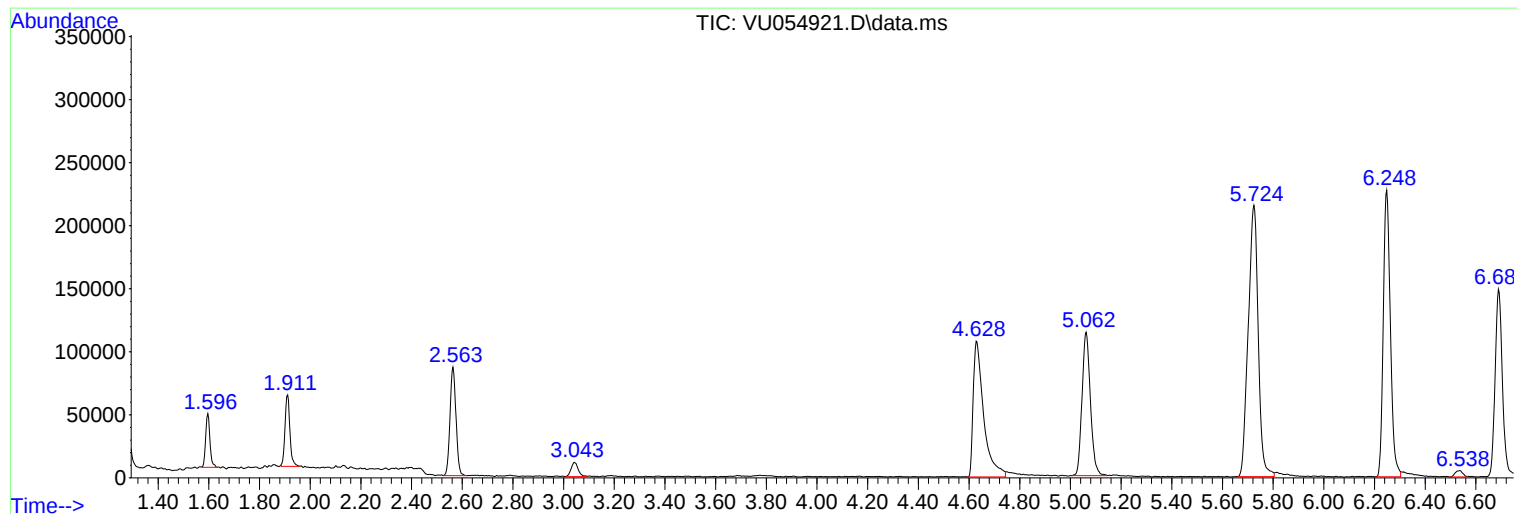

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054921.D
Acq On : 28 Aug 2023 14:06
Operator : MD/SY
Sample : VU0828WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054921.D
Acq On : 28 Aug 2023 14:06
Operator : MD/SY
Sample : VU0828WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc