

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
 Data File : VU054927.D
 Acq On : 28 Aug 2023 16:34
 Operator : MD/SY
 Sample : 04173-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	86	96	111	rBV2	294045	357240	16.75%	4.400%
2	1.910	186	193	206	rVB	55941	82787	3.88%	1.020%
3	2.563	385	396	409	rBV	84015	134344	6.30%	1.655%
4	2.798	450	469	518	rBV2	55763	271098	12.71%	3.339%
5	3.351	630	641	657	rBV3	19520	40528	1.90%	0.499%
6	4.663	1026	1049	1085	rBV2	790043	2132412	100.00%	26.262%
7	5.061	1157	1173	1189	rBV2	114777	252673	11.85%	3.112%
8	5.724	1359	1379	1409	rBV2	210347	584959	27.43%	7.204%
9	6.248	1529	1542	1563	rBV	236949	461856	21.66%	5.688%
10	6.541	1622	1633	1649	rVB5	13810	27333	1.28%	0.337%
11	6.688	1666	1679	1696	rBV	149134	293091	13.74%	3.610%
12	7.566	1939	1952	1978	rBV2	63065	118640	5.56%	1.461%
13	7.897	2042	2055	2073	rBV	263136	474515	22.25%	5.844%
14	8.180	2131	2143	2163	rBV2	38808	71955	3.37%	0.886%
15	8.637	2273	2285	2322	rBV2	365995	807809	37.88%	9.949%
16	9.415	2513	2527	2551	rBV	348399	663794	31.13%	8.175%
17	10.756	2931	2944	2960	rBV	127039	215123	10.09%	2.649%
18	11.810	3260	3272	3291	rBV	368904	634310	29.75%	7.812%
19	12.193	3378	3391	3409	rBV	297308	495383	23.23%	6.101%




Sum of corrected areas: 8119850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054927.D
Acq On : 28 Aug 2023 16:34
Operator : MD/SY
Sample : 04173-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

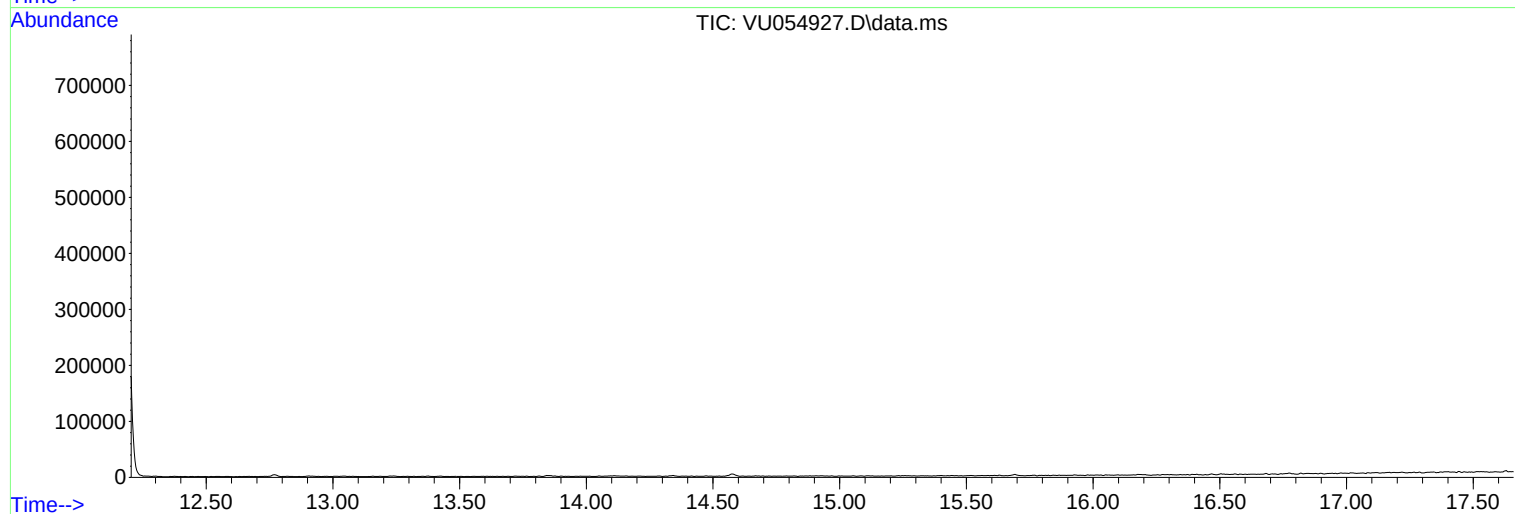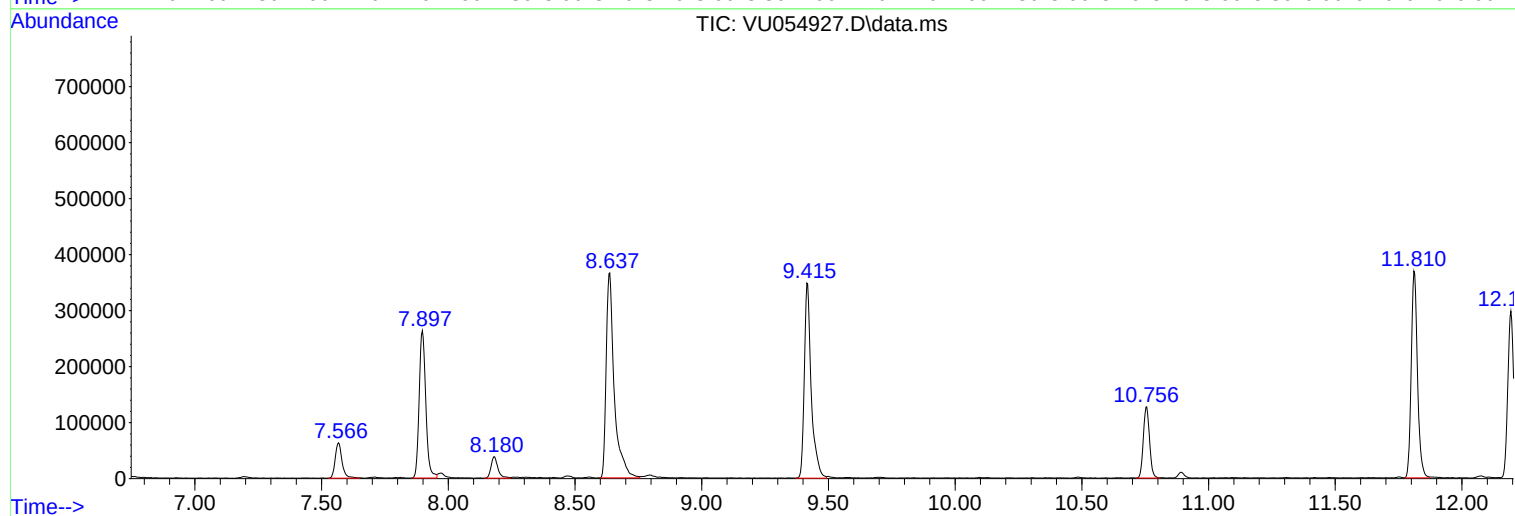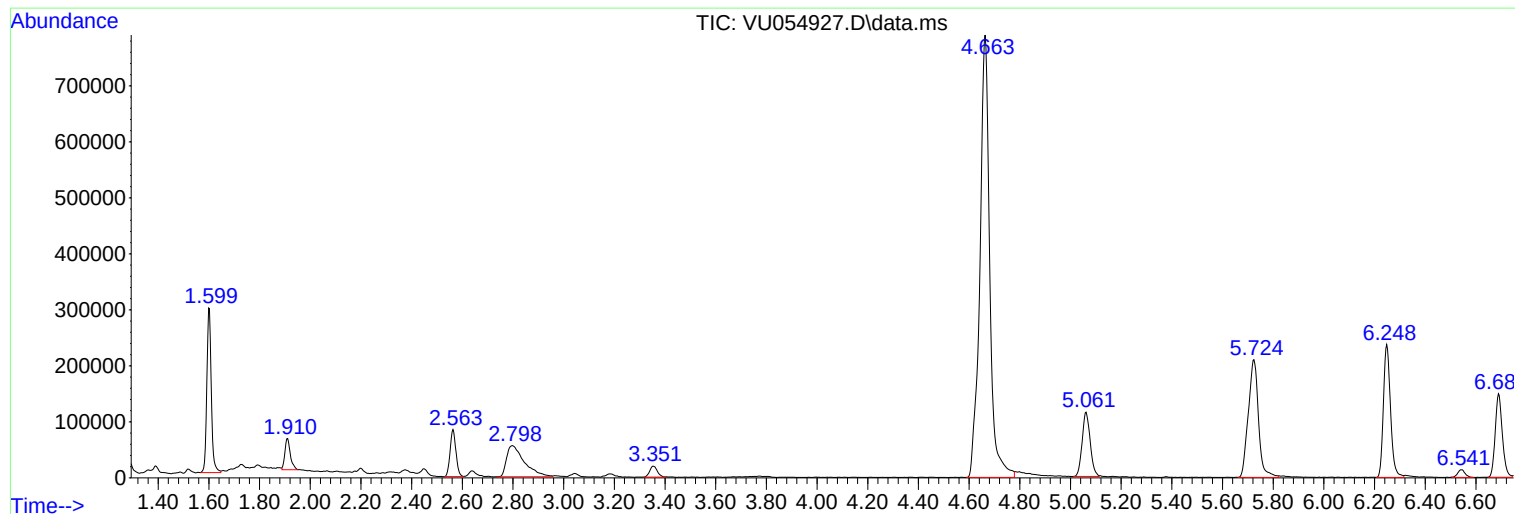

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054927.D
Acq On : 28 Aug 2023 16:34
Operator : MD/SY
Sample : 04173-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.798	2.93 ug/L	271098	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56

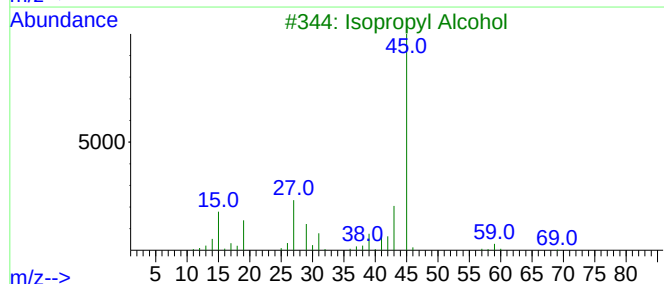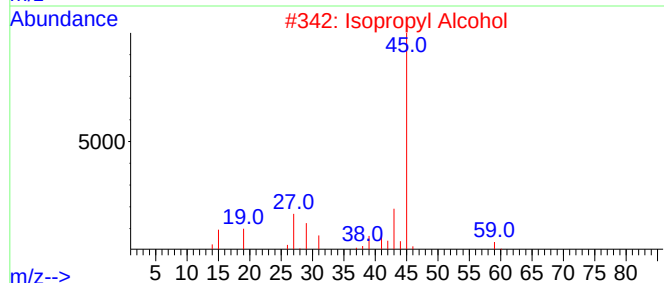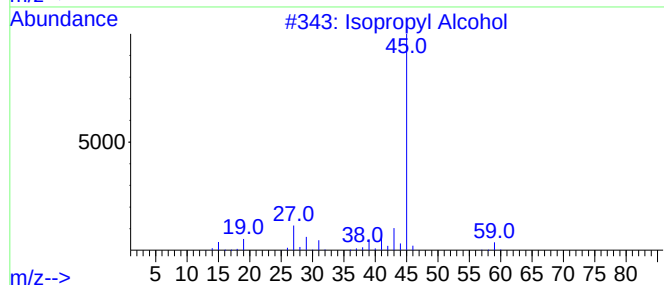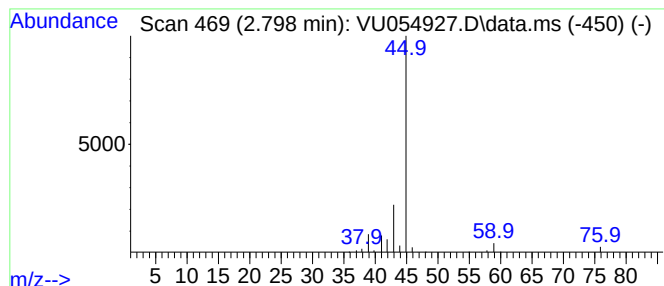

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054927.D
Acq On : 28 Aug 2023 16:34
Operator : MD/SY
Sample : 04173-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.798	2.9	ug/L	271098	1	6.248	461856	5.0