

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
 Data File : VU054931.D
 Acq On : 28 Aug 2023 18:13
 Operator : MD/SY
 Sample : 04173-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rVB2	79445	93951	3.34%	0.967%
2	1.911	185	193	203	rVB	51239	64675	2.30%	0.666%
3	2.563	384	396	410	rBV2	83170	147746	5.25%	1.521%
4	2.795	453	468	507	rBV2	46978	237502	8.44%	2.445%
5	3.351	631	641	655	rBV4	17093	34752	1.23%	0.358%
6	4.663	1025	1049	1091	rBV2	1094090	2815084	100.00%	28.975%
7	5.062	1158	1173	1198	rVB	108253	241994	8.60%	2.491%
8	5.724	1358	1379	1400	rBV2	205583	544432	19.34%	5.604%
9	6.248	1528	1542	1561	rBV	232101	452035	16.06%	4.653%
10	6.541	1615	1633	1654	rBV	820133	1560258	55.42%	16.060%
11	6.689	1667	1679	1696	rVB	138573	271523	9.65%	2.795%
12	7.566	1940	1952	1976	rBV	55920	107368	3.81%	1.105%
13	7.898	2041	2055	2070	rBV	244988	434892	15.45%	4.476%
14	8.180	2132	2143	2157	rBV2	35357	61603	2.19%	0.634%
15	8.634	2272	2284	2322	rBV3	351668	776513	27.58%	7.993%
16	9.415	2513	2527	2555	rBV	335811	594398	21.11%	6.118%
17	10.753	2932	2943	2963	rBV	124116	203087	7.21%	2.090%
18	11.811	3259	3272	3292	rBV	356948	602224	21.39%	6.199%
19	12.193	3379	3391	3413	rBV	280696	471366	16.74%	4.852%




Sum of corrected areas: 9715403

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054931.D
Acq On : 28 Aug 2023 18:13
Operator : MD/SY
Sample : 04173-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

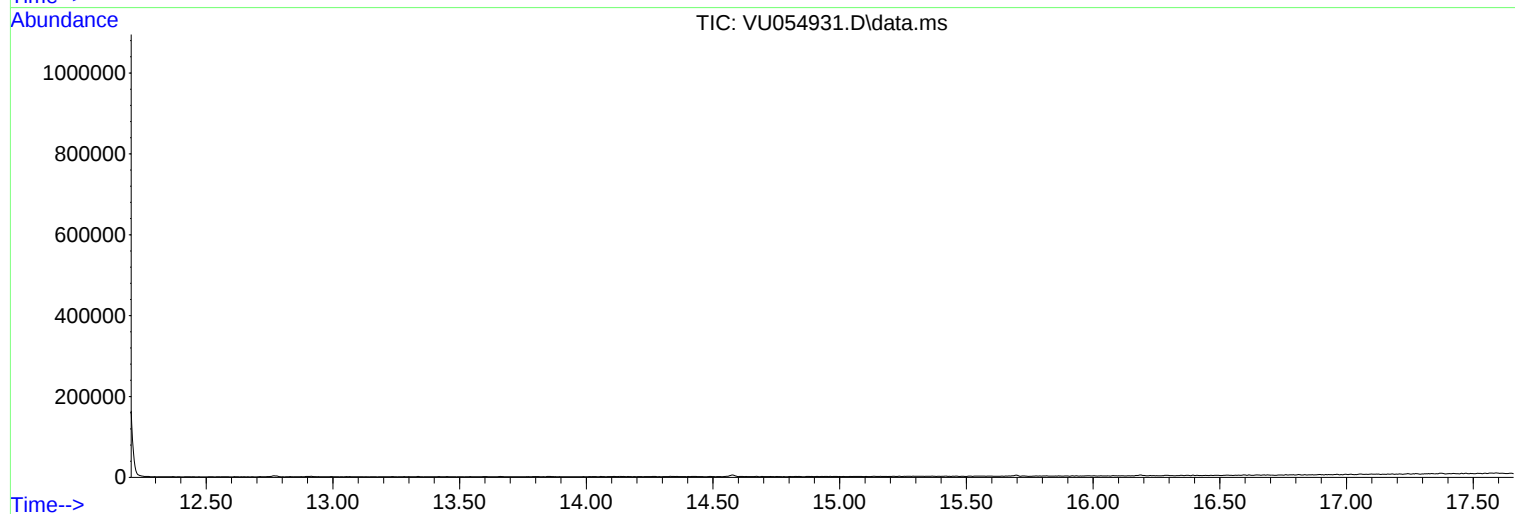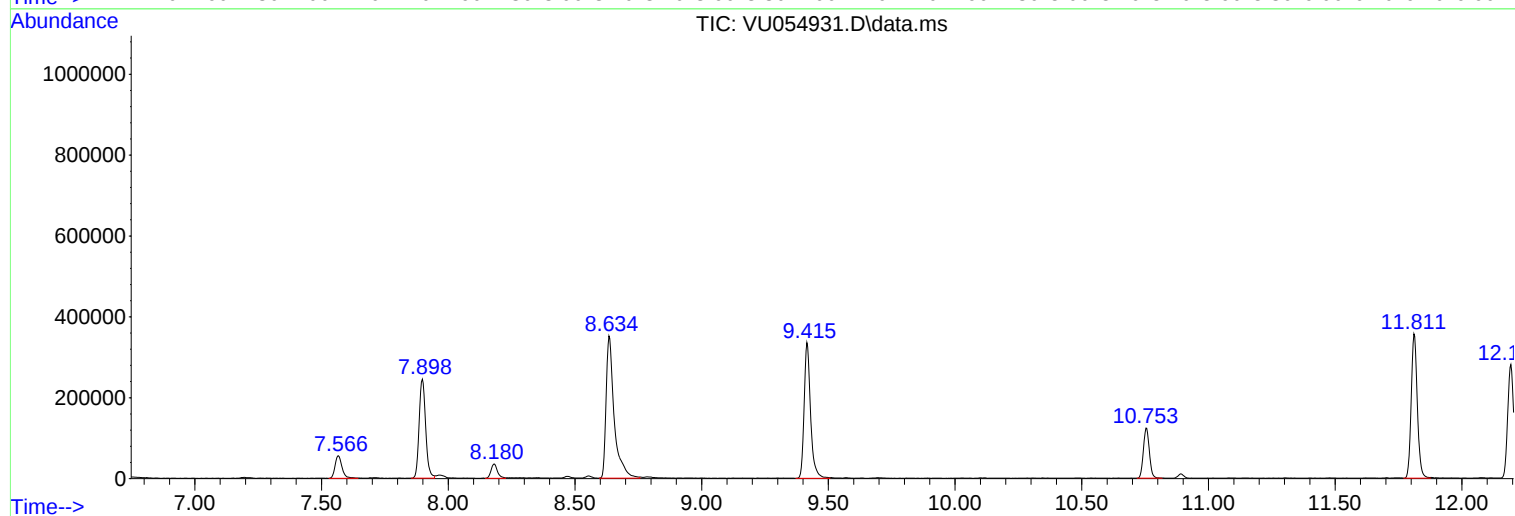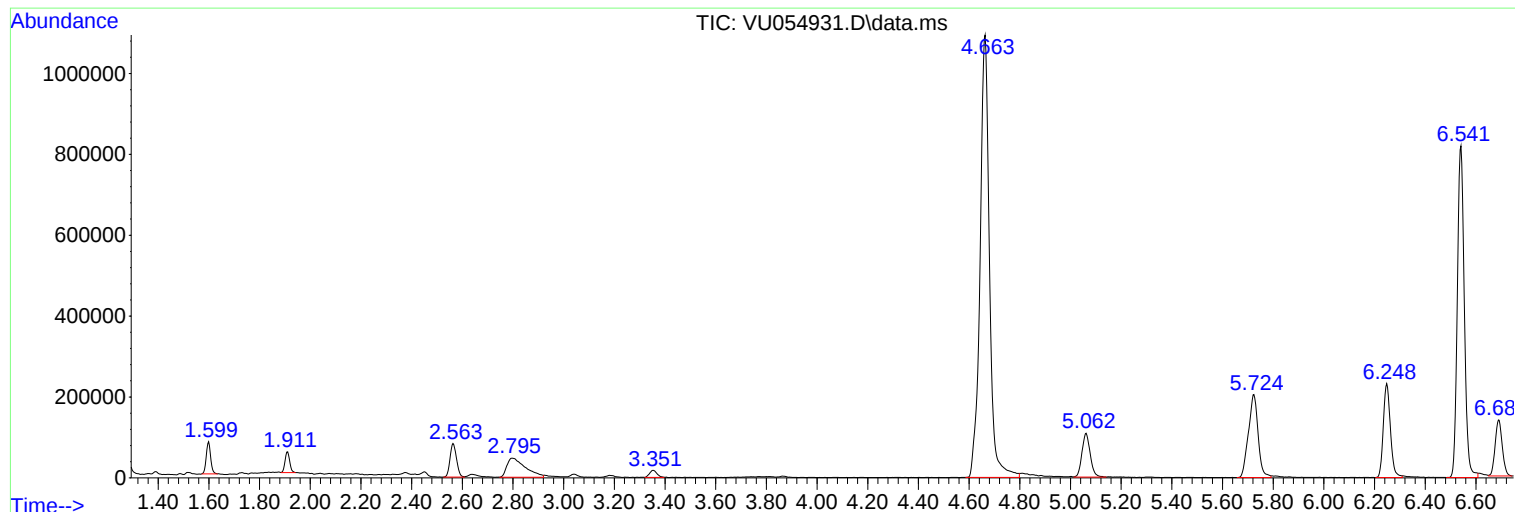

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054931.D
Acq On : 28 Aug 2023 18:13
Operator : MD/SY
Sample : 04173-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.795	2.63 ug/L	237502	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	56

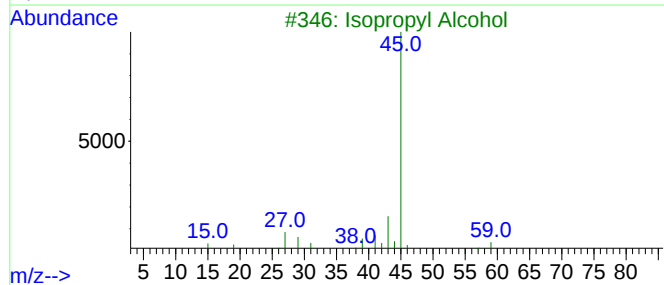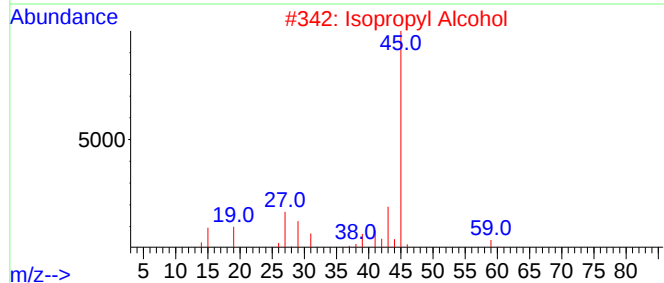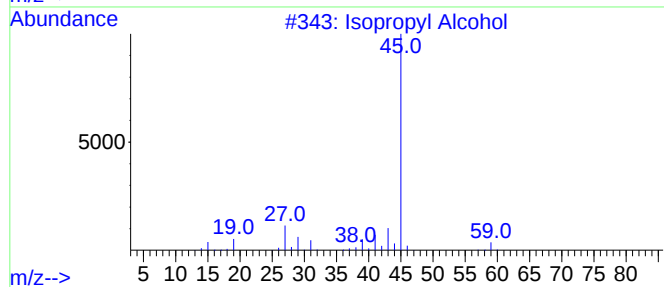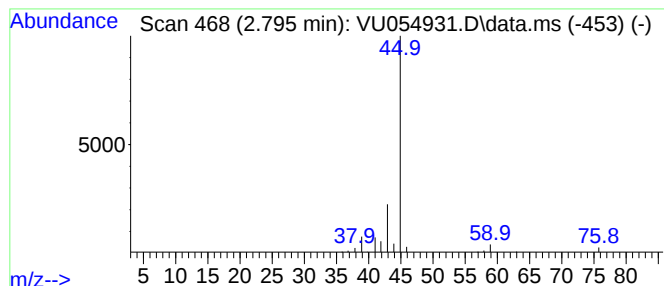

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082823\
Data File : VU054931.D
Acq On : 28 Aug 2023 18:13
Operator : MD/SY
Sample : 04173-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.795	2.6	ug/L	237502	1	6.248	452035	5.0