

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082824\
 Data File : VU060559.D
 Acq On : 28 Aug 2024 16:45
 Operator : MD/SY
 Sample : P3755-01DL 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0UE3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	108	rVB	42500	49657	7.77%	1.021%
2	1.908	183	192	209	rVB	43764	57818	9.05%	1.189%
3	2.567	383	397	417	rBV3	86421	167105	26.16%	3.437%
4	3.039	531	544	558	rBV2	10247	20081	3.14%	0.413%
5	4.660	1029	1048	1079	rBV3	220323	638784	100.00%	13.139%
6	5.055	1156	1171	1203	rBV	88143	200313	31.36%	4.120%
7	5.309	1236	1250	1268	rBV2	55219	123357	19.31%	2.537%
8	5.721	1353	1378	1412	rBV3	158615	437012	68.41%	8.989%
9	6.245	1528	1541	1565	rBV	183849	362448	56.74%	7.455%
10	6.538	1620	1632	1666	rBV	221191	425839	66.66%	8.759%
11	6.685	1666	1678	1698	rBV	108836	215241	33.70%	4.427%
12	7.563	1939	1951	1973	rBV	43058	80501	12.60%	1.656%
13	7.894	2043	2054	2075	rBV	170734	307314	48.11%	6.321%
14	8.177	2131	2142	2157	rBV2	25829	46459	7.27%	0.956%
15	8.631	2270	2283	2306	rBV2	229570	471902	73.88%	9.706%
16	9.412	2514	2526	2546	rBV	260945	464448	72.71%	9.553%
17	10.753	2931	2943	2959	rBV	97154	159280	24.93%	3.276%
18	11.807	3257	3271	3292	rBV	215352	359996	56.36%	7.405%
19	12.190	3378	3390	3409	rBV	158206	274170	42.92%	5.639%




Sum of corrected areas: 4861725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082824\
Data File : VU060559.D
Acq On : 28 Aug 2024 16:45
Operator : MD/SY
Sample : P3755-01DL 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

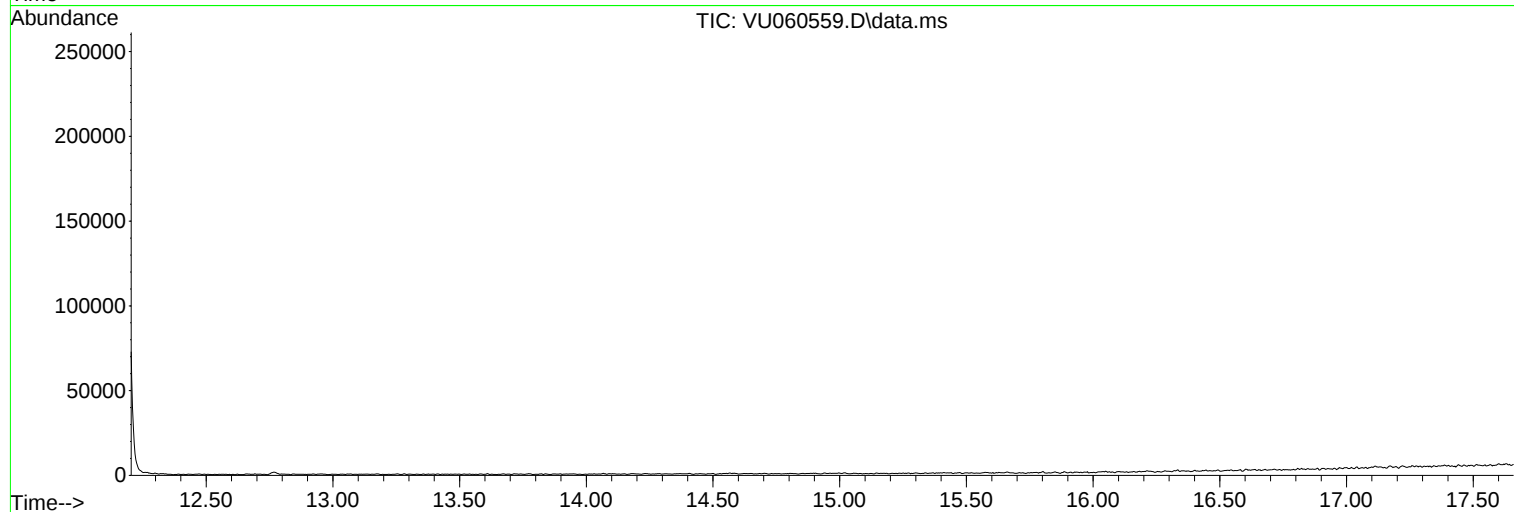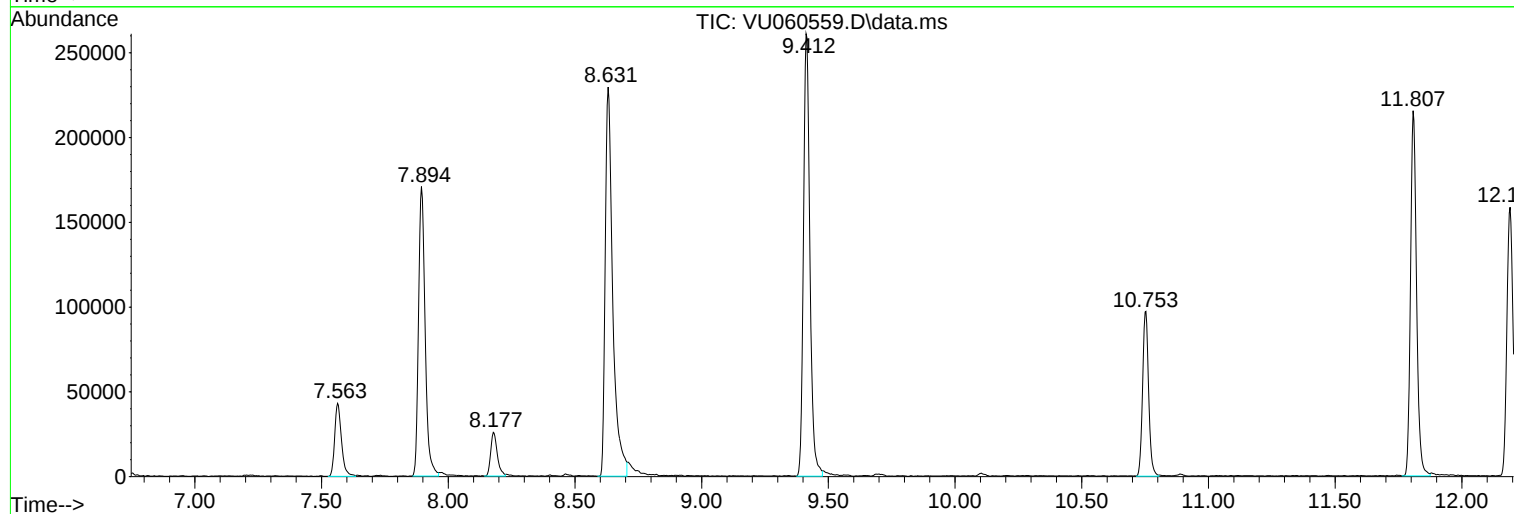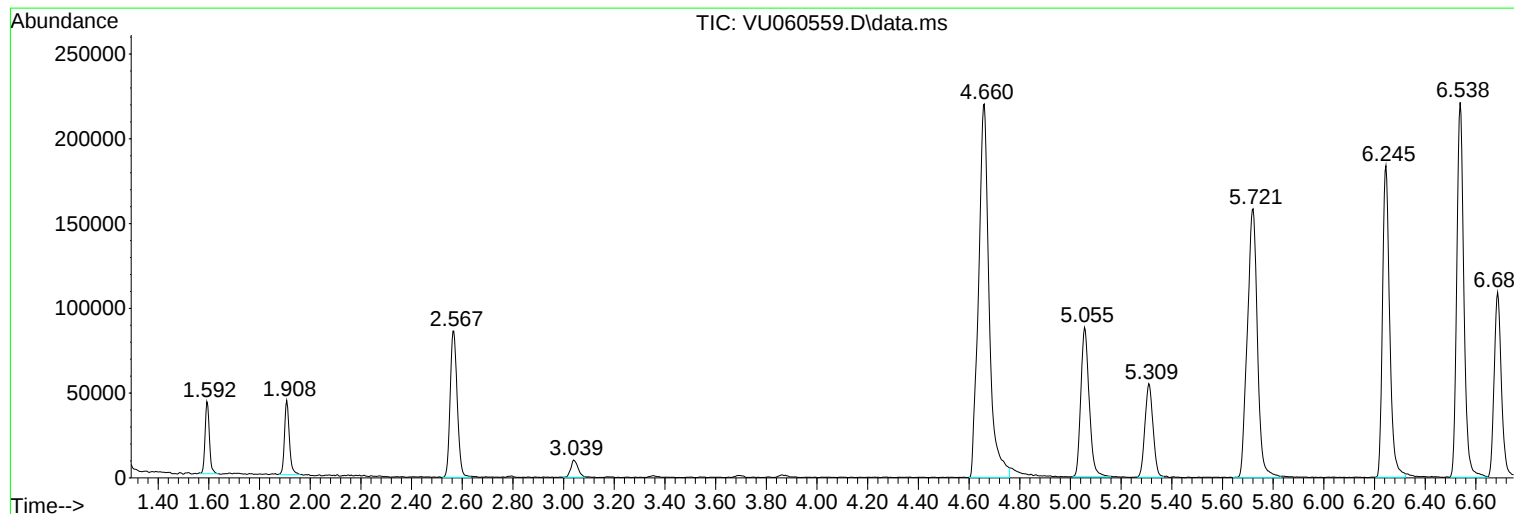

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082824\
Data File : VU060559.D
Acq On : 28 Aug 2024 16:45
Operator : MD/SY
Sample : P3755-01DL 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082824\
Data File : VU060559.D
Acq On : 28 Aug 2024 16:45
Operator : MD/SY
Sample : P3755-01DL 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc