


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082918\
Data File : VU026421.D
Acq On : 29 Aug 2018 13:58
Operator : MD/SY
Sample : BFB43
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Title : VOC Analysis
Last Update : Thu Aug 30 02:20:47 2018

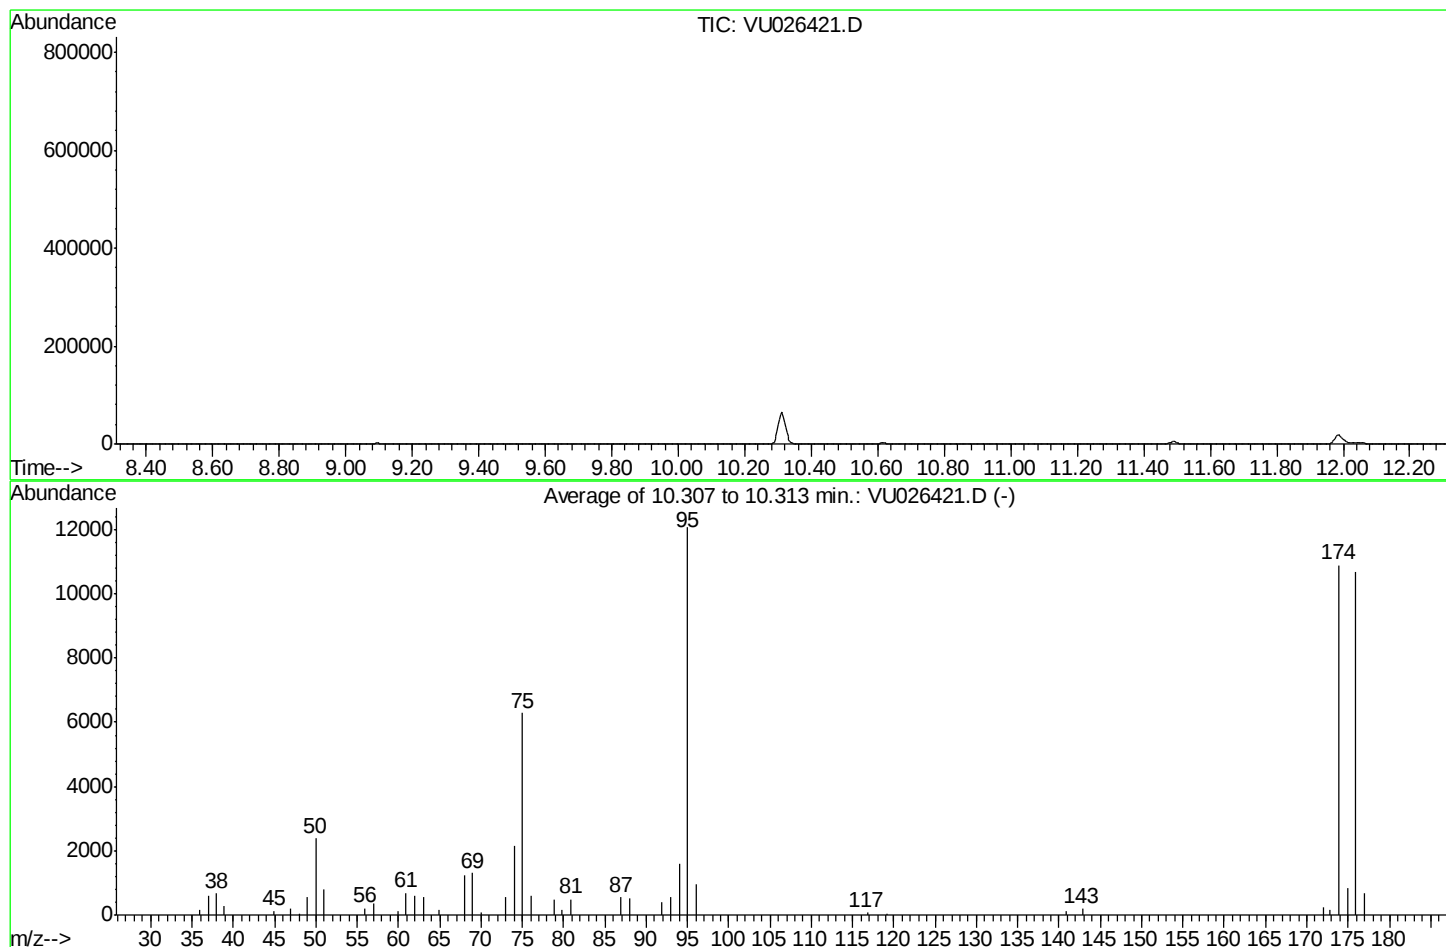

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	2380	PASS
75	95	30	80	52.1	6293	PASS
95	95	100	100	100.0	12069	PASS
96	95	5	9	7.8	939	PASS
173	174	0.00	2	1.5	160	PASS
174	95	50	120	90.2	10882	PASS
175	174	5	9	7.6	830	PASS
176	174	95	101	98.0	10668	PASS
177	176	5	9	6.3	675	PASS

m/z	Abundance
44.00	255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	134.0
37.00	603.0
38.00	655.0
38.90	271.0
44.00	224.0
44.90	126.0
47.00	234.0
49.00	583.0
50.00	2329.0
51.00	731.0
56.00	186.0
57.00	346.0
60.00	137.0
61.00	753.0
62.00	564.0
63.00	569.0
64.90	130.0
68.00	1194.0
69.00	1264.0
70.00	119.0
72.90	579.0
74.00	2014.0
75.00	6170.0
76.00	561.0
78.80	491.0
79.80	155.0
80.90	448.0
87.00	570.0
88.00	495.0
91.90	362.0
92.90	568.0
94.00	1537.0
95.00	11611.0
96.00	899.0
140.80	105.0
142.80	162.0
171.90	242.0
172.80	131.0
173.90	10305.0
174.90	797.0
175.90	9913.0
176.90	633.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	144.0
37.00	612.0
38.00	676.0
38.90	290.0
43.90	228.0
45.00	137.0
47.00	228.0
48.00	109.0
48.90	573.0
50.00	2429.0
51.00	822.0
55.90	217.0
57.00	370.0
59.90	134.0
61.00	702.0
62.00	633.0
63.00	590.0
65.00	174.0
68.00	1266.0
69.00	1338.0
70.00	104.0
72.90	548.0
74.00	2258.0
75.00	6504.0
76.00	621.0
78.80	502.0
79.90	148.0
80.90	499.0
87.00	538.0
88.00	521.0
91.90	394.0
93.00	595.0
94.00	1629.0
95.00	12443.0
96.00	988.0
116.80	109.0
119.10	104.0
140.80	109.0
142.80	200.0
171.90	276.0
172.80	173.0
173.90	11260.0
174.90	860.0
175.90	11052.0
176.90	717.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	152.0
37.00	575.0
38.00	647.0
38.90	277.0
43.90	256.0
45.00	112.0
47.00	190.0
48.90	513.0
50.00	2382.0
51.00	839.0
55.90	206.0
57.00	339.0
59.90	114.0
60.90	629.0
62.00	609.0
63.00	556.0
65.00	188.0
68.00	1216.0
69.00	1314.0
72.90	539.0
74.00	2244.0
75.00	6206.0
76.00	595.0
78.90	460.0
79.90	148.0
80.90	506.0
86.90	537.0
88.00	494.0
91.90	413.0
93.00	552.0
94.00	1626.0
95.00	12155.0
96.00	930.0
116.80	122.0
140.80	113.0
142.80	223.0
172.00	261.0
172.80	176.0
173.90	11082.0
174.90	833.0
175.90	11041.0
176.90	676.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43