



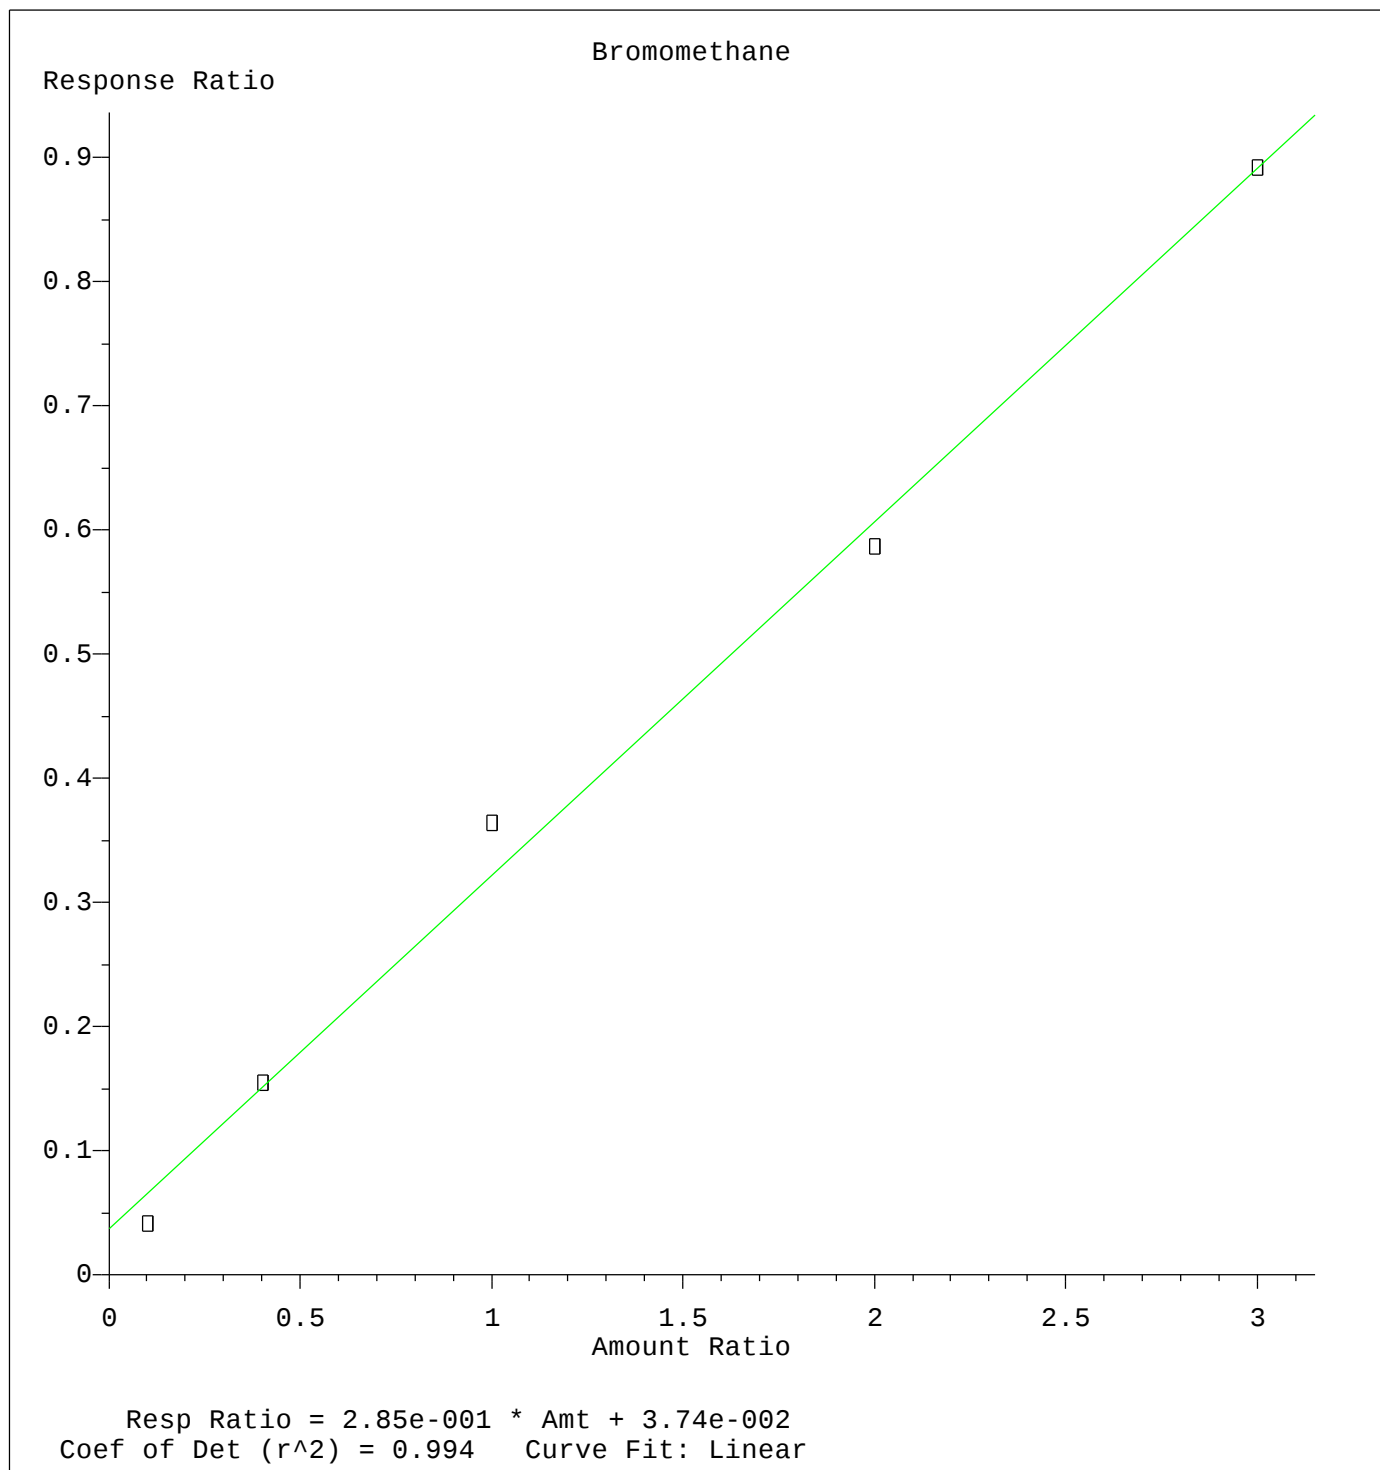


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Calibration Table Last Updated: Thu Aug 29 04:11:12 2019

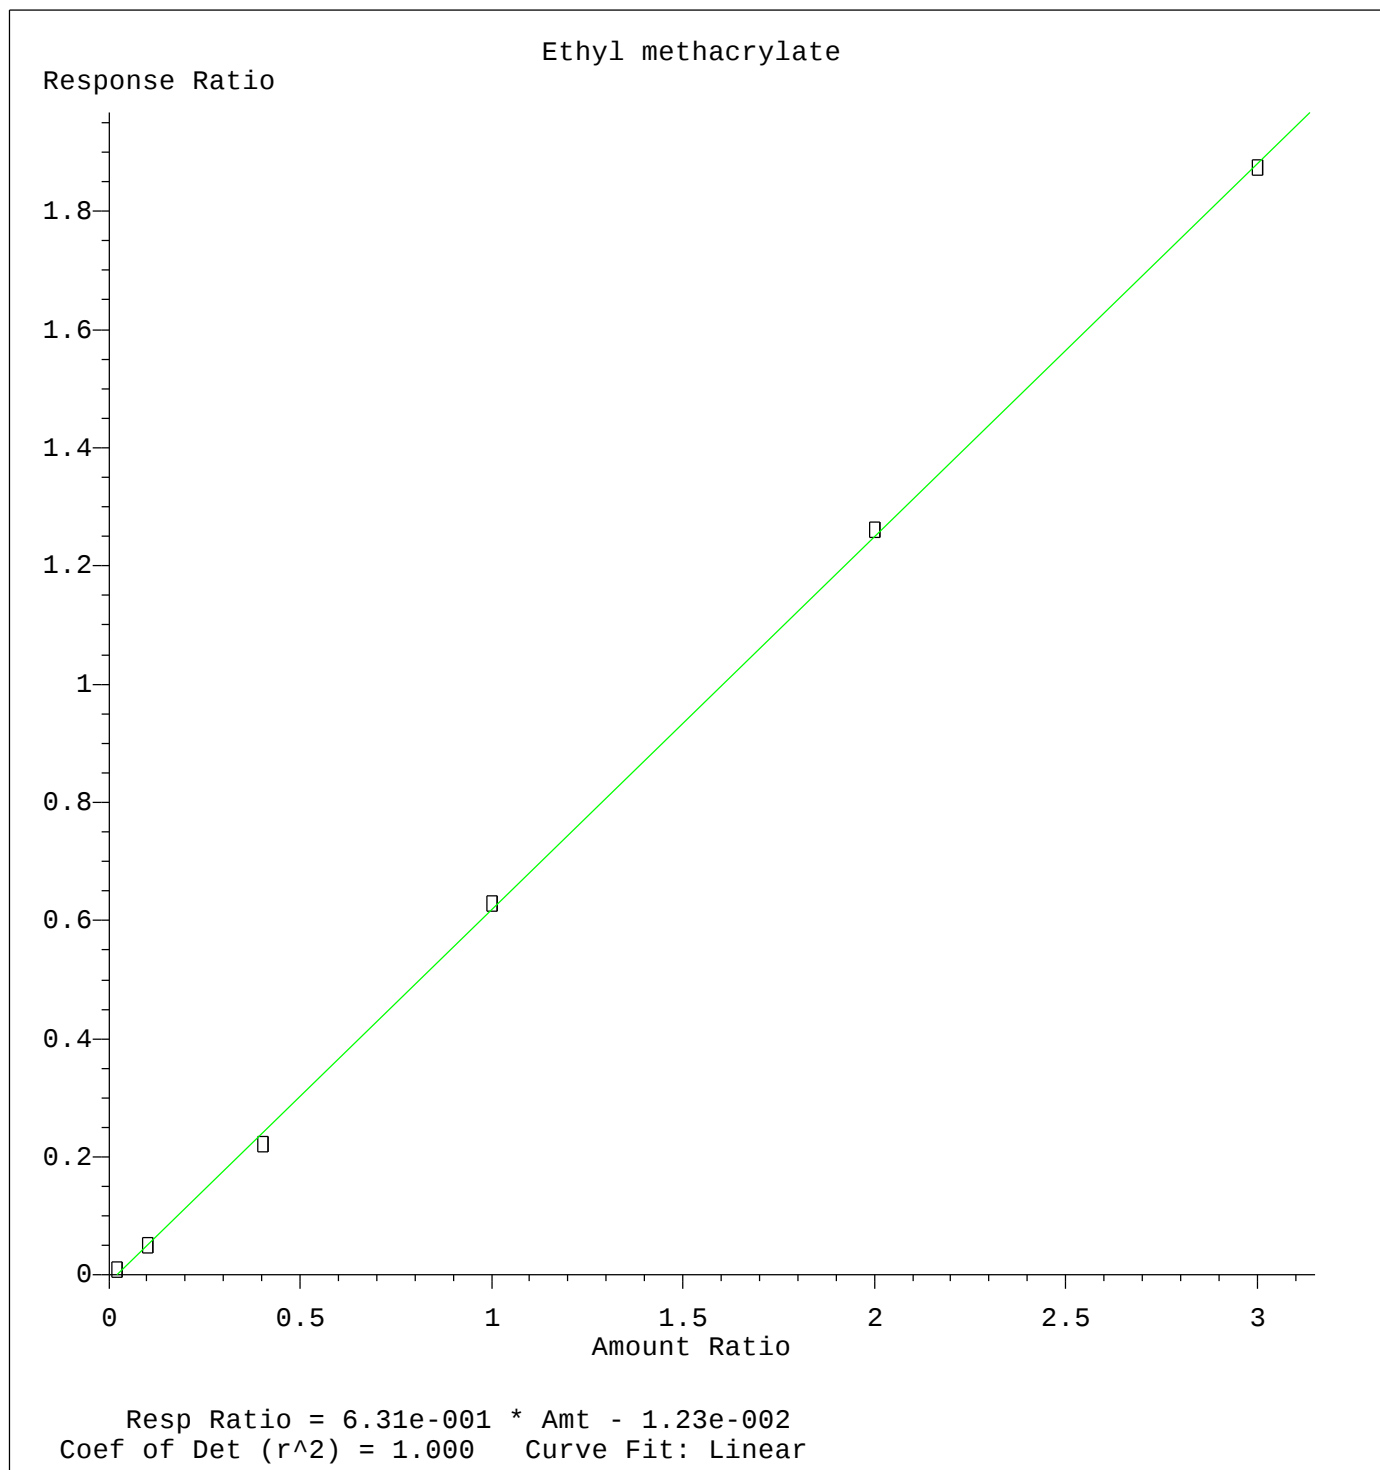

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Calibration Table Last Updated: Thu Aug 29 04:11:12 2019

1,2,4-Trichlorobenzene

Response Ratio

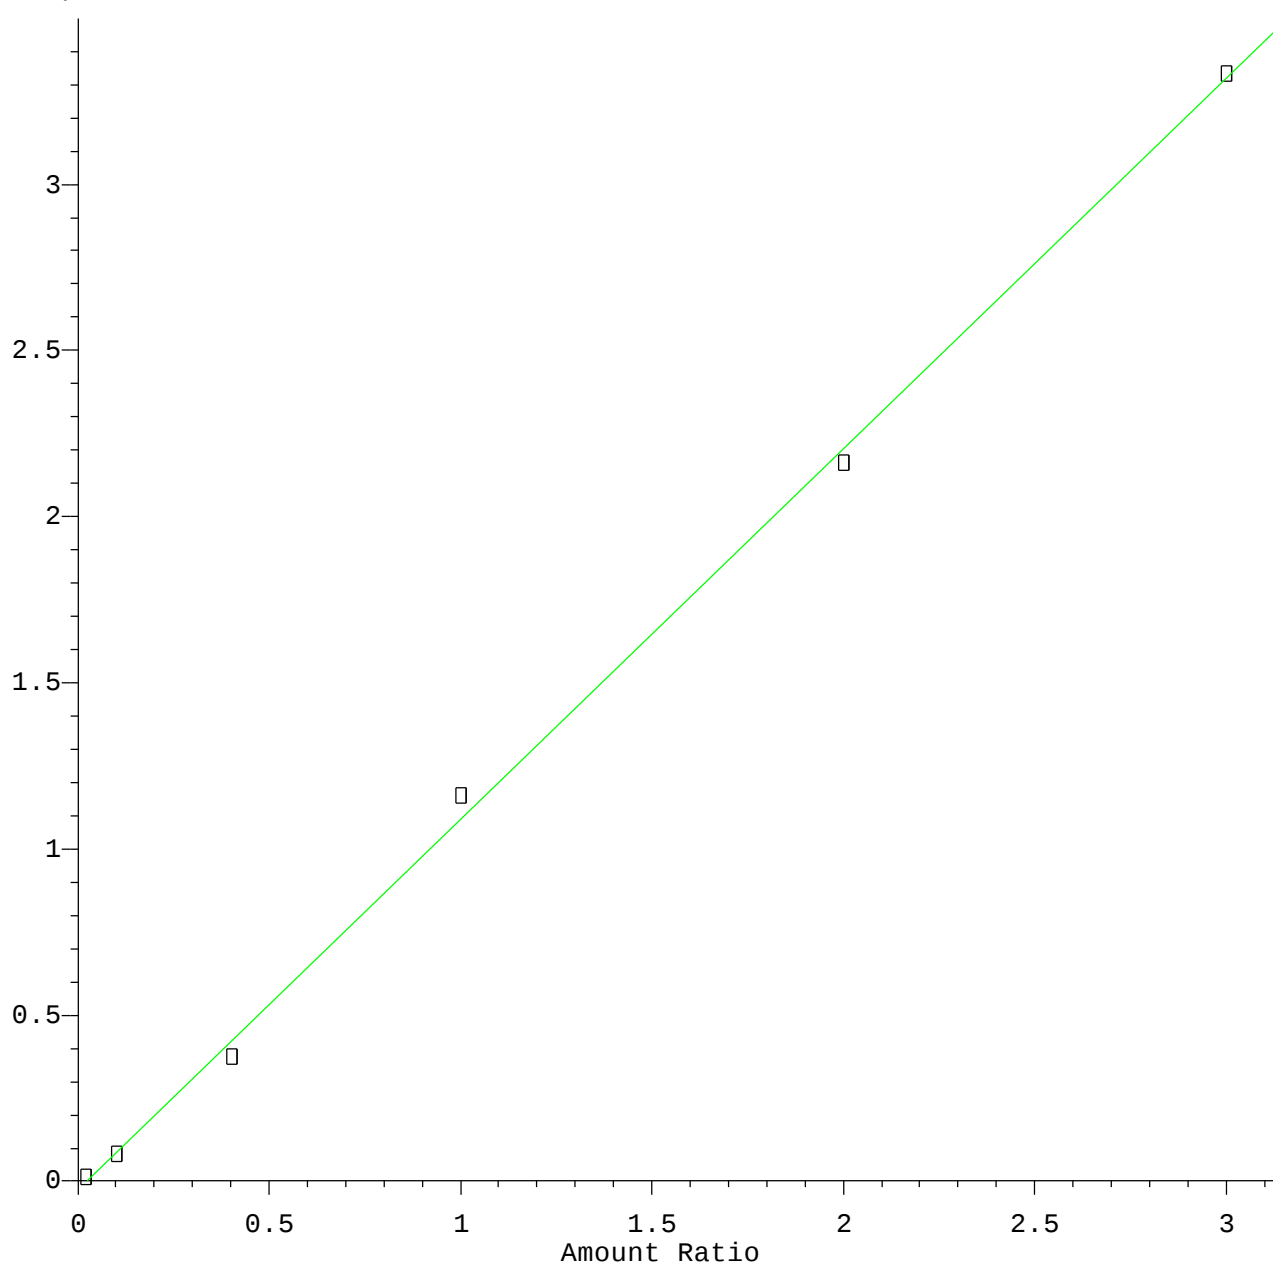


Resp Ratio = 1.11e+000 * Amt - 2.48e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Calibration Table Last Updated: Thu Aug 29 04:11:12 2019


Naphthalene

Response Ratio

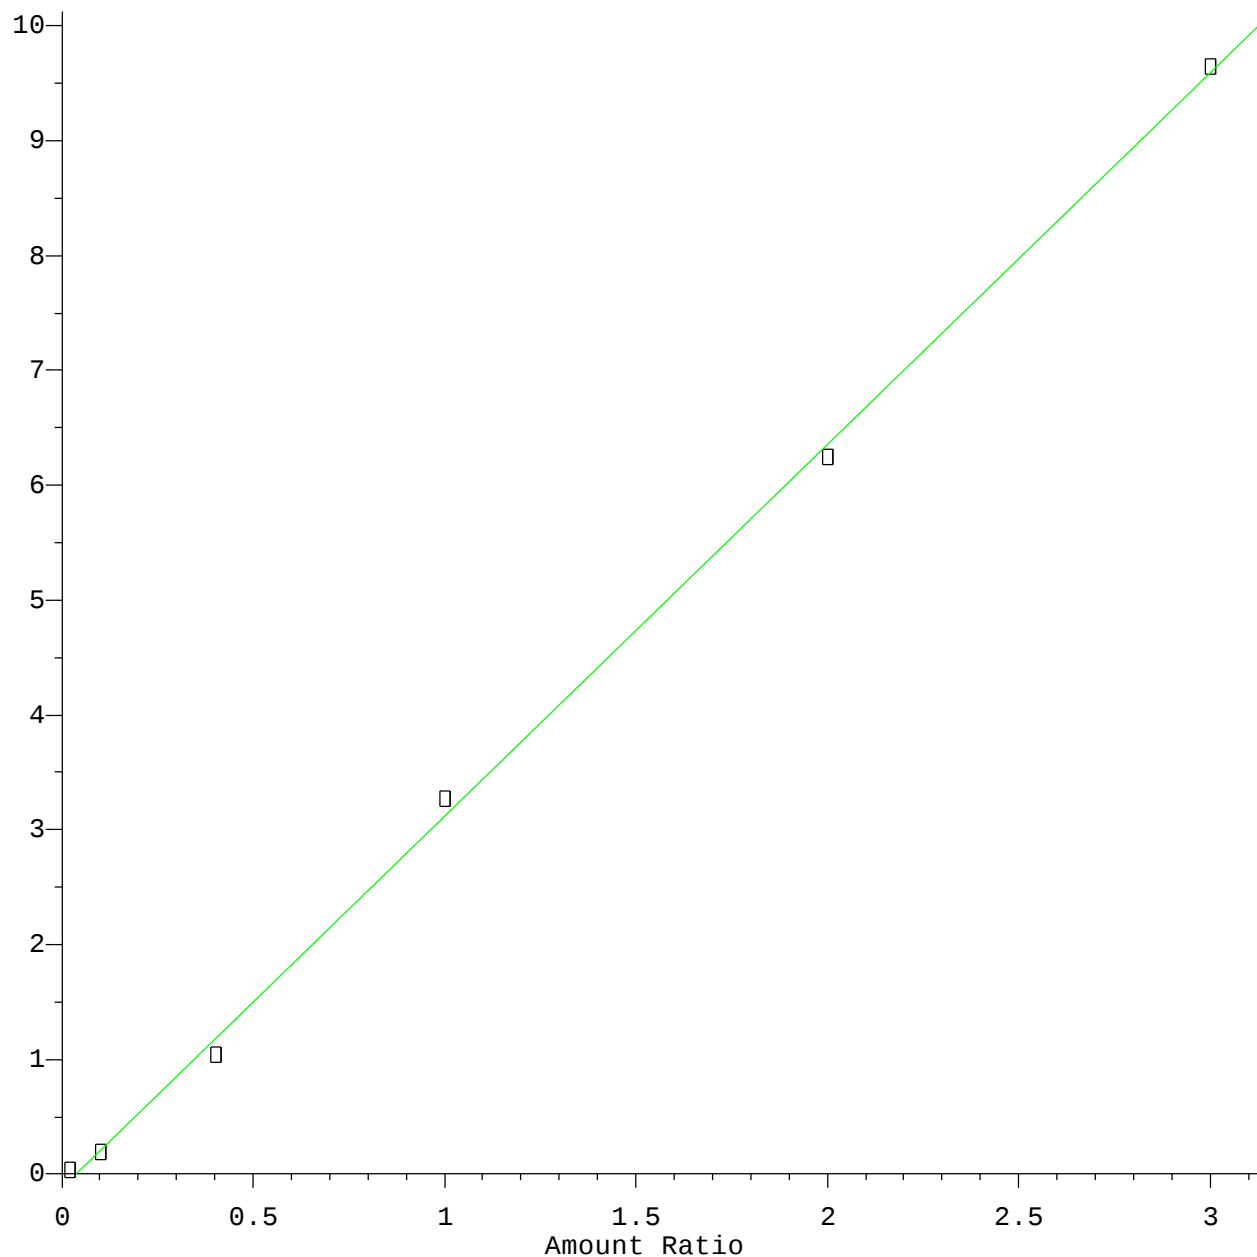

Resp Ratio = 3.24×10^0 * Amt - 1.16×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Calibration Table Last Updated: Thu Aug 29 04:11:12 2019

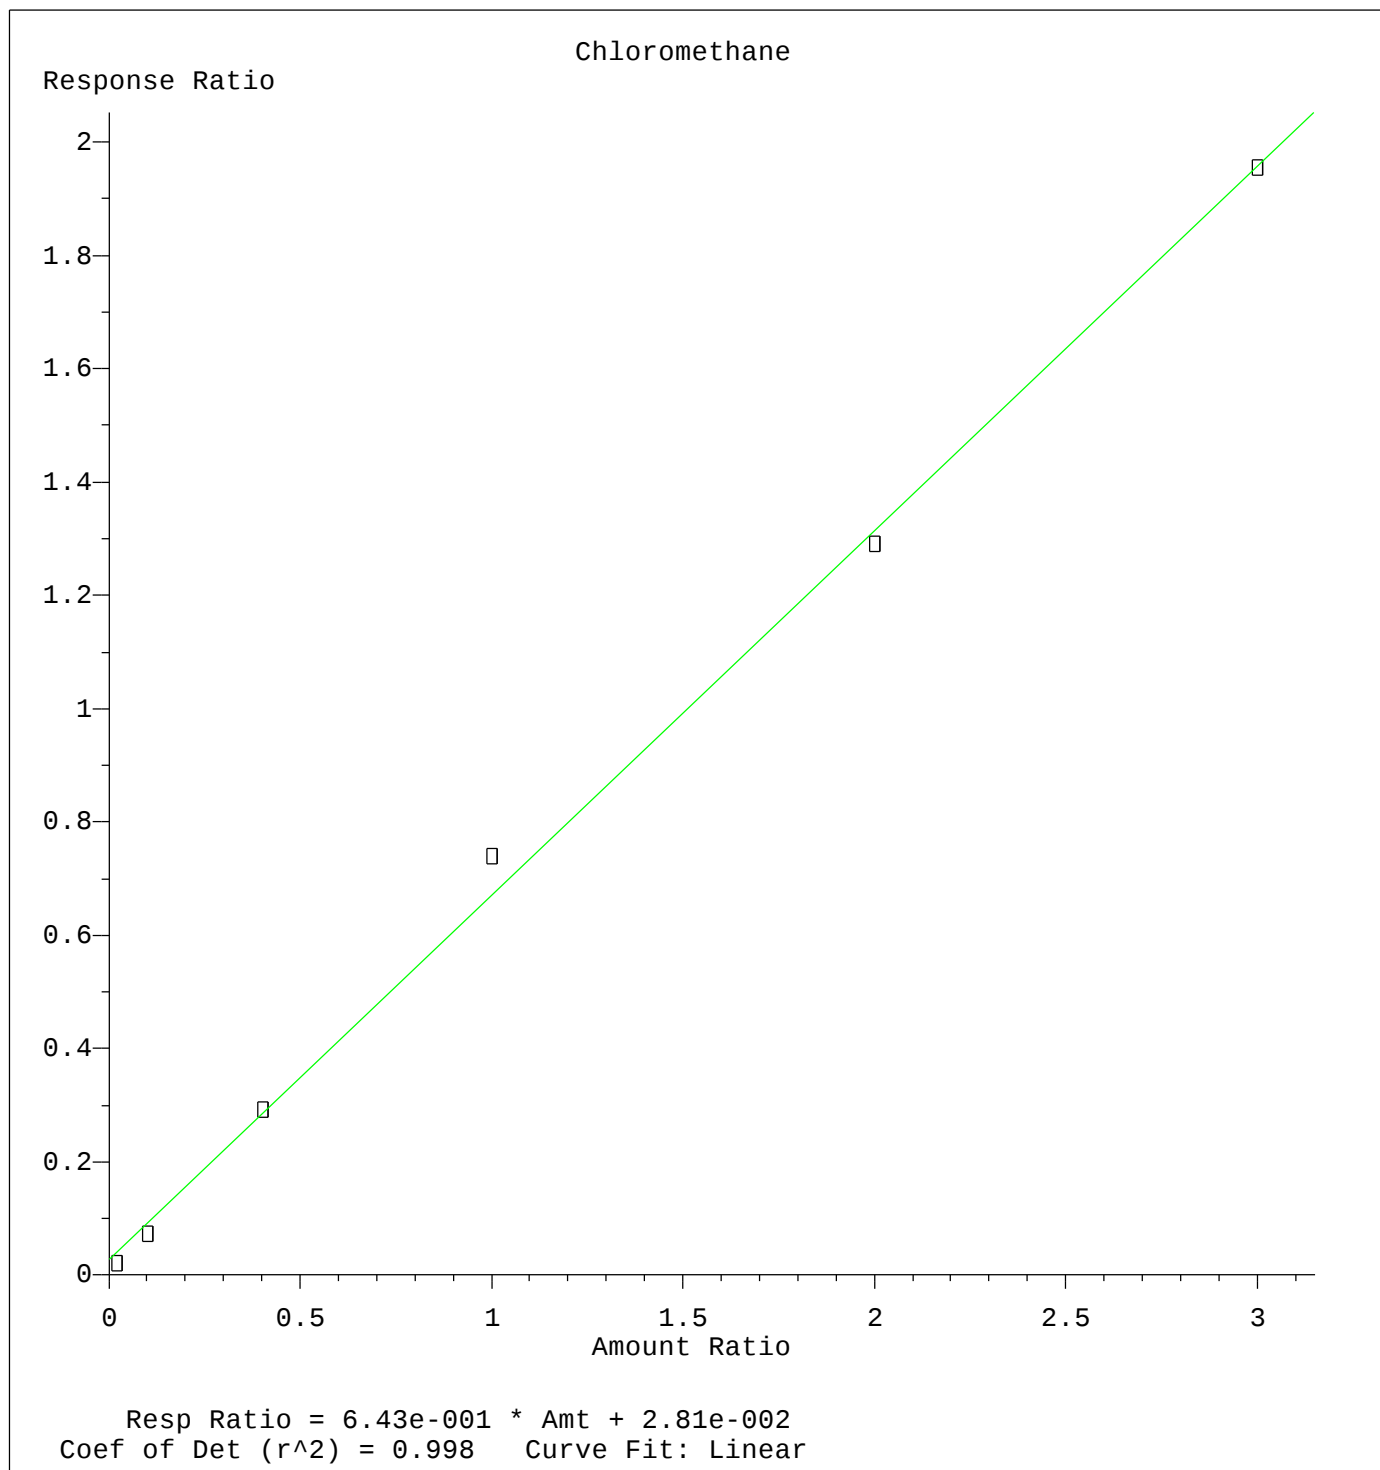

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Calibration Table Last Updated: Thu Aug 29 04:11:12 2019