


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082919\
Data File : VU034014.D
Acq On : 28 Aug 2019 09:02
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Title : SW846 8260
Last Update : Thu Aug 29 04:11:12 2019

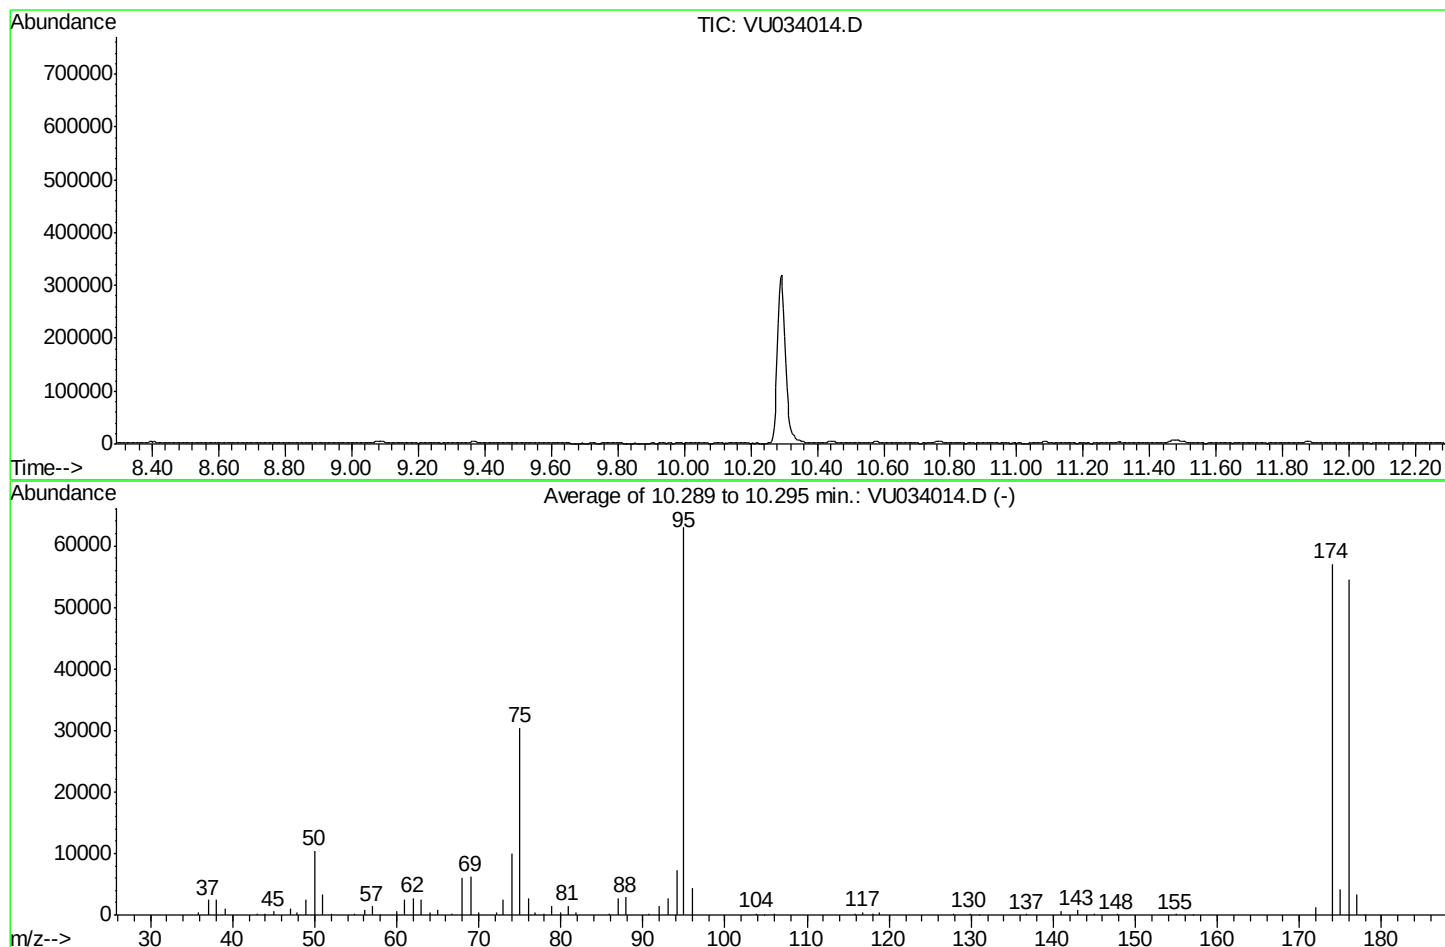

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	10402	PASS
75	95	30	60	48.3	30400	PASS
95	95	100	100	100.0	62984	PASS
96	95	5	9	7.0	4415	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.6	57058	PASS
175	174	5	9	7.4	4242	PASS
176	174	95	101	95.6	54557	PASS
177	176	5	9	6.2	3379	PASS