


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU082919\
 Data File : VU034022.D
 Acq On : 28 Aug 2019 14:25
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Title : SW846 8260
 Last Update : Thu Aug 29 04:11:12 2019

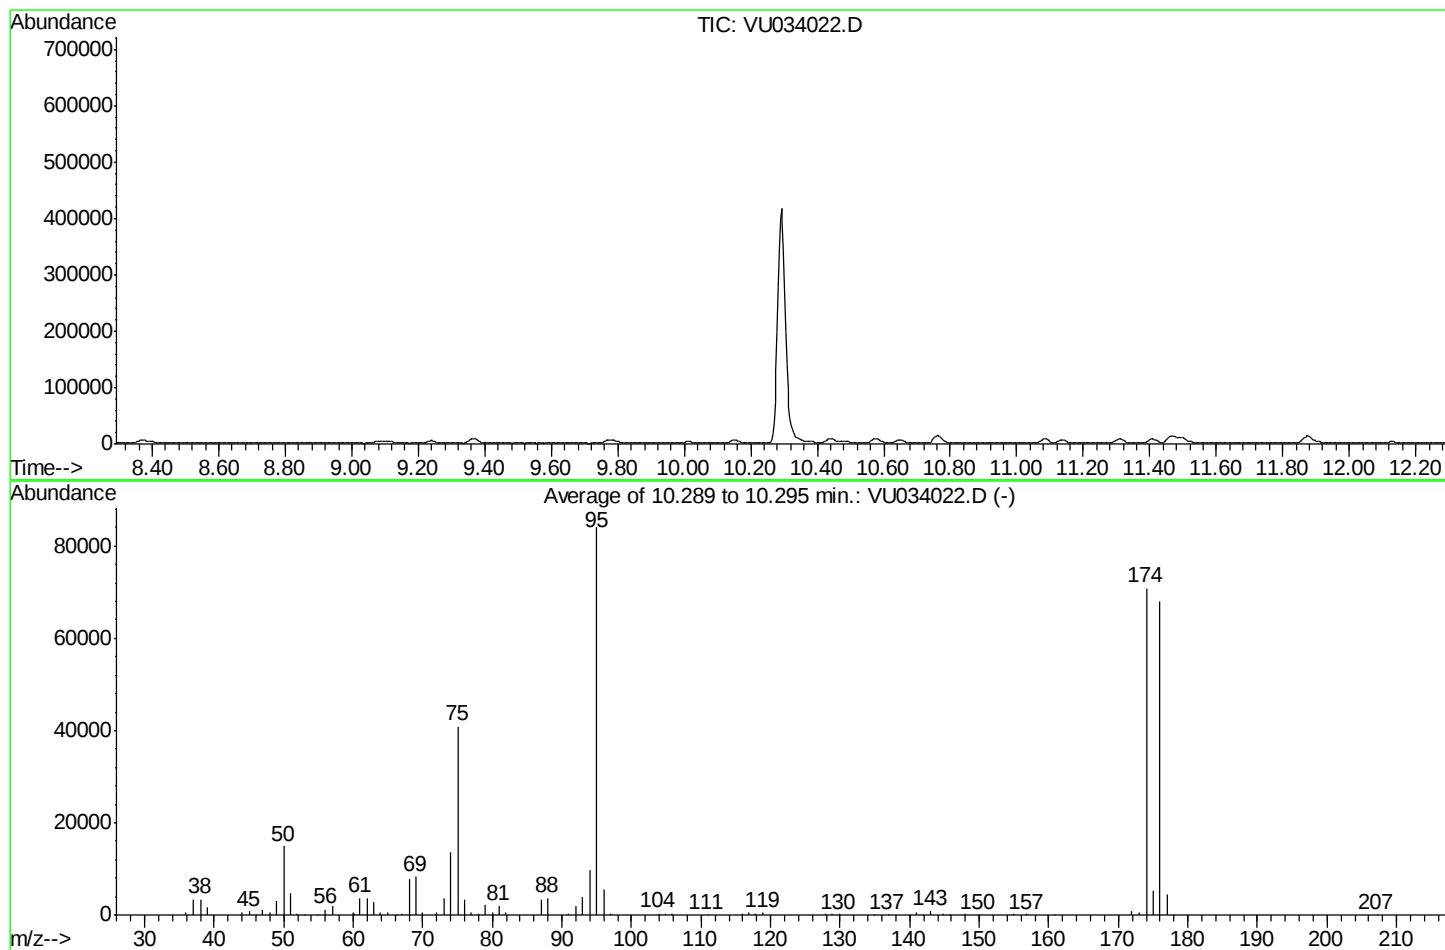

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	14923	PASS
75	95	30	60	48.7	40909	PASS
95	95	100	100	100.0	84072	PASS
96	95	5	9	6.7	5630	PASS
173	174	0.00	2	0.6	436	PASS
174	95	50	100	84.4	70917	PASS
175	174	5	9	7.3	5197	PASS
176	174	95	101	95.8	67949	PASS
177	176	5	9	6.5	4426	PASS