

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050480.D
 Acq On : 29 Aug 2022 13:26
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Quant Time: Aug 30 02:14:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 30 02:11:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	189604	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	177834	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	59767	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	102743	45.828	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	91.660%	
7) Chloroethane-d5	1.893	69	80154	48.317	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	96.640%	
11) 1,1-Dichloroethene-d2	2.559	63	121627	38.388	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	76.780%	
21) 2-Butanone-d5	4.623	46	202101	137.724	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	137.720%#	
24) Chloroform-d	5.060	84	167596	46.569	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.140%	
26) 1,2-Dichloroethane-d4	5.700	65	107756	48.176	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.360%	
32) Benzene-d6	5.726	84	332747	50.640	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.280%	
36) 1,2-Dichloropropane-d6	6.690	67	112375	51.624	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.240%	
41) Toluene-d8	7.899	98	252365	43.892	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.780%	
43) trans-1,3-Dichloroprop...	8.179	79	39072	43.030	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.060%	
47) 2-Hexanone-d5	8.632	63	89585	110.897	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	110.900%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	181094	53.937	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	107.880%	
66) 1,2-Dichlorobenzene-d4	12.195	152	78537	55.009	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	110.020%	
Target Compounds						
13) Acetone	2.626	43	8951	9.277	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050480.D
Acq On : 29 Aug 2022 13:26
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Time: Aug 30 02:14:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 30 02:11:49 2022
Response via : Initial Calibration

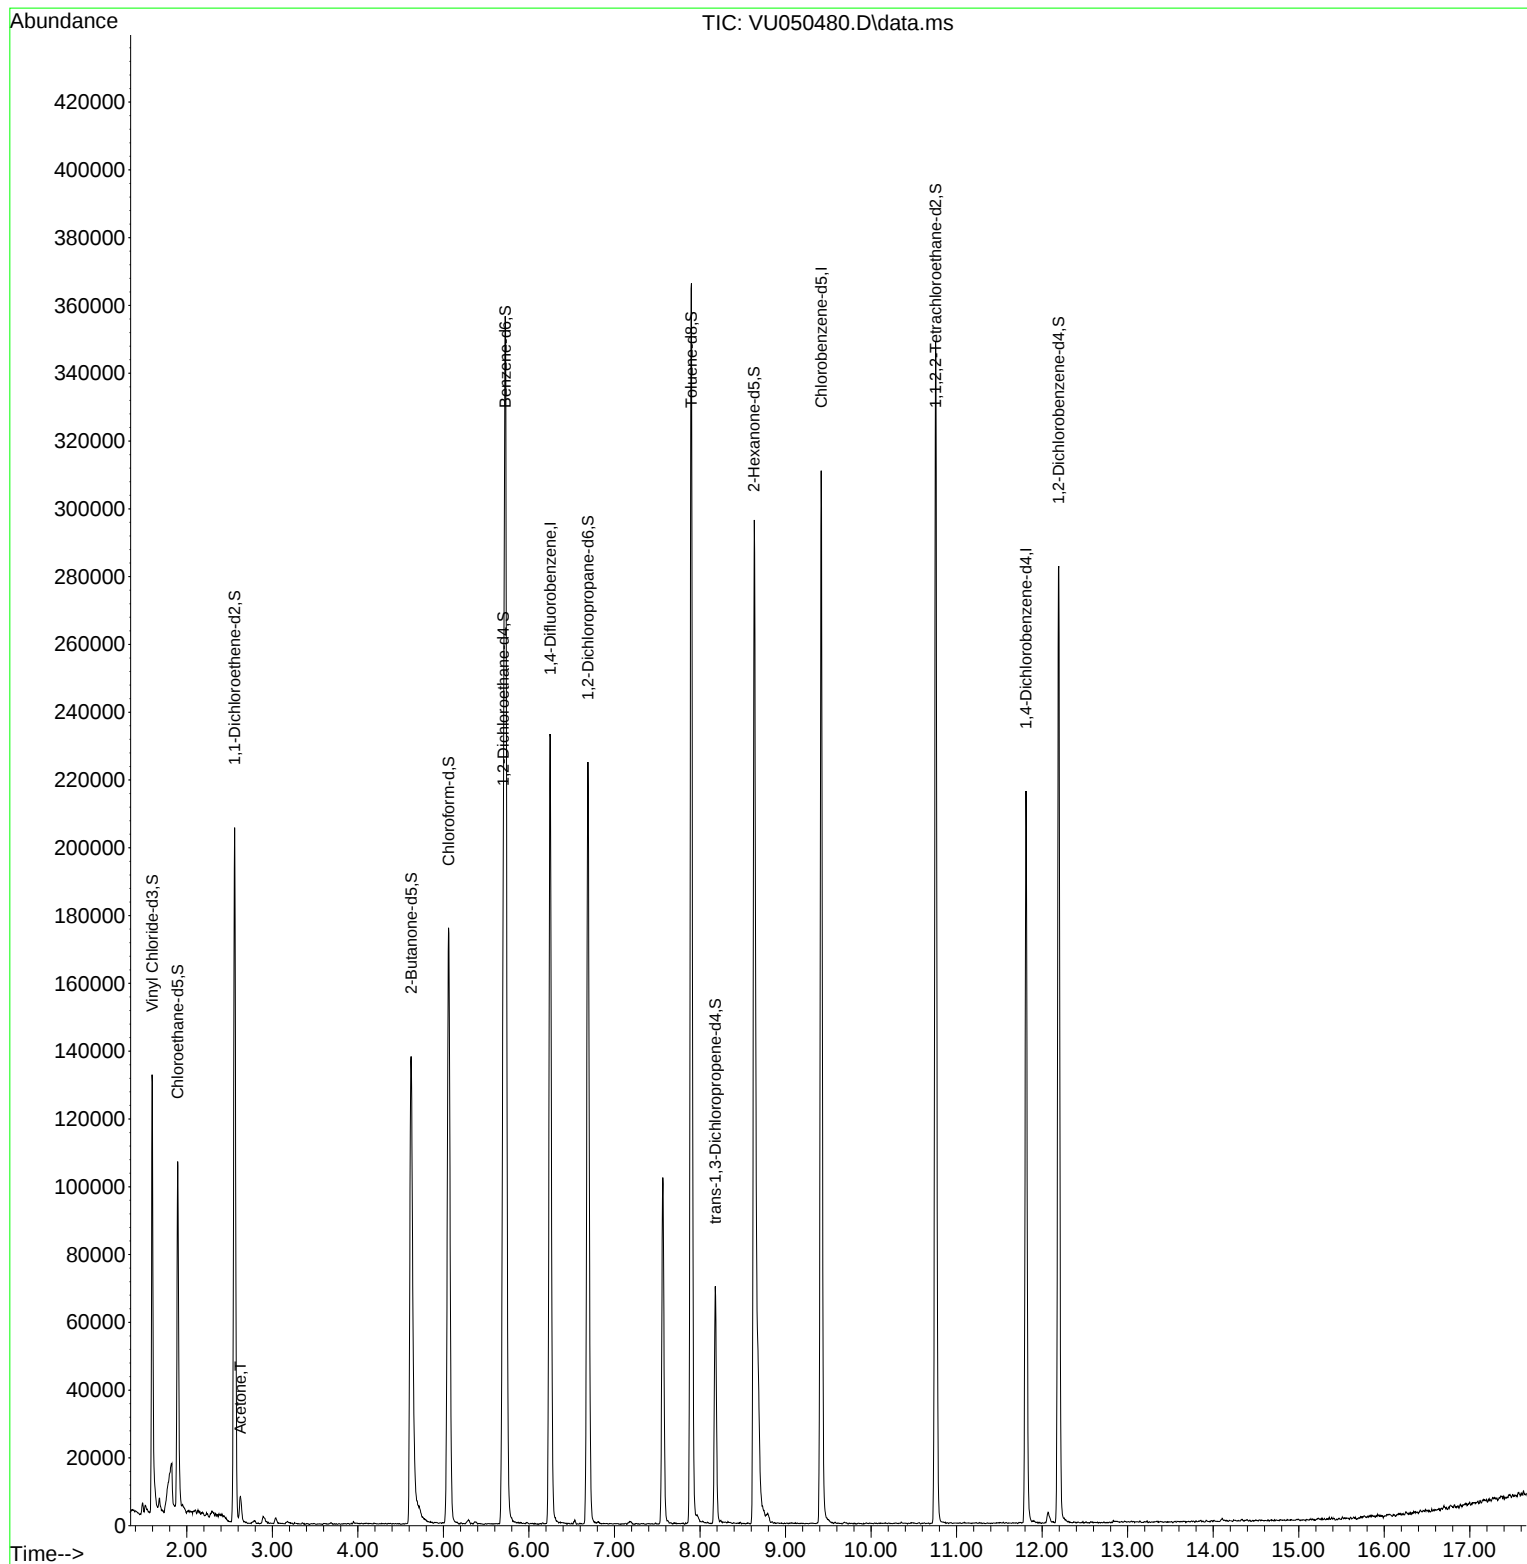

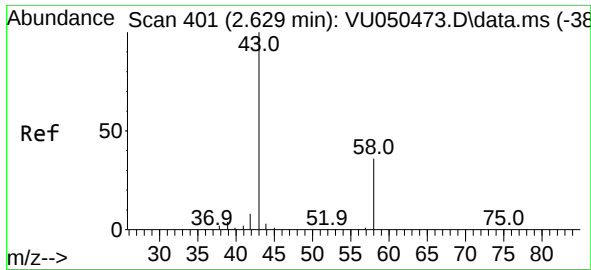

#13

Acetone

Concen: 9.277 ug/L

RT: 2.626 min Scan# 40

Delta R.T. -0.003 min

Lab File: VU050480.D


Acq: 29 Aug 2022 13:26

Instrument :

MSVOA_U

ClientSampleId :

DBVJ6

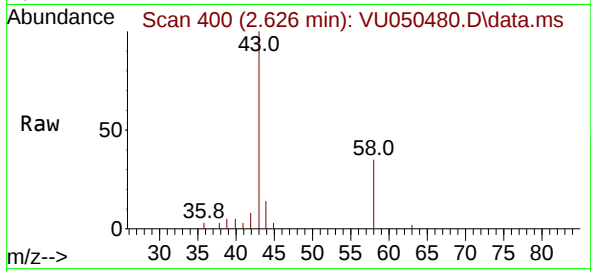

Tgt Ion: 43 Resp: 8951

Ion Ratio Lower Upper

43 100

58 33.4 0.0 72.2

