

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050508.D
 Acq On : 30 Aug 2022 01:03
 Operator : SY/MD
 Sample : N4344-08ME
 Misc : 5.09g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ7ME

Quant Time: Aug 30 05:32:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 30 05:29:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	403656	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	382908	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	140286	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	67991	14.245	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	28.500%#		
7) Chloroethane-d5	1.893	69	30389	8.605	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	17.200%#		
11) 1,1-Dichloroethene-d2	2.527	63	159491	23.645	ug/L	-0.04
Spiked Amount 50.000	Range 60 - 125		Recovery =	47.280%#		
21) 2-Butanone-d5	4.649	46	267821	85.728	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.730%		
24) Chloroform-d	5.060	84	256660	33.499	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	67.000%#		
26) 1,2-Dichloroethane-d4	5.700	65	183465	38.528	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.060%		
32) Benzene-d6	5.719	84	562144	39.732	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.460%		
36) 1,2-Dichloropropane-d6	6.690	67	188963	40.316	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	80.640%		
41) Toluene-d8	7.899	98	453609	36.640	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.280%#		
43) trans-1,3-Dichloroprop...	8.182	79	53159	27.189	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.380%#		
47) 2-Hexanone-d5	8.665	63	159304	91.587	ug/L	0.03
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.590%		
56) 1,1,2,2-Tetrachloroeth...	10.764	84	253148	35.017	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	70.040%		
66) 1,2-Dichlorobenzene-d4	12.198	152	145444	43.401	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.800%		
Target Compounds						Qvalue
16) Methylene chloride	3.031	84	4296	1.245	ug/L	96
46) Tetrachloroethene	8.552	164	99602	49.418	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050508.D
Acq On : 30 Aug 2022 01:03
Operator : SY/MD
Sample : N4344-08ME
Misc : 5.09g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVQ7ME

Quant Time: Aug 30 05:32:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 30 05:29:53 2022
Response via : Initial Calibration




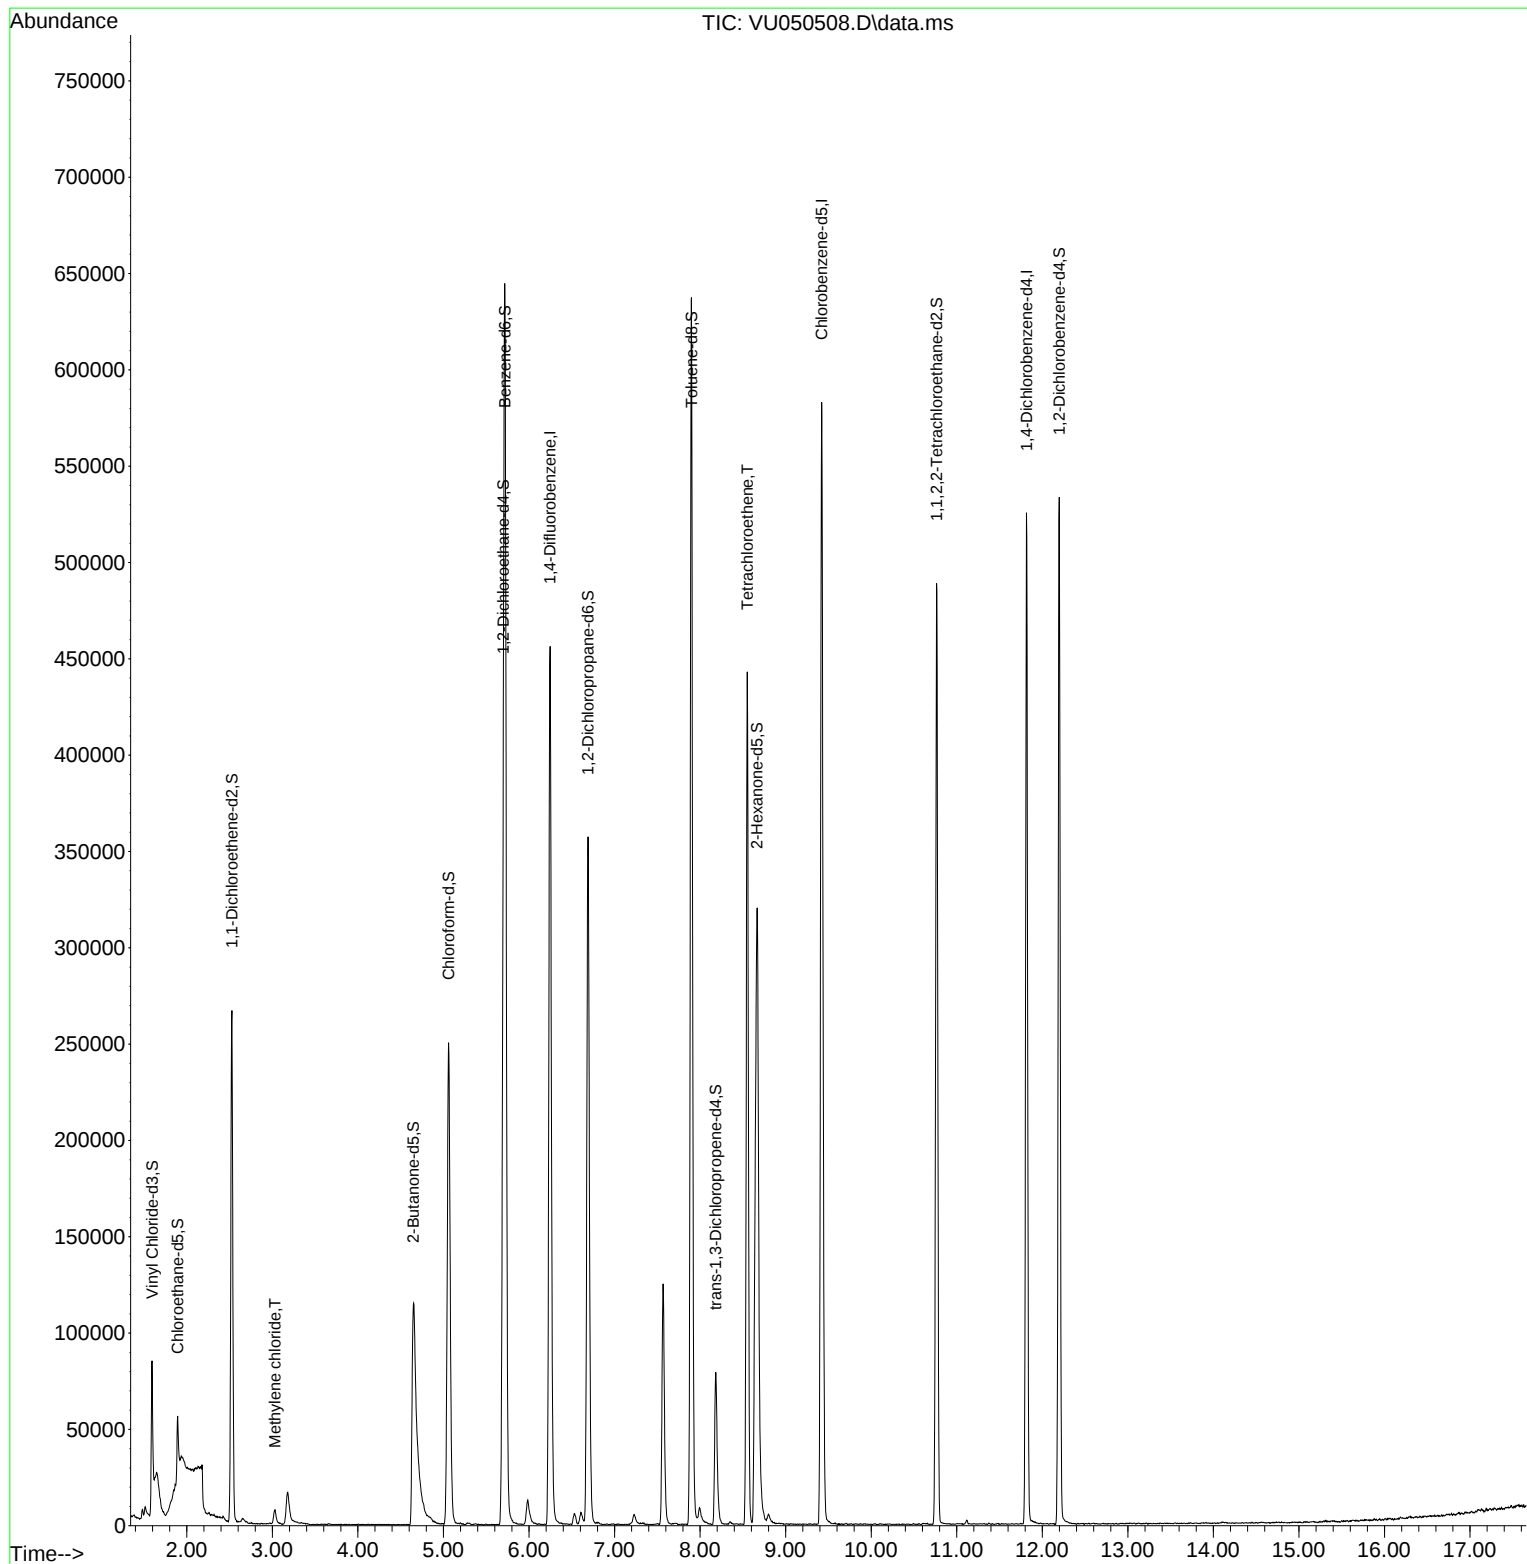


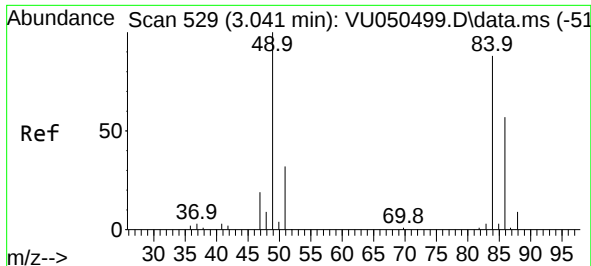

#16
Methylene chloride
Concen: 1.245 ug/L
RT: 3.031 min Scan# 51
Delta R.T. -0.009 min
Lab File: VU050508.D
Acq: 30 Aug 2022 01:03

Instrument :
MSVOA_U
ClientSampleId :
DBVQ7ME

Tgt Ion: 84 Resp: 4296
Ion Ratio Lower Upper
84 100
86 70.2 43.9 81.5
49 113.2 80.4 149.4

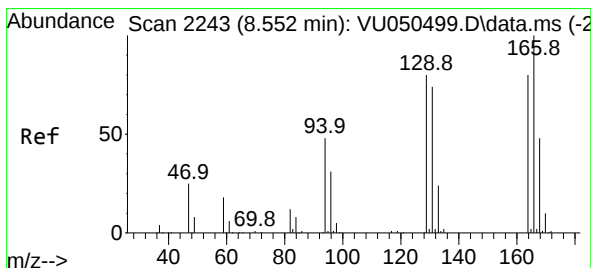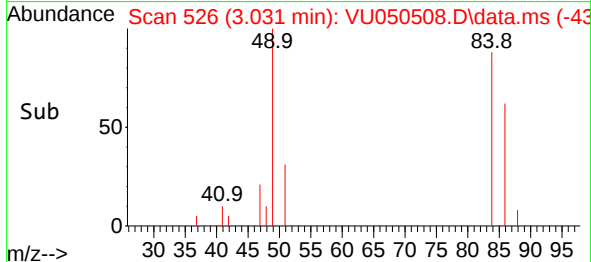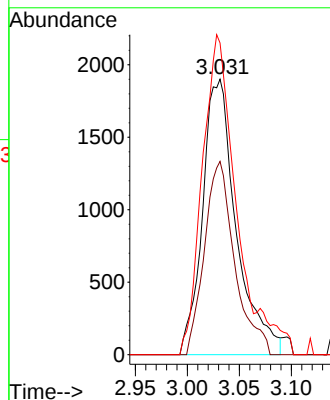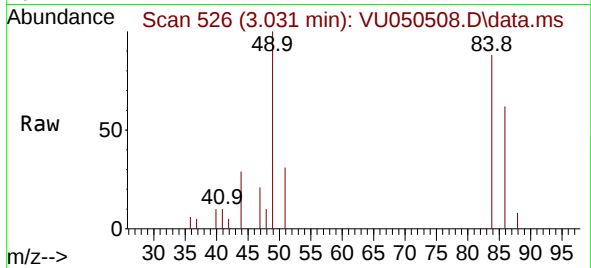

#46
Tetrachloroethene
Concen: 49.418 ug/L
RT: 8.552 min Scan# 2243
Delta R.T. 0.000 min
Lab File: VU050508.D
Acq: 30 Aug 2022 01:03

Tgt Ion:164 Resp: 99602
Ion Ratio Lower Upper
164 100
129 97.0 68.0 126.4
131 95.7 65.4 121.4
166 125.6 86.5 160.7

