

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050476.D
 Acq On : 29 Aug 2022 11:44
 Operator : SY/MD
 Sample : VU0829WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	98	rBV	169315	204227	13.91%	2.002%
2	1.897	165	173	194	rVB	147573	200112	13.63%	1.962%
3	2.559	367	379	397	rBV	277208	443811	30.23%	4.351%
4	2.739	433	435	438	rVB3	390	171	0.01%	0.002%
5	2.784	445	449	457	rVB5	834	1131	0.08%	0.011%
6	2.919	489	491	497	rVB4	277	215	0.01%	0.002%
7	2.961	501	504	508	rVB2	268	234	0.02%	0.002%
8	3.044	519	530	542	rVB5	3286	6381	0.43%	0.063%
9	3.183	562	573	593	rVB3	2320	5752	0.39%	0.056%
10	3.257	593	596	598	rBV2	214	139	0.01%	0.001%
11	3.273	598	601	604	rVB	326	202	0.01%	0.002%
12	3.295	604	608	614	rBV	238	281	0.02%	0.003%
13	3.356	622	627	630	rBV3	334	319	0.02%	0.003%
14	3.588	695	699	705	rVB2	256	261	0.02%	0.003%
15	3.720	734	740	742	rBV2	214	208	0.01%	0.002%
16	3.864	782	785	786	rBV	359	154	0.01%	0.002%
17	4.006	818	829	834	rBV	245	377	0.03%	0.004%
18	4.064	842	847	849	rBV2	220	211	0.01%	0.002%
19	4.080	849	852	856	rVB	322	268	0.02%	0.003%
20	4.121	862	865	868	rBV2	235	199	0.01%	0.002%
21	4.160	873	877	881	rVV	162	162	0.01%	0.002%
22	4.459	964	970	976	rBV2	429	606	0.04%	0.006%
23	4.488	976	979	981	rBV	220	161	0.01%	0.002%
24	4.572	1001	1005	1008	rBV2	235	163	0.01%	0.002%
25	4.623	1008	1021	1053	rBV	151374	398564	27.15%	3.908%
26	4.845	1088	1090	1094	rVB2	476	268	0.02%	0.003%
27	4.909	1108	1110	1116	rVB3	296	235	0.02%	0.002%
28	4.967	1126	1128	1133	rBV2	200	184	0.01%	0.002%
29	5.060	1140	1157	1186	rBV	267199	585773	39.91%	5.743%
30	5.285	1221	1227	1230	rBV4	1046	1227	0.08%	0.012%
31	5.359	1244	1250	1251	rBV	750	678	0.05%	0.007%
32	5.523	1298	1301	1307	rVB2	421	360	0.02%	0.004%
33	5.556	1307	1311	1313	rBV	189	176	0.01%	0.002%
34	5.652	1337	1341	1342	rBV2	244	150	0.01%	0.001%
35	5.723	1342	1363	1397	rVV2	539168	1467911	100.00%	14.393%
36	6.002	1447	1450	1455	rBV2	227	221	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050476.D
 Acq On : 29 Aug 2022 11:44
 Operator : SY/MD
 Sample : VU0829WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.038	1455	1461	1466	rBV4	437	534	0.04%	0.005%
38	6.064	1466	1469	1473	rVB2	299	218	0.01%	0.002%
39	6.083	1473	1475	1478	rBV2	206	162	0.01%	0.002%
40	6.112	1481	1484	1486	rBV2	190	168	0.01%	0.002%
41	6.247	1511	1526	1546	rBV	353410	671024	45.71%	6.579%
42	6.533	1608	1615	1616	rBV2	1218	1386	0.09%	0.014%
43	6.604	1634	1637	1642	rBV2	259	272	0.02%	0.003%
44	6.691	1649	1664	1685	rBV	347181	679795	46.31%	6.665%
45	6.835	1707	1709	1712	rVB2	299	165	0.01%	0.002%
46	6.858	1712	1716	1718	rBV3	325	185	0.01%	0.002%
47	6.922	1734	1736	1743	rVB	319	276	0.02%	0.003%
48	6.957	1743	1747	1751	rBV2	228	224	0.02%	0.002%
49	7.109	1792	1794	1798	rVB3	541	361	0.02%	0.004%
50	7.134	1798	1802	1807	rBV2	176	148	0.01%	0.001%
51	7.179	1810	1816	1828	rVV5	800	1476	0.10%	0.014%
52	7.298	1850	1853	1857	rVB2	230	182	0.01%	0.002%
53	7.366	1869	1874	1875	rBV	243	168	0.01%	0.002%
54	7.565	1924	1936	1955	rBV2	167462	296690	20.21%	2.909%
55	7.793	2001	2007	2019	rVB5	882	1578	0.11%	0.015%
56	7.899	2025	2040	2058	rBV	589097	1018882	69.41%	9.990%
57	8.179	2116	2127	2147	rBV	115634	197084	13.43%	1.932%
58	8.340	2173	2177	2179	rBV2	256	218	0.01%	0.002%
59	8.395	2192	2194	2202	rVB4	643	518	0.04%	0.005%
60	8.478	2217	2220	2222	rBV	235	172	0.01%	0.002%
61	8.581	2246	2252	2256	rBV2	268	385	0.03%	0.004%
62	8.636	2256	2269	2299	rBV2	375286	821967	56.00%	8.059%
63	8.903	2348	2352	2355	rBV3	167	152	0.01%	0.001%
64	8.970	2371	2373	2376	rVV2	321	174	0.01%	0.002%
65	8.986	2376	2378	2382	rVB	260	170	0.01%	0.002%
66	9.170	2431	2435	2438	rBV2	242	187	0.01%	0.002%
67	9.417	2499	2512	2534	rBV	510059	848870	57.83%	8.323%
68	9.568	2553	2559	2563	rVB4	618	681	0.05%	0.007%
69	9.694	2593	2598	2605	rBV3	671	803	0.05%	0.008%
70	9.816	2633	2636	2640	rVB	207	144	0.01%	0.001%
71	9.858	2646	2649	2651	rBV	198	142	0.01%	0.001%
72	10.044	2704	2707	2710	rVB2	236	142	0.01%	0.001%
73	10.112	2719	2728	2737	rVB4	877	1601	0.11%	0.016%
74	10.575	2869	2872	2874	rBV	200	155	0.01%	0.002%
75	10.755	2915	2928	2946	rBV	524267	845602	57.61%	8.291%
76	10.883	2966	2968	2972	rVV2	276	165	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050476.D
 Acq On : 29 Aug 2022 11:44
 Operator : SY/MD
 Sample : VU0829WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.999	3001	3004	3008	rBV	306	208	0.01%	0.002%
78	11.060	3020	3023	3026	rBV2	215	169	0.01%	0.002%
79	11.092	3027	3033	3036	rVV2	457	537	0.04%	0.005%
80	11.147	3045	3050	3053	rBV2	273	303	0.02%	0.003%
81	11.314	3100	3102	3105	rBV2	213	139	0.01%	0.001%
82	11.340	3108	3110	3117	rVB2	286	220	0.01%	0.002%
83	11.401	3125	3129	3131	rBV	244	206	0.01%	0.002%
84	11.748	3232	3237	3239	rBV3	797	734	0.05%	0.007%
85	11.813	3244	3257	3281	rBV	389977	635527	43.29%	6.231%
86	12.192	3361	3375	3395	rBV	508355	836051	56.96%	8.197%
87	12.346	3420	3423	3428	rBV3	311	258	0.02%	0.003%
88	12.417	3442	3445	3446	rBV2	310	194	0.01%	0.002%
89	12.481	3461	3465	3469	rBV2	469	519	0.04%	0.005%
90	12.726	3539	3541	3543	rBV2	248	161	0.01%	0.002%
91	12.803	3561	3565	3567	rBV2	260	230	0.02%	0.002%
92	12.848	3577	3579	3582	rBV3	309	221	0.02%	0.002%
93	12.993	3622	3624	3627	rVB	317	140	0.01%	0.001%
94	13.015	3628	3631	3633	rBV2	252	151	0.01%	0.001%
95	13.394	3746	3749	3751	rBV3	411	284	0.02%	0.003%
96	13.578	3803	3806	3809	rBV2	327	236	0.02%	0.002%
97	13.848	3886	3890	3902	rVB5	1913	2214	0.15%	0.022%
98	14.095	3960	3967	3975	rBV3	3015	4392	0.30%	0.043%
99	14.333	4037	4041	4042	rBV3	1328	918	0.06%	0.009%
100	15.179	4302	4304	4308	rBV	613	392	0.03%	0.004%




Sum of corrected areas: 10199122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050476.D
Acq On : 29 Aug 2022 11:44
Operator : SY/MD
Sample : VU0829WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK171

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

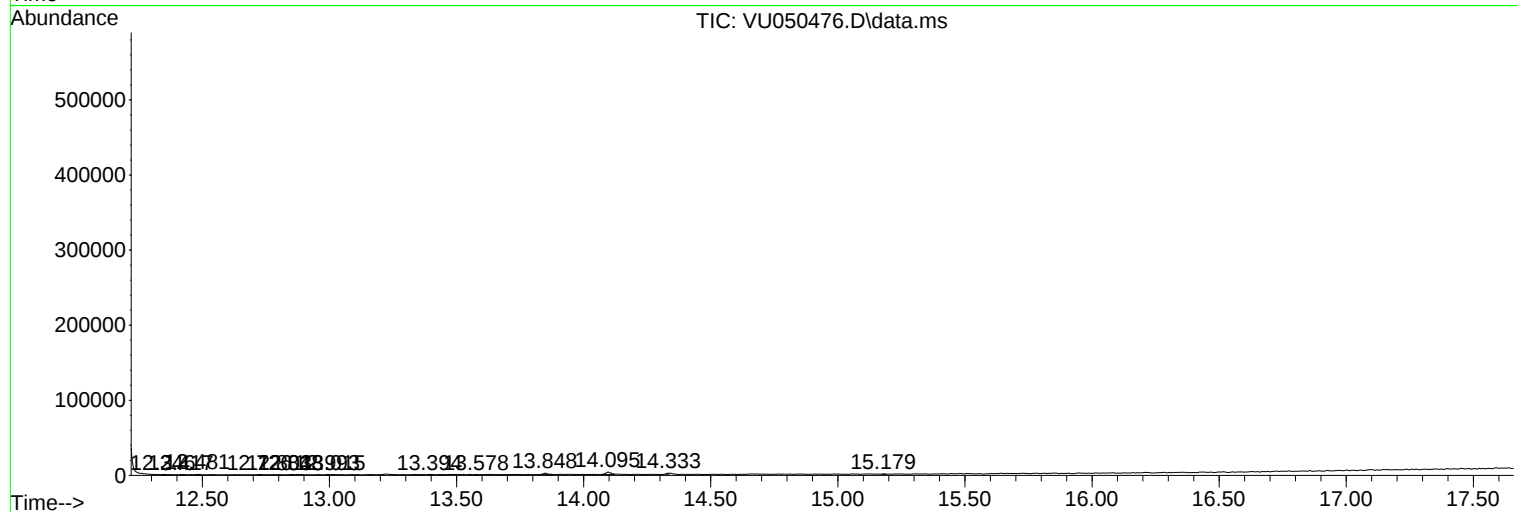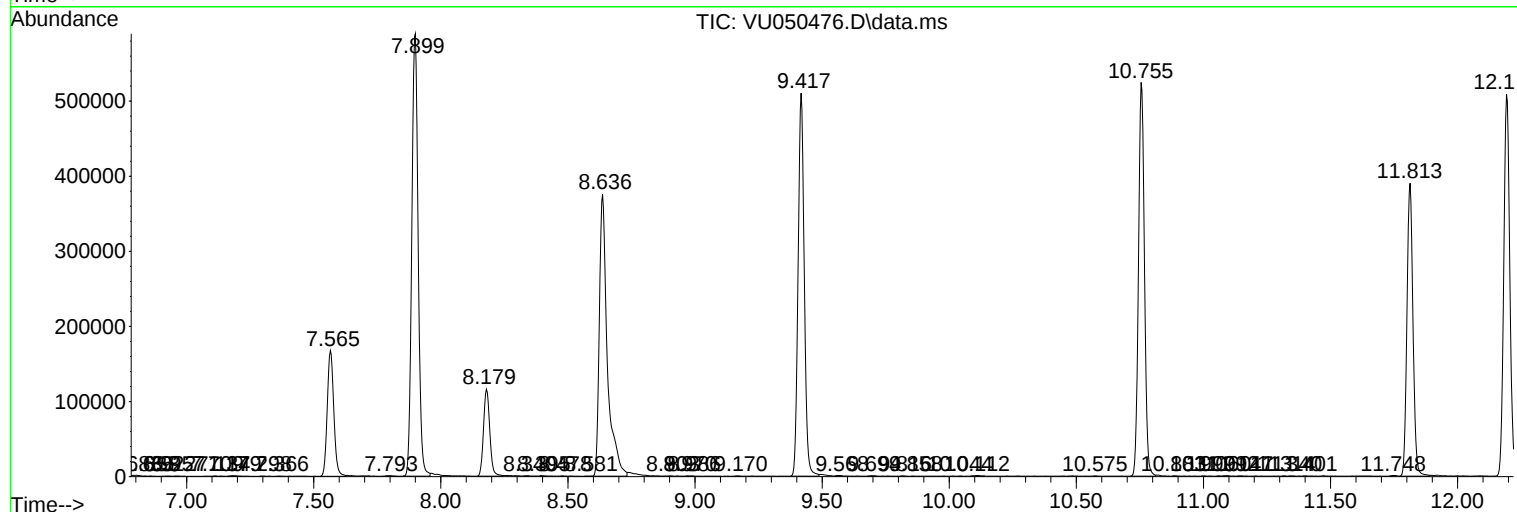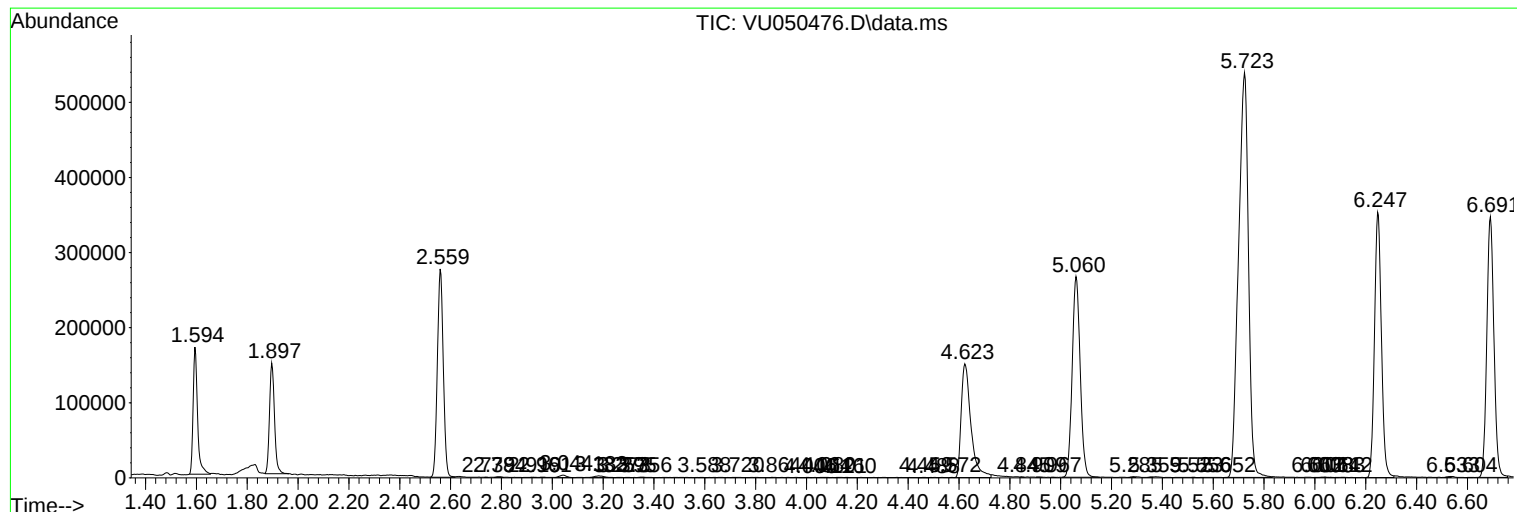

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050476.D
Acq On : 29 Aug 2022 11:44
Operator : SY/MD
Sample : VU0829WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK171

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050476.D
Acq On : 29 Aug 2022 11:44
Operator : SY/MD
Sample : VU0829WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK171

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc