

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050479.D
 Acq On : 29 Aug 2022 13:02
 Operator : SY/MD
 Sample : N4319-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rBV4	2899	3012	0.24%	0.035%
2	1.514	51	54	63	rVV2	2976	3518	0.28%	0.041%
3	1.594	72	79	98	rBV	156176	190825	15.38%	2.216%
4	1.903	166	175	195	rVB	128975	175526	14.15%	2.038%
5	2.562	365	380	394	rBV	246760	396271	31.94%	4.601%
6	2.777	445	447	450	rBV2	269	185	0.01%	0.002%
7	2.900	481	485	491	rBV	197	210	0.02%	0.002%
8	2.957	499	503	512	rVB2	556	741	0.06%	0.009%
9	3.041	521	529	538	rVB5	1770	3003	0.24%	0.035%
10	3.118	550	553	556	rBV2	269	222	0.02%	0.003%
11	3.134	556	558	563	rVV2	243	185	0.01%	0.002%
12	3.189	563	575	586	rVV4	1819	4215	0.34%	0.049%
13	3.356	623	627	633	rVB	349	280	0.02%	0.003%
14	3.404	637	642	645	rBV2	156	181	0.01%	0.002%
15	3.498	668	671	676	rVV2	311	275	0.02%	0.003%
16	3.636	707	714	717	rBV2	218	280	0.02%	0.003%
17	3.687	725	730	735	rVB2	365	369	0.03%	0.004%
18	3.726	739	742	748	rBV2	184	179	0.01%	0.002%
19	3.761	748	753	757	rVB2	277	262	0.02%	0.003%
20	3.993	822	825	833	rBV2	208	263	0.02%	0.003%
21	4.092	853	856	860	rBV2	213	190	0.02%	0.002%
22	4.395	947	950	954	rBV	278	256	0.02%	0.003%
23	4.472	970	974	977	rBV2	243	209	0.02%	0.002%
24	4.620	1008	1020	1042	rBV	158821	389065	31.36%	4.517%
25	4.970	1127	1129	1131	rBV	324	168	0.01%	0.002%
26	5.060	1141	1157	1175	rBV	233476	513391	41.38%	5.961%
27	5.215	1203	1205	1209	rBV2	373	302	0.02%	0.004%
28	5.240	1209	1213	1216	rVB2	377	327	0.03%	0.004%
29	5.289	1220	1228	1237	rVB5	1563	3076	0.25%	0.036%
30	5.375	1246	1255	1262	rBV3	897	1616	0.13%	0.019%
31	5.459	1275	1281	1289	rVB2	190	294	0.02%	0.003%
32	5.723	1341	1363	1396	rBV2	455138	1240629	100.00%	14.405%
33	5.893	1414	1416	1421	rVB	309	232	0.02%	0.003%
34	5.970	1435	1440	1443	rVV4	329	314	0.03%	0.004%
35	5.986	1443	1445	1449	rVB2	386	261	0.02%	0.003%
36	6.012	1449	1453	1455	rBV2	249	195	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050479.D
 Acq On : 29 Aug 2022 13:02
 Operator : SY/MD
 Sample : N4319-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.047	1462	1464	1468	rVB2	594	356	0.03%	0.004%
38	6.080	1472	1474	1478	rBV	219	190	0.02%	0.002%
39	6.173	1499	1503	1507	rBV	202	178	0.01%	0.002%
40	6.250	1512	1527	1547	rBV	285955	547267	44.11%	6.354%
41	6.526	1604	1613	1614	rBV4	753	736	0.06%	0.009%
42	6.539	1615	1617	1621	rVB4	1245	893	0.07%	0.010%
43	6.581	1626	1630	1632	rBV2	335	225	0.02%	0.003%
44	6.690	1649	1664	1692	rVV	298061	572514	46.15%	6.647%
45	6.797	1692	1697	1701	rBV5	763	781	0.06%	0.009%
46	6.845	1709	1712	1713	rBV	285	179	0.01%	0.002%
47	6.887	1722	1725	1727	rBV3	256	169	0.01%	0.002%
48	6.899	1727	1729	1735	rVB3	441	267	0.02%	0.003%
49	6.967	1747	1750	1755	rVB2	242	180	0.01%	0.002%
50	7.186	1810	1818	1821	rBV3	437	675	0.05%	0.008%
51	7.288	1848	1850	1852	rBV	244	175	0.01%	0.002%
52	7.565	1923	1936	1960	rVV	137356	243304	19.61%	2.825%
53	7.687	1971	1974	1976	rBV	350	254	0.02%	0.003%
54	7.793	1999	2007	2018	rBV5	1942	3261	0.26%	0.038%
55	7.899	2026	2040	2062	rBV	483185	846083	68.20%	9.824%
56	8.179	2115	2127	2148	rBV2	92724	159487	12.86%	1.852%
57	8.388	2188	2192	2198	rBV	330	484	0.04%	0.006%
58	8.536	2236	2238	2243	rVB2	259	191	0.02%	0.002%
59	8.636	2256	2269	2304	rBV4	349117	781176	62.97%	9.070%
60	8.787	2309	2316	2326	rVB4	7850	14235	1.15%	0.165%
61	8.893	2347	2349	2355	rVB2	323	223	0.02%	0.003%
62	8.941	2360	2364	2365	rBV	313	202	0.02%	0.002%
63	8.980	2371	2376	2378	rBV	260	216	0.02%	0.003%
64	9.015	2384	2387	2390	rBV3	316	223	0.02%	0.003%
65	9.163	2431	2433	2436	rVB	342	212	0.02%	0.002%
66	9.189	2436	2441	2444	rVB2	261	251	0.02%	0.003%
67	9.311	2476	2479	2486	rVV2	329	315	0.03%	0.004%
68	9.417	2499	2512	2549	rVV	397922	670193	54.02%	7.782%
69	9.562	2554	2557	2558	rBV3	283	168	0.01%	0.002%
70	9.767	2617	2621	2622	rBV	269	173	0.01%	0.002%
71	9.845	2640	2645	2647	rBV2	220	193	0.02%	0.002%
72	9.964	2677	2682	2690	rBV2	820	1238	0.10%	0.014%
73	10.086	2708	2720	2726	rBV3	1685	2764	0.22%	0.032%
74	10.343	2798	2800	2806	rVB2	382	240	0.02%	0.003%
75	10.488	2840	2845	2848	rVV2	432	404	0.03%	0.005%
76	10.510	2849	2852	2855	rVB2	271	175	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050479.D
 Acq On : 29 Aug 2022 13:02
 Operator : SY/MD
 Sample : N4319-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.603	2877	2881	2884	rBV2	229	221	0.02%	0.003%
78	10.755	2912	2928	2951	rBV	440234	713218	57.49%	8.281%
79	11.118	3037	3041	3044	rBV2	314	288	0.02%	0.003%
80	11.488	3152	3156	3163	rVB5	769	1057	0.09%	0.012%
81	11.520	3163	3166	3169	rBV	240	183	0.01%	0.002%
82	11.665	3205	3211	3214	rBV	477	668	0.05%	0.008%
83	11.812	3244	3257	3282	rBV	290991	467238	37.66%	5.425%
84	11.922	3289	3291	3294	rVB4	355	179	0.01%	0.002%
85	12.031	3322	3325	3329	rBV	309	258	0.02%	0.003%
86	12.073	3331	3338	3349	rVV5	1650	2749	0.22%	0.032%
87	12.192	3359	3375	3398	rBV	386053	636502	51.30%	7.390%
88	12.488	3463	3467	3468	rBV2	323	201	0.02%	0.002%
89	12.545	3481	3485	3488	rBV	339	358	0.03%	0.004%
90	12.581	3493	3496	3499	rBV3	372	290	0.02%	0.003%
91	12.703	3530	3534	3535	rBV	428	317	0.03%	0.004%
92	12.864	3581	3584	3591	rVB4	549	457	0.04%	0.005%
93	12.906	3594	3597	3600	rBV3	340	234	0.02%	0.003%
94	13.089	3651	3654	3655	rBV	424	205	0.02%	0.002%
95	13.221	3690	3695	3708	rVB4	966	1643	0.13%	0.019%
96	13.272	3708	3711	3715	rBV2	438	318	0.03%	0.004%
97	13.378	3741	3744	3747	rBV3	389	274	0.02%	0.003%
98	13.825	3879	3883	3884	rBV3	560	361	0.03%	0.004%
99	13.854	3884	3892	3903	rVB4	1173	2183	0.18%	0.025%
100	14.336	4034	4042	4050	rBV5	1245	2153	0.17%	0.025%




Sum of corrected areas: 8612532

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050479.D
Acq On : 29 Aug 2022 13:02
Operator : SY/MD
Sample : N4319-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

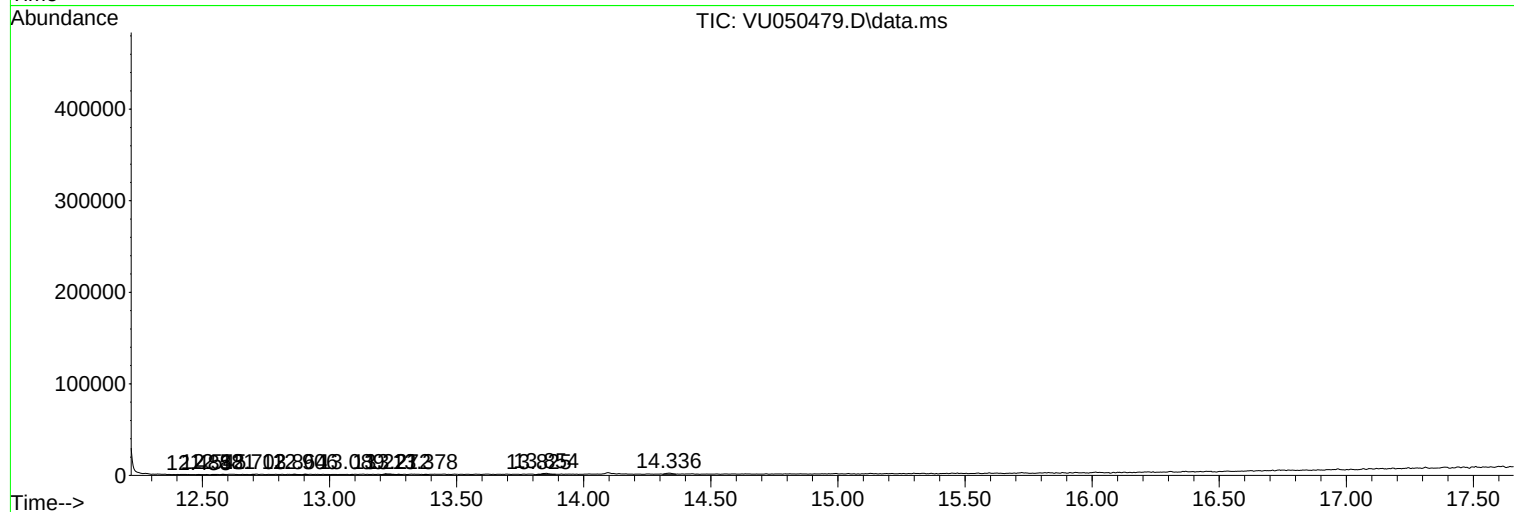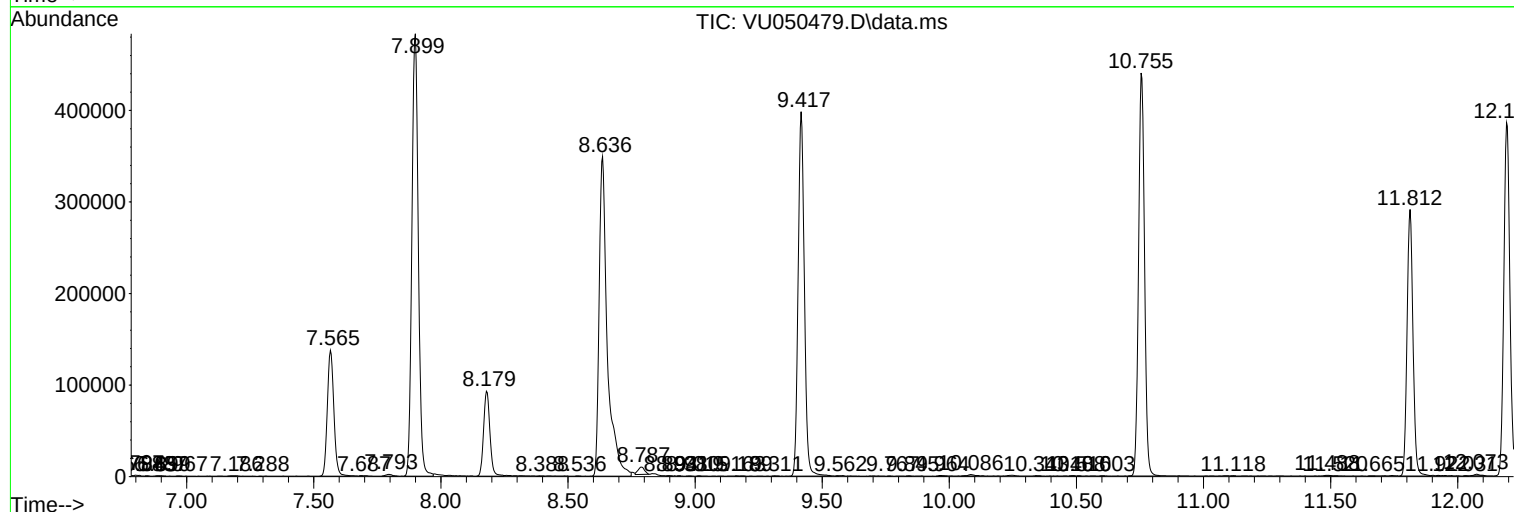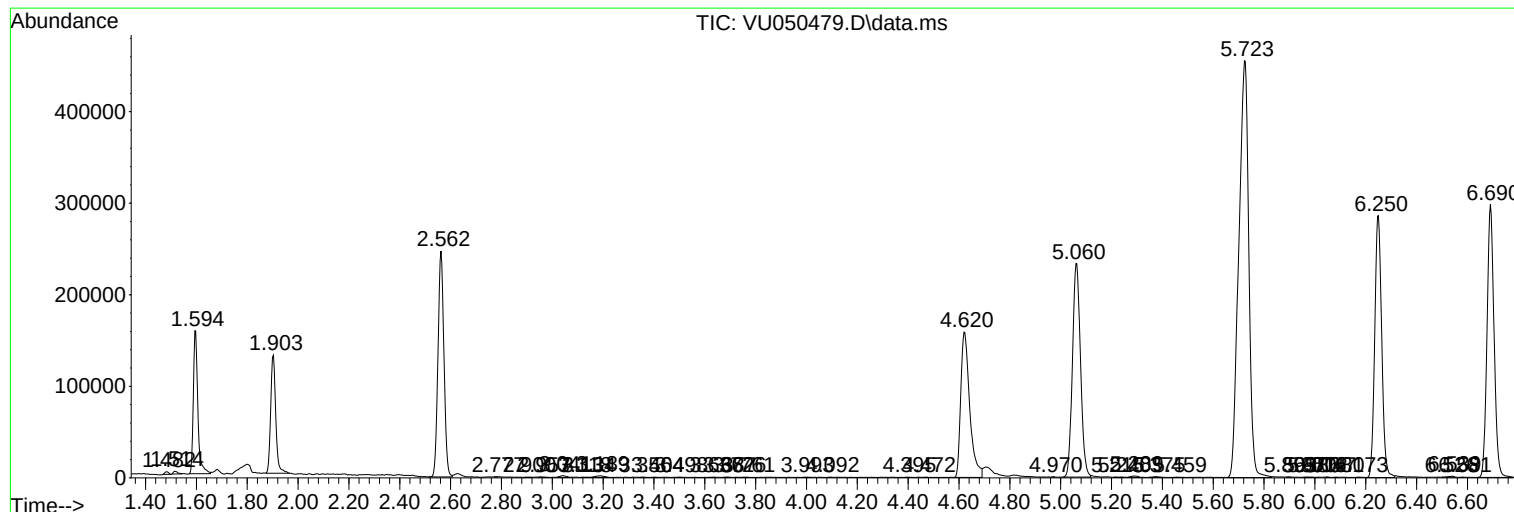

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050479.D
Acq On : 29 Aug 2022 13:02
Operator : SY/MD
Sample : N4319-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050479.D
Acq On : 29 Aug 2022 13:02
Operator : SY/MD
Sample : N4319-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
