

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050480.D
 Acq On : 29 Aug 2022 13:26
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	100	rBV	129107	160860	16.76%	2.377%
2	1.893	164	172	187	rVB	101561	137131	14.28%	2.026%
3	2.559	367	379	393	rBV	204771	329181	34.29%	4.864%
4	2.626	394	400	413	rVB2	7514	12960	1.35%	0.192%
5	2.893	475	483	494	rBV4	2026	4165	0.43%	0.062%
6	2.951	499	501	506	rVB2	370	197	0.02%	0.003%
7	3.038	521	528	537	rBV5	1723	2795	0.29%	0.041%
8	3.176	562	571	578	rBV4	689	1246	0.13%	0.018%
9	3.260	593	597	608	rBV2	467	771	0.08%	0.011%
10	3.353	622	626	631	rVB2	341	312	0.03%	0.005%
11	3.401	636	641	643	rBV2	205	165	0.02%	0.002%
12	3.485	664	667	675	rVB2	260	321	0.03%	0.005%
13	3.597	699	702	704	rBV	344	265	0.03%	0.004%
14	3.678	721	727	728	rVV2	239	213	0.02%	0.003%
15	3.684	728	729	734	rVV2	408	288	0.03%	0.004%
16	3.784	753	760	764	rVB2	181	234	0.02%	0.003%
17	3.922	798	803	805	rBV	323	239	0.02%	0.004%
18	3.948	805	811	817	rVV	684	700	0.07%	0.010%
19	4.102	857	859	865	rVB2	211	185	0.02%	0.003%
20	4.189	882	886	889	rBV2	301	219	0.02%	0.003%
21	4.324	926	928	934	rVB2	206	162	0.02%	0.002%
22	4.411	952	955	960	rBV	194	168	0.02%	0.002%
23	4.488	975	979	984	rVB2	268	221	0.02%	0.003%
24	4.533	984	993	997	rBV2	193	282	0.03%	0.004%
25	4.559	997	1001	1003	rBV	242	174	0.02%	0.003%
26	4.623	1008	1021	1046	rBV	137756	344354	35.87%	5.088%
27	4.896	1102	1106	1107	rBV	269	187	0.02%	0.003%
28	4.993	1132	1136	1140	rBV3	290	267	0.03%	0.004%
29	5.060	1141	1157	1183	rVV	175597	386733	40.28%	5.715%
30	5.205	1198	1202	1208	rBV3	443	428	0.04%	0.006%
31	5.292	1218	1229	1237	rVB5	1201	2344	0.24%	0.035%
32	5.327	1237	1240	1245	rBV2	224	179	0.02%	0.003%
33	5.369	1245	1253	1256	rBV3	633	821	0.09%	0.012%
34	5.491	1286	1291	1296	rBV	229	302	0.03%	0.004%
35	5.723	1341	1363	1391	rBV2	356262	960022	100.00%	14.186%
36	5.861	1403	1406	1409	rBV3	209	151	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050480.D
 Acq On : 29 Aug 2022 13:26
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	5.977	1436	1442	1451	rVB3	479	642	0.07%	0.009%
38	6.163	1495	1500	1504	rBV3	377	393	0.04%	0.006%
39	6.247	1513	1526	1549	rBV	232925	441965	46.04%	6.531%
40	6.456	1588	1591	1592	rBV	280	174	0.02%	0.003%
41	6.526	1609	1613	1614	rVV2	698	450	0.05%	0.007%
42	6.536	1614	1616	1623	rVB2	1309	1038	0.11%	0.015%
43	6.690	1649	1664	1686	rBV	224648	440074	45.84%	6.503%
44	6.803	1697	1699	1701	rBV2	275	177	0.02%	0.003%
45	7.160	1805	1810	1811	rBV	494	338	0.04%	0.005%
46	7.179	1812	1816	1817	rVV3	436	293	0.03%	0.004%
47	7.260	1838	1841	1845	rVV2	220	193	0.02%	0.003%
48	7.337	1863	1865	1875	rVB2	250	266	0.03%	0.004%
49	7.388	1875	1881	1883	rBV	186	206	0.02%	0.003%
50	7.481	1907	1910	1914	rBV2	296	205	0.02%	0.003%
51	7.565	1923	1936	1952	rBV	102167	181565	18.91%	2.683%
52	7.694	1973	1976	1978	rBV2	395	283	0.03%	0.004%
53	7.806	2009	2011	2014	rVB2	365	207	0.02%	0.003%
54	7.832	2016	2019	2022	rBV	320	207	0.02%	0.003%
55	7.899	2027	2040	2056	rBV	365590	638532	66.51%	9.435%
56	8.179	2114	2127	2142	rBV	70049	118142	12.31%	1.746%
57	8.472	2215	2218	2222	rVB2	516	431	0.04%	0.006%
58	8.501	2222	2227	2230	rBV2	195	205	0.02%	0.003%
59	8.636	2255	2269	2297	rBV3	296175	665728	69.35%	9.837%
60	8.906	2348	2353	2356	rBV3	199	187	0.02%	0.003%
61	9.417	2499	2512	2531	rBV	310481	517205	53.87%	7.643%
62	9.549	2551	2553	2556	rVB3	335	188	0.02%	0.003%
63	9.690	2588	2597	2603	rBV3	503	894	0.09%	0.013%
64	9.745	2610	2614	2617	rBV2	331	257	0.03%	0.004%
65	9.803	2629	2632	2635	rBV	257	155	0.02%	0.002%
66	9.948	2671	2677	2680	rVV2	226	249	0.03%	0.004%
67	9.983	2685	2688	2694	rBV	182	161	0.02%	0.002%
68	10.041	2702	2706	2709	rBV	223	184	0.02%	0.003%
69	10.166	2743	2745	2753	rVB	291	232	0.02%	0.003%
70	10.211	2754	2759	2762	rVB2	218	209	0.02%	0.003%
71	10.353	2800	2803	2808	rBV2	418	300	0.03%	0.004%
72	10.436	2826	2829	2834	rBV	237	267	0.03%	0.004%
73	10.465	2835	2838	2841	rVV2	230	165	0.02%	0.002%
74	10.597	2874	2879	2881	rBV2	268	218	0.02%	0.003%
75	10.703	2907	2912	2914	rBV	227	195	0.02%	0.003%
76	10.755	2915	2928	2955	rVV	348606	570053	59.38%	8.423%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050480.D
 Acq On : 29 Aug 2022 13:26
 Operator : SY/MD
 Sample : N4399-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.893	2966	2971	2975	rVB3	301	317	0.03%	0.005%
78	10.915	2975	2978	2980	rBV2	240	174	0.02%	0.003%
79	11.089	3030	3032	3036	rVB2	271	156	0.02%	0.002%
80	11.266	3084	3087	3090	rBV	232	154	0.02%	0.002%
81	11.285	3091	3093	3097	rVB	289	169	0.02%	0.002%
82	11.427	3135	3137	3145	rBV2	140	212	0.02%	0.003%
83	11.549	3171	3175	3179	rVB2	353	254	0.03%	0.004%
84	11.732	3227	3232	3234	rBV2	391	404	0.04%	0.006%
85	11.812	3245	3257	3278	rBV	215785	346756	36.12%	5.124%
86	11.954	3299	3301	3304	rVB	303	188	0.02%	0.003%
87	11.973	3304	3307	3313	rVB2	354	281	0.03%	0.004%
88	12.037	3324	3327	3329	rBV2	256	179	0.02%	0.003%
89	12.070	3329	3337	3351	rVV5	3156	6403	0.67%	0.095%
90	12.195	3362	3376	3395	rBV	282263	476586	49.64%	7.042%
91	12.369	3429	3430	3435	rBV2	229	167	0.02%	0.002%
92	12.571	3489	3493	3495	rBV2	366	272	0.03%	0.004%
93	12.607	3501	3504	3508	rBV2	232	208	0.02%	0.003%
94	12.671	3519	3524	3527	rBV2	235	225	0.02%	0.003%
95	12.722	3538	3540	3544	rVB2	323	218	0.02%	0.003%
96	12.835	3571	3575	3577	rBV	712	557	0.06%	0.008%
97	13.144	3668	3671	3678	rVB3	462	436	0.05%	0.006%
98	13.227	3694	3697	3701	rVB3	553	343	0.04%	0.005%
99	13.687	3838	3840	3842	rBV2	275	177	0.02%	0.003%
100	14.237	4009	4011	4017	rBV3	449	503	0.05%	0.007%




Sum of corrected areas: 6767414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050480.D
Acq On : 29 Aug 2022 13:26
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

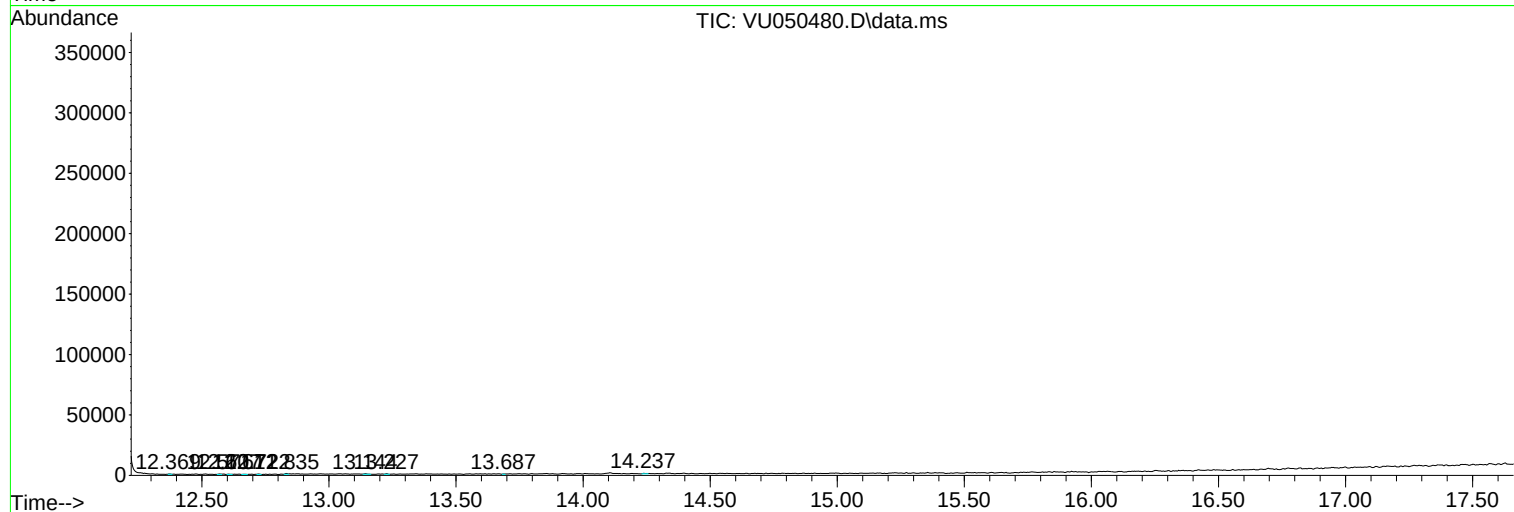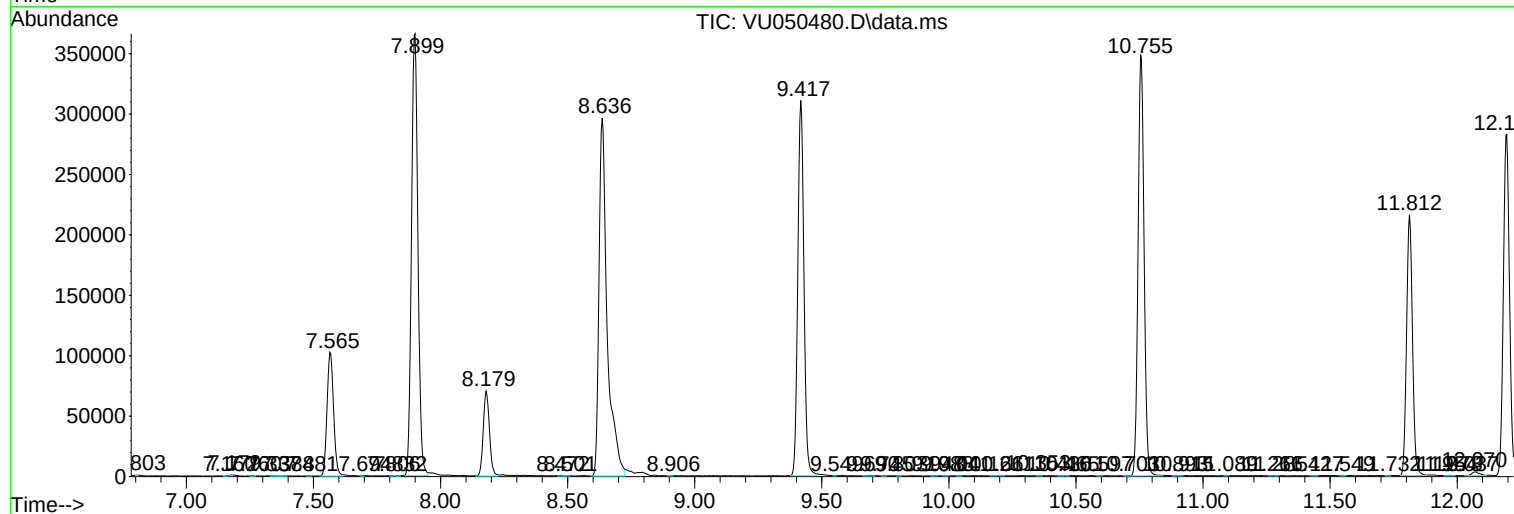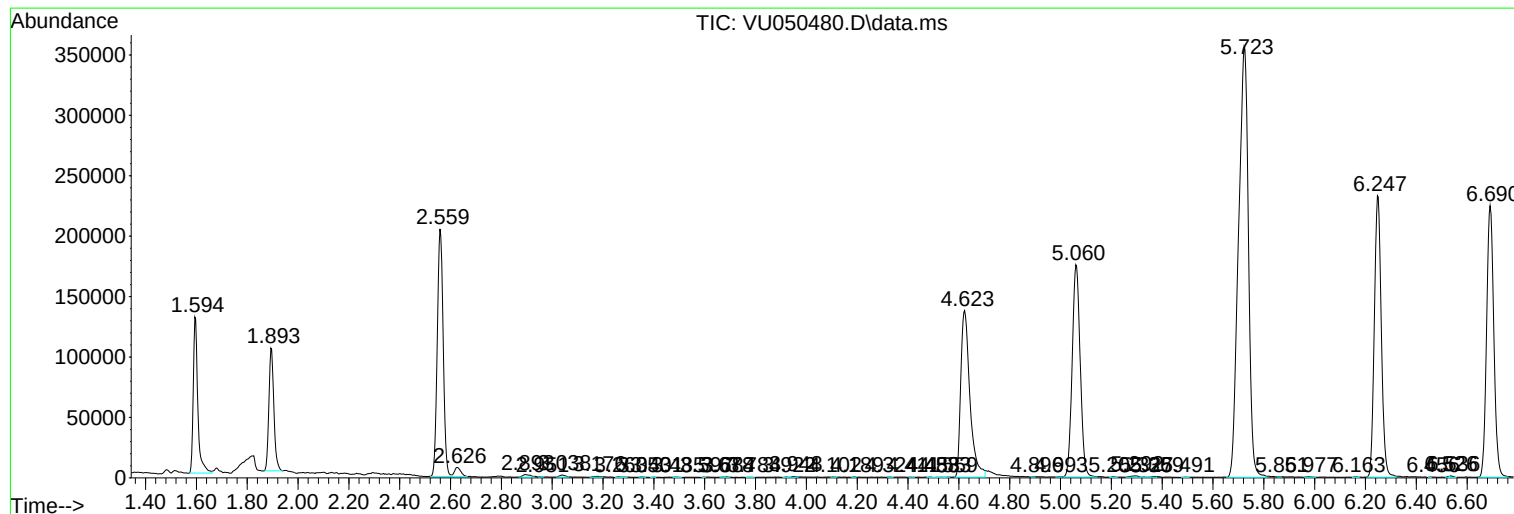

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050480.D
Acq On : 29 Aug 2022 13:26
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050480.D
Acq On : 29 Aug 2022 13:26
Operator : SY/MD
Sample : N4399-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------