

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050482.D
 Acq On : 29 Aug 2022 14:13
 Operator : SY/MD
 Sample : N4322-23DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rBV	166304	203778	13.50%	1.883%
2	1.903	167	175	195	rVB	153162	205900	13.64%	1.903%
3	2.562	368	380	398	rBV	264725	426640	28.26%	3.943%
4	2.784	445	449	451	rBV3	584	414	0.03%	0.004%
5	2.796	451	453	457	rVB3	360	247	0.02%	0.002%
6	2.890	479	482	485	rBV	220	152	0.01%	0.001%
7	2.909	485	488	491	rBV2	257	213	0.01%	0.002%
8	3.044	520	530	541	rBV4	4827	8919	0.59%	0.082%
9	3.112	548	551	557	rVB	363	246	0.02%	0.002%
10	3.182	562	573	594	rBV2	6553	14480	0.96%	0.134%
11	3.356	617	627	635	rVB4	1433	2710	0.18%	0.025%
12	3.475	662	664	666	rVV	307	144	0.01%	0.001%
13	3.600	700	703	705	rBV	191	119	0.01%	0.001%
14	3.681	725	728	731	rBV2	182	155	0.01%	0.001%
15	3.825	767	773	775	rBV2	179	185	0.01%	0.002%
16	3.874	775	788	802	rVB3	4782	10271	0.68%	0.095%
17	4.031	833	837	841	rVB2	226	173	0.01%	0.002%
18	4.095	849	857	860	rBV2	197	247	0.02%	0.002%
19	4.163	875	878	882	rVB2	168	129	0.01%	0.001%
20	4.189	882	886	890	rBV2	182	160	0.01%	0.001%
21	4.211	890	893	897	rVB2	273	172	0.01%	0.002%
22	4.414	952	956	960	rBV2	272	263	0.02%	0.002%
23	4.475	972	975	978	rVB	200	122	0.01%	0.001%
24	4.533	991	993	997	rBV2	147	119	0.01%	0.001%
25	4.629	1009	1023	1068	rBV	158088	451454	29.90%	4.172%
26	5.063	1141	1158	1180	rBV	275282	606275	40.16%	5.603%
27	5.192	1196	1198	1199	rBV	295	108	0.01%	0.001%
28	5.295	1221	1230	1231	rBV3	1653	1964	0.13%	0.018%
29	5.369	1248	1253	1265	rVB3	887	1459	0.10%	0.013%
30	5.491	1288	1291	1294	rVB	381	258	0.02%	0.002%
31	5.513	1294	1298	1306	rVB2	167	191	0.01%	0.002%
32	5.552	1306	1310	1317	rBV2	179	209	0.01%	0.002%
33	5.607	1324	1327	1332	rBV2	154	131	0.01%	0.001%
34	5.726	1342	1364	1399	rBV2	561152	1509778	100.00%	13.953%
35	5.976	1440	1442	1445	rVV4	374	205	0.01%	0.002%
36	5.996	1445	1448	1449	rVV	199	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050482.D
 Acq On : 29 Aug 2022 14:13
 Operator : SY/MD
 Sample : N4322-23DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.009	1450	1452	1457	rVV	351	211	0.01%	0.002%
38	6.034	1457	1460	1463	rVV2	245	177	0.01%	0.002%
39	6.063	1467	1469	1475	rVB2	323	255	0.02%	0.002%
40	6.169	1500	1502	1507	rVB2	303	215	0.01%	0.002%
41	6.195	1507	1510	1511	rBV	301	188	0.01%	0.002%
42	6.250	1513	1527	1557	rVV	357993	690928	45.76%	6.385%
43	6.385	1567	1569	1572	rVV3	393	249	0.02%	0.002%
44	6.401	1572	1574	1576	rVB	283	121	0.01%	0.001%
45	6.542	1604	1618	1646	rBV	234190	440245	29.16%	4.069%
46	6.690	1650	1664	1694	rVV	361953	709536	47.00%	6.557%
47	6.809	1695	1701	1712	rVB4	1055	1395	0.09%	0.013%
48	6.880	1720	1723	1725	rVB2	297	148	0.01%	0.001%
49	6.899	1725	1729	1733	rBV2	235	216	0.01%	0.002%
50	7.057	1773	1778	1781	rBV2	376	288	0.02%	0.003%
51	7.118	1793	1797	1800	rBV2	328	269	0.02%	0.002%
52	7.134	1800	1802	1805	rVB2	175	114	0.01%	0.001%
53	7.189	1813	1819	1820	rBV2	813	751	0.05%	0.007%
54	7.230	1829	1832	1837	rBV2	315	254	0.02%	0.002%
55	7.308	1853	1856	1858	rBV	257	144	0.01%	0.001%
56	7.324	1858	1861	1863	rBV2	213	168	0.01%	0.002%
57	7.369	1872	1875	1882	rVB2	198	234	0.02%	0.002%
58	7.410	1884	1888	1893	rVB2	297	269	0.02%	0.002%
59	7.436	1893	1896	1898	rBV	231	151	0.01%	0.001%
60	7.565	1924	1936	1958	rBV	172495	303407	20.10%	2.804%
61	7.816	2012	2014	2018	rVB	227	140	0.01%	0.001%
62	7.899	2023	2040	2065	rBV	601176	1047457	69.38%	9.680%
63	8.025	2076	2079	2085	rVB4	577	538	0.04%	0.005%
64	8.179	2116	2127	2143	rBV	114249	195557	12.95%	1.807%
65	8.475	2216	2219	2220	rBV2	342	193	0.01%	0.002%
66	8.523	2230	2234	2238	rVB2	320	199	0.01%	0.002%
67	8.639	2257	2270	2314	rBV2	380163	876535	58.06%	8.101%
68	8.915	2354	2356	2360	rBV	245	158	0.01%	0.001%
69	8.976	2370	2375	2377	rBV2	623	532	0.04%	0.005%
70	9.163	2430	2433	2440	rBV3	240	229	0.02%	0.002%
71	9.417	2499	2512	2535	rBV	513538	860800	57.02%	7.955%
72	9.658	2584	2587	2590	rBV2	291	242	0.02%	0.002%
73	9.745	2611	2614	2616	rBV2	217	169	0.01%	0.002%
74	9.783	2623	2626	2634	rVB2	305	270	0.02%	0.002%
75	10.082	2716	2719	2721	rBV2	350	214	0.01%	0.002%
76	10.098	2722	2724	2730	rVB3	345	324	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050482.D
 Acq On : 29 Aug 2022 14:13
 Operator : SY/MD
 Sample : N4322-23DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY178DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.176	2743	2748	2751	rBV2	354	311	0.02%	0.003%
78	10.198	2753	2755	2756	rVV	289	115	0.01%	0.001%
79	10.211	2757	2759	2762	rVB2	299	117	0.01%	0.001%
80	10.240	2763	2768	2772	rBV2	268	288	0.02%	0.003%
81	10.417	2821	2823	2826	rVB2	194	104	0.01%	0.001%
82	10.439	2826	2830	2833	rBV	302	254	0.02%	0.002%
83	10.606	2878	2882	2887	rBV	321	404	0.03%	0.004%
84	10.758	2915	2929	2950	rBV	514381	839076	55.58%	7.754%
85	10.870	2961	2964	2966	rBV2	294	172	0.01%	0.002%
86	10.986	2997	3000	3003	rBV	268	171	0.01%	0.002%
87	11.250	3079	3082	3087	rVB	282	252	0.02%	0.002%
88	11.282	3088	3092	3095	rBV	317	297	0.02%	0.003%
89	11.500	3155	3160	3163	rBV2	205	229	0.02%	0.002%
90	11.594	3187	3189	3193	rBV2	221	106	0.01%	0.001%
91	11.812	3245	3257	3281	rBV	372778	600416	39.77%	5.549%
92	12.018	3319	3321	3323	rBV2	288	165	0.01%	0.002%
93	12.095	3343	3345	3348	rBV2	296	203	0.01%	0.002%
94	12.195	3362	3376	3399	rBV	475104	793738	52.57%	7.335%
95	12.417	3443	3445	3448	rBV2	269	191	0.01%	0.002%
96	12.455	3454	3457	3460	rBV3	415	329	0.02%	0.003%
97	13.076	3646	3650	3656	rBV3	432	624	0.04%	0.006%
98	13.169	3677	3679	3682	rBV2	336	198	0.01%	0.002%
99	14.944	4228	4231	4233	rBV2	647	381	0.03%	0.004%
100	15.545	4413	4418	4422	rBV5	716	856	0.06%	0.008%




Sum of corrected areas: 10820588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050482.D
Acq On : 29 Aug 2022 14:13
Operator : SY/MD
Sample : N4322-23DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

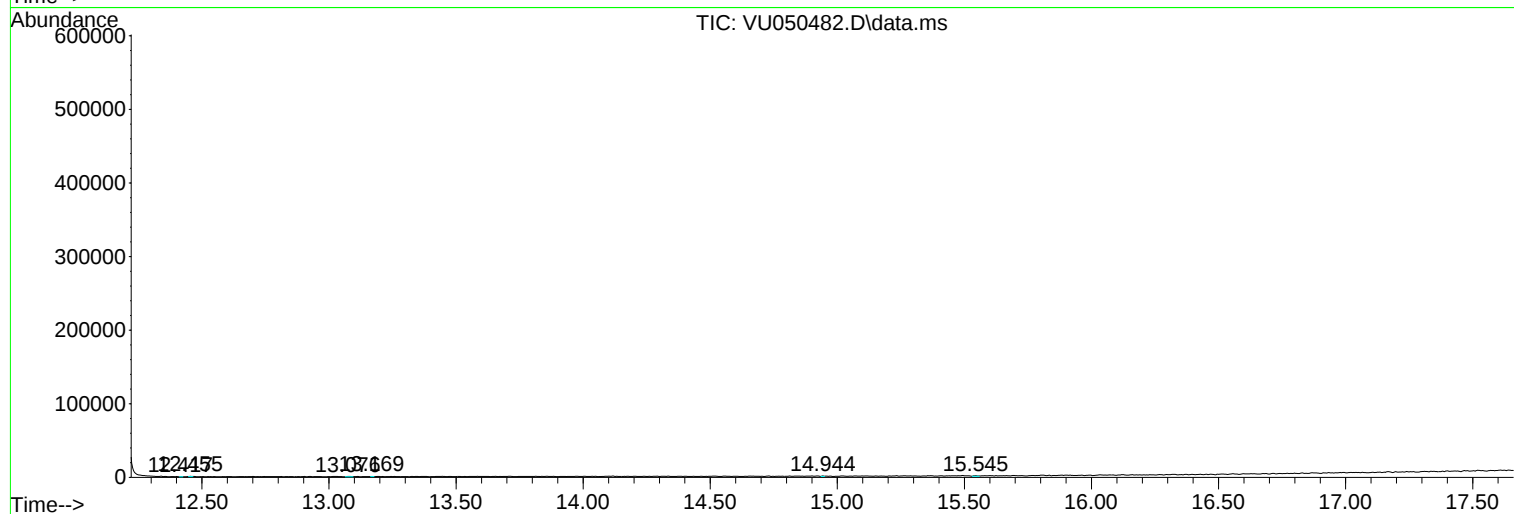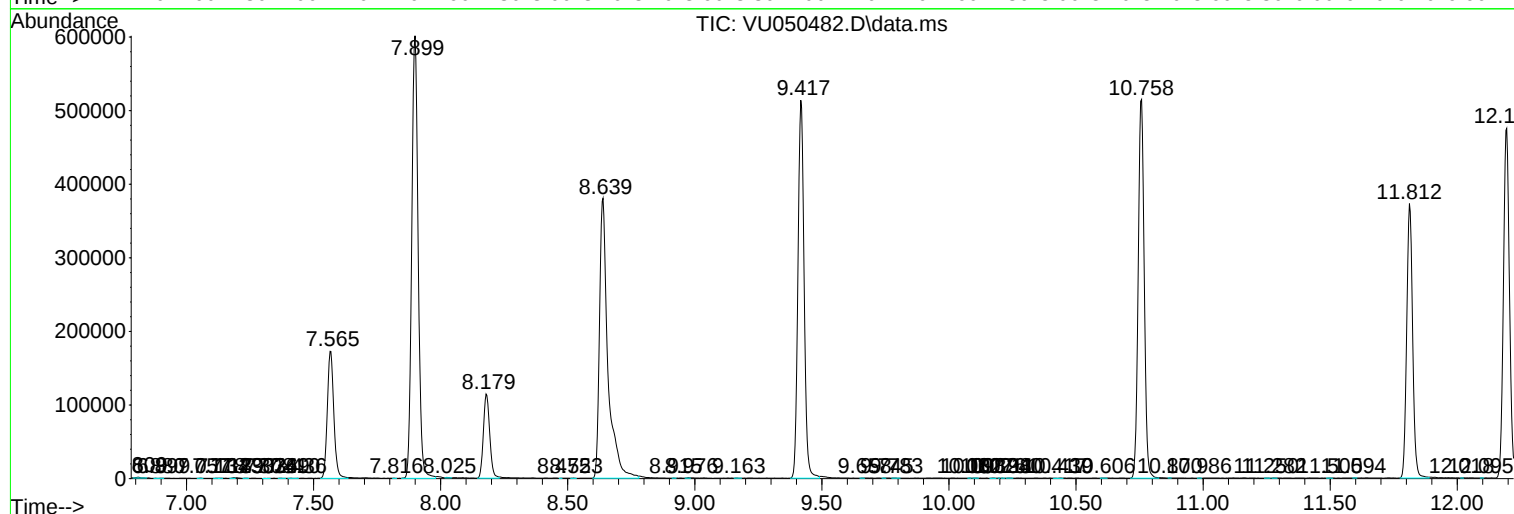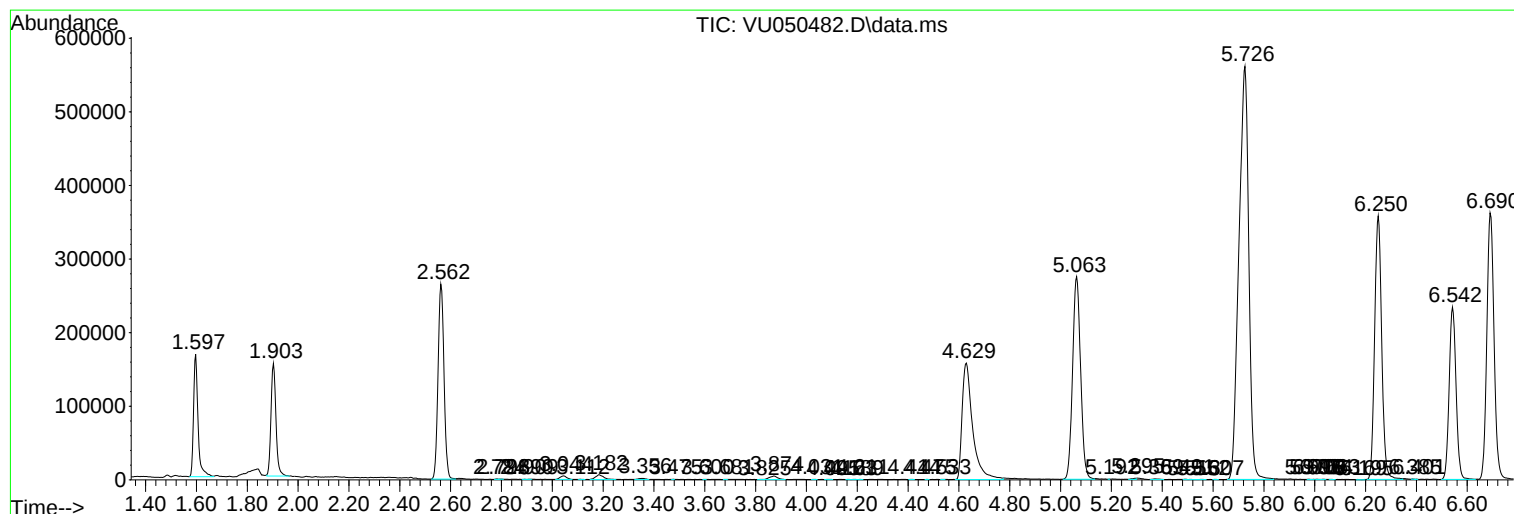

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050482.D
Acq On : 29 Aug 2022 14:13
Operator : SY/MD
Sample : N4322-23DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050482.D
Acq On : 29 Aug 2022 14:13
Operator : SY/MD
Sample : N4322-23DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY178DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc