

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050483.D
 Acq On : 29 Aug 2022 14:37
 Operator : SY/MD
 Sample : N4322-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY179

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	3440	3558	0.28%	0.040%
2	1.597	72	80	100	rBV	159263	193763	15.07%	2.167%
3	1.903	166	175	195	rVB	135920	184932	14.38%	2.068%
4	2.562	368	380	395	rBV	251910	403147	31.35%	4.509%
5	2.787	438	450	467	rBV4	5164	15753	1.23%	0.176%
6	2.951	498	501	506	rVB3	296	228	0.02%	0.003%
7	3.041	522	529	532	rBV4	1783	2249	0.17%	0.025%
8	3.186	564	574	589	rVB3	2564	5910	0.46%	0.066%
9	3.427	645	649	654	rBV2	195	241	0.02%	0.003%
10	3.469	659	662	669	rVB2	227	204	0.02%	0.002%
11	3.851	779	781	786	rVV	261	187	0.01%	0.002%
12	3.915	798	801	806	rVB	304	254	0.02%	0.003%
13	4.028	831	836	840	rBV2	158	170	0.01%	0.002%
14	4.054	840	844	847	rBV	254	216	0.02%	0.002%
15	4.112	852	862	865	rBV2	275	439	0.03%	0.005%
16	4.292	909	918	922	rBV2	304	466	0.04%	0.005%
17	4.494	976	981	984	rBV2	194	191	0.01%	0.002%
18	4.568	997	1004	1006	rBV	230	269	0.02%	0.003%
19	4.629	1009	1023	1061	rBV	145833	397687	30.93%	4.448%
20	4.890	1102	1104	1107	rBV3	421	219	0.02%	0.002%
21	5.063	1141	1158	1187	rBV2	244161	595533	46.31%	6.661%
22	5.279	1218	1225	1226	rBV3	931	769	0.06%	0.009%
23	5.333	1239	1242	1246	rVB2	227	185	0.01%	0.002%
24	5.369	1249	1253	1264	rVB2	896	1382	0.11%	0.015%
25	5.565	1310	1314	1319	rVB2	216	204	0.02%	0.002%
26	5.642	1333	1338	1342	rBV2	195	225	0.02%	0.003%
27	5.726	1342	1364	1388	rBV2	474472	1285946	100.00%	14.383%
28	5.983	1441	1444	1449	rVB3	397	316	0.02%	0.004%
29	6.041	1459	1462	1465	rBV2	334	264	0.02%	0.003%
30	6.073	1470	1472	1478	rVB	271	176	0.01%	0.002%
31	6.112	1478	1484	1485	rBV2	285	260	0.02%	0.003%
32	6.250	1511	1527	1554	rBV	314624	600251	46.68%	6.714%
33	6.404	1572	1575	1579	rVB	271	198	0.02%	0.002%
34	6.439	1584	1586	1590	rBV	257	240	0.02%	0.003%
35	6.539	1607	1617	1628	rBV10	3069	6493	0.50%	0.073%
36	6.690	1650	1664	1692	rBV	308048	596480	46.38%	6.672%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050483.D
 Acq On : 29 Aug 2022 14:37
 Operator : SY/MD
 Sample : N4322-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY179

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.796	1694	1697	1698	rBV2	478	246	0.02%	0.003%
38	6.838	1708	1710	1715	rVB2	322	258	0.02%	0.003%
39	6.944	1734	1743	1745	rBV2	182	203	0.02%	0.002%
40	6.960	1745	1748	1754	rVB	190	172	0.01%	0.002%
41	7.063	1777	1780	1786	rVB	214	187	0.01%	0.002%
42	7.182	1811	1817	1822	rBV4	767	1005	0.08%	0.011%
43	7.243	1830	1836	1839	rBV2	229	225	0.02%	0.003%
44	7.279	1843	1847	1852	rVB	292	241	0.02%	0.003%
45	7.317	1852	1859	1864	rBV2	221	305	0.02%	0.003%
46	7.346	1864	1868	1871	rBV2	186	169	0.01%	0.002%
47	7.414	1885	1889	1895	rVB2	222	235	0.02%	0.003%
48	7.565	1924	1936	1960	rBV	137928	249320	19.39%	2.789%
49	7.764	1994	1998	2002	rVB2	298	225	0.02%	0.003%
50	7.809	2009	2012	2017	rBV3	345	299	0.02%	0.003%
51	7.899	2025	2040	2070	rBV	499435	870771	67.71%	9.739%
52	8.105	2101	2104	2109	rVB2	358	325	0.03%	0.004%
53	8.179	2116	2127	2145	rBV	96815	163696	12.73%	1.831%
54	8.279	2155	2158	2161	rBV3	606	522	0.04%	0.006%
55	8.401	2192	2196	2197	rBV3	315	192	0.01%	0.002%
56	8.443	2206	2209	2213	rVB3	380	296	0.02%	0.003%
57	8.636	2256	2269	2301	rBV2	343226	782845	60.88%	8.756%
58	8.973	2371	2374	2378	rVB2	205	165	0.01%	0.002%
59	9.009	2379	2385	2387	rBV	348	337	0.03%	0.004%
60	9.095	2409	2412	2417	rVB2	280	226	0.02%	0.003%
61	9.417	2498	2512	2537	rBV	425717	716898	55.75%	8.018%
62	9.568	2557	2559	2562	rVB	479	202	0.02%	0.002%
63	9.632	2576	2579	2584	rBV2	257	198	0.02%	0.002%
64	9.754	2615	2617	2624	rVB2	358	270	0.02%	0.003%
65	9.796	2628	2630	2634	rVV2	196	180	0.01%	0.002%
66	9.947	2673	2677	2682	rVB	220	207	0.02%	0.002%
67	10.108	2723	2727	2730	rVB	450	305	0.02%	0.003%
68	10.140	2730	2737	2739	rBV2	227	218	0.02%	0.002%
69	10.275	2773	2779	2783	rBV2	302	483	0.04%	0.005%
70	10.417	2820	2823	2826	rVB	311	211	0.02%	0.002%
71	10.581	2872	2874	2879	rVB2	304	168	0.01%	0.002%
72	10.600	2879	2880	2887	rVB2	215	177	0.01%	0.002%
73	10.758	2915	2929	2951	rVV	447795	724888	56.37%	8.108%
74	10.893	2969	2971	2977	rVB2	289	306	0.02%	0.003%
75	10.954	2986	2990	2997	rVB	281	213	0.02%	0.002%
76	10.986	2997	3000	3003	rBV3	335	249	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050483.D
 Acq On : 29 Aug 2022 14:37
 Operator : SY/MD
 Sample : N4322-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY179

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	11.025	3010	3012	3017	rBV2	227	179	0.01%	0.002%
78	11.066	3021	3025	3028	rBV	226	217	0.02%	0.002%
79	11.179	3055	3060	3063	rBV2	711	677	0.05%	0.008%
80	11.468	3147	3150	3151	rBV2	304	190	0.01%	0.002%
81	11.735	3231	3233	3239	rVB2	240	178	0.01%	0.002%
82	11.812	3245	3257	3280	rBV	295697	483060	37.56%	5.403%
83	12.082	3334	3341	3346	rBV6	599	803	0.06%	0.009%
84	12.195	3362	3376	3396	rVV	384241	633355	49.25%	7.084%
85	12.349	3422	3424	3429	rVB3	379	233	0.02%	0.003%
86	12.378	3430	3433	3436	rBV3	370	244	0.02%	0.003%
87	12.597	3499	3501	3506	rVB3	428	312	0.02%	0.003%
88	12.777	3553	3557	3561	rVB2	338	294	0.02%	0.003%
89	12.803	3561	3565	3567	rBV2	475	393	0.03%	0.004%
90	12.973	3615	3618	3621	rBV2	352	243	0.02%	0.003%
91	13.188	3682	3685	3689	rBV	415	321	0.02%	0.004%
92	13.282	3711	3714	3716	rBV2	276	212	0.02%	0.002%
93	13.526	3787	3790	3792	rBV	324	201	0.02%	0.002%
94	13.622	3817	3820	3825	rBV2	462	475	0.04%	0.005%
95	14.082	3959	3963	3965	rBV2	302	254	0.02%	0.003%
96	14.188	3994	3996	3998	rBV	411	247	0.02%	0.003%
97	14.786	4180	4182	4185	rBV2	552	287	0.02%	0.003%
98	14.973	4236	4240	4243	rBV3	898	757	0.06%	0.008%
99	15.195	4307	4309	4315	rVB2	654	326	0.03%	0.004%
100	15.709	4467	4469	4472	rBV2	701	527	0.04%	0.006%


Sum of corrected areas: 8940628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050483.D
Acq On : 29 Aug 2022 14:37
Operator : SY/MD
Sample : N4322-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY179

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

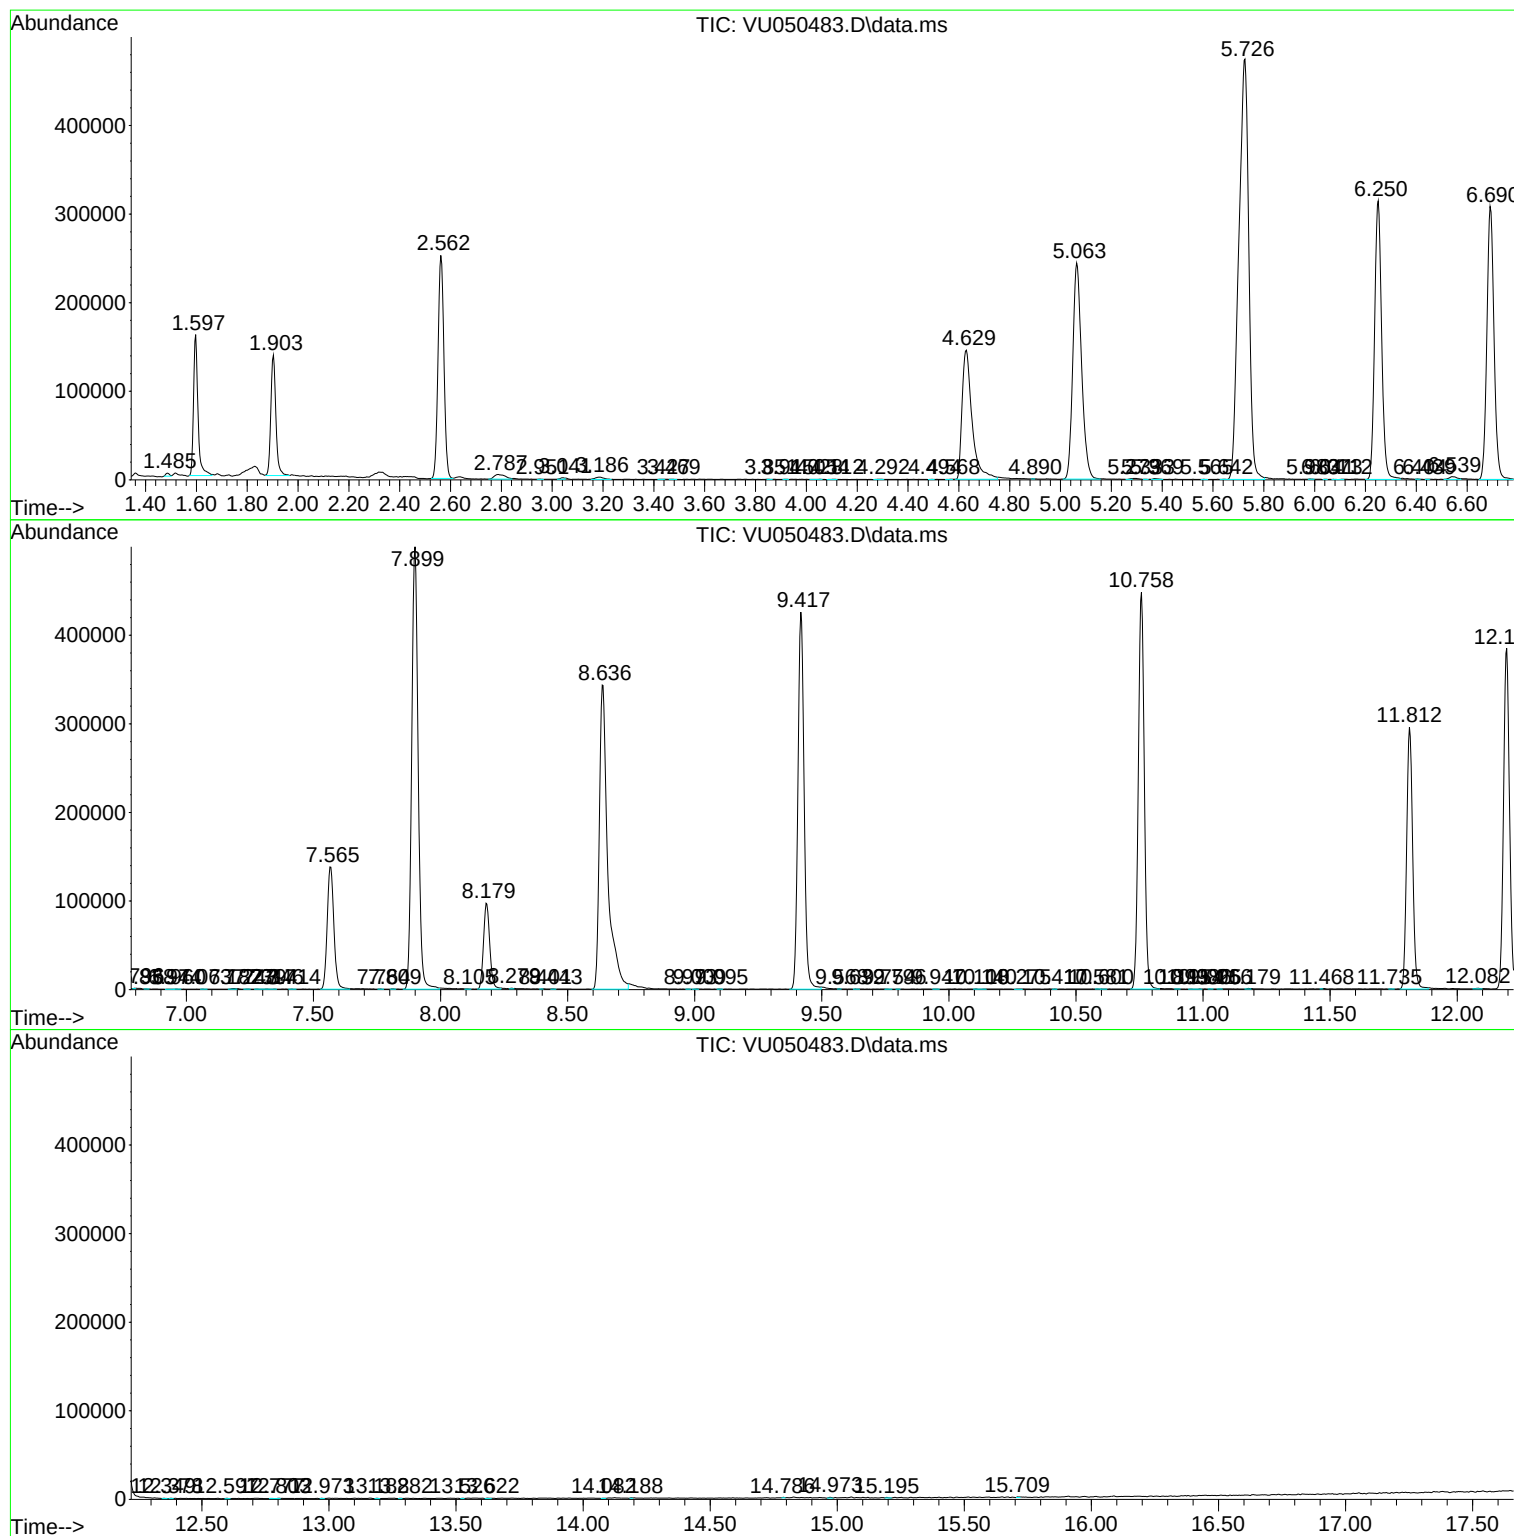

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050483.D
Acq On : 29 Aug 2022 14:37
Operator : SY/MD
Sample : N4322-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY179

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050483.D
Acq On : 29 Aug 2022 14:37
Operator : SY/MD
Sample : N4322-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY179

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------