

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050485.D
 Acq On : 29 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4399-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	49	rBV2	2980	2768	0.18%	0.026%
2	1.597	72	80	101	rBV	144795	175761	11.31%	1.654%
3	1.903	166	175	194	rVB	161892	217157	13.97%	2.043%
4	2.562	367	380	396	rBV	281798	451115	29.02%	4.244%
5	2.790	445	451	461	rBV3	839	1326	0.09%	0.012%
6	2.925	486	493	499	rBV2	394	546	0.04%	0.005%
7	3.044	519	530	542	rBV	7503	13233	0.85%	0.125%
8	3.186	562	574	584	rBV2	4026	7834	0.50%	0.074%
9	3.414	642	645	650	rBV2	124	135	0.01%	0.001%
10	3.681	725	728	733	rVB2	223	186	0.01%	0.002%
11	3.707	733	736	740	rBV	208	160	0.01%	0.002%
12	3.787	756	761	762	rBV2	200	175	0.01%	0.002%
13	3.900	790	796	802	rVB2	207	300	0.02%	0.003%
14	3.932	802	806	811	rBV	163	202	0.01%	0.002%
15	4.118	859	864	870	rVB	233	219	0.01%	0.002%
16	4.173	877	881	884	rBV2	174	137	0.01%	0.001%
17	4.289	912	917	922	rBV2	147	196	0.01%	0.002%
18	4.523	984	990	994	rBV2	224	274	0.02%	0.003%
19	4.626	1009	1022	1065	rBV	164374	442557	28.47%	4.164%
20	5.063	1141	1158	1187	rBV	284650	624844	40.20%	5.879%
21	5.211	1202	1204	1207	rVB2	448	172	0.01%	0.002%
22	5.282	1218	1226	1227	rBV4	1116	1124	0.07%	0.011%
23	5.362	1248	1251	1254	rBV2	740	610	0.04%	0.006%
24	5.504	1292	1295	1301	rBV2	257	259	0.02%	0.002%
25	5.536	1301	1305	1309	rVB2	241	205	0.01%	0.002%
26	5.600	1321	1325	1330	rVB2	216	213	0.01%	0.002%
27	5.723	1339	1363	1399	rBV2	572262	1554303	100.00%	14.624%
28	5.951	1432	1434	1438	rVV	219	129	0.01%	0.001%
29	5.973	1438	1441	1447	rVB2	577	403	0.03%	0.004%
30	6.044	1460	1463	1464	rBV	299	171	0.01%	0.002%
31	6.086	1473	1476	1480	rVB2	276	180	0.01%	0.002%
32	6.118	1483	1486	1490	rVB2	449	405	0.03%	0.004%
33	6.137	1490	1492	1494	rBV	290	201	0.01%	0.002%
34	6.166	1498	1501	1503	rBV2	267	173	0.01%	0.002%
35	6.198	1508	1511	1513	rVB	274	168	0.01%	0.002%
36	6.250	1513	1527	1548	rBV	381649	730181	46.98%	6.870%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050485.D
 Acq On : 29 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4399-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.398	1570	1573	1575	rBV2	256	155	0.01%	0.001%
38	6.497	1602	1604	1608	rBV2	384	320	0.02%	0.003%
39	6.533	1608	1615	1617	rBV2	1792	1933	0.12%	0.018%
40	6.600	1632	1636	1637	rBV	276	213	0.01%	0.002%
41	6.690	1646	1664	1688	rBV	370736	723444	46.54%	6.807%
42	6.870	1717	1720	1725	rBV	236	195	0.01%	0.002%
43	6.893	1725	1727	1730	rVB2	299	185	0.01%	0.002%
44	6.919	1730	1735	1739	rBV	253	246	0.02%	0.002%
45	6.944	1739	1743	1746	rBV2	246	195	0.01%	0.002%
46	6.964	1746	1749	1752	rBV2	243	164	0.01%	0.002%
47	7.002	1757	1761	1766	rVV2	170	165	0.01%	0.002%
48	7.028	1766	1769	1775	rVB2	138	128	0.01%	0.001%
49	7.105	1785	1793	1802	rBV2	606	1024	0.07%	0.010%
50	7.182	1812	1817	1819	rBV3	774	646	0.04%	0.006%
51	7.314	1855	1858	1860	rBV	180	129	0.01%	0.001%
52	7.407	1884	1887	1889	rBV2	210	142	0.01%	0.001%
53	7.491	1910	1913	1919	rVB2	271	235	0.02%	0.002%
54	7.565	1924	1936	1960	rBV	144806	259471	16.69%	2.441%
55	7.758	1993	1996	2001	rVB2	294	283	0.02%	0.003%
56	7.816	2008	2014	2017	rBV	387	371	0.02%	0.003%
57	7.899	2026	2040	2067	rBV	603619	1074383	69.12%	10.109%
58	8.102	2100	2103	2106	rVB3	482	326	0.02%	0.003%
59	8.179	2116	2127	2145	rBV	78205	136952	8.81%	1.289%
60	8.308	2162	2167	2170	rBV3	355	349	0.02%	0.003%
61	8.446	2207	2210	2212	rBV	319	174	0.01%	0.002%
62	8.472	2214	2218	2220	rBV	363	284	0.02%	0.003%
63	8.555	2235	2244	2253	rBV3	9559	15091	0.97%	0.142%
64	8.636	2257	2269	2309	rBV3	395217	896251	57.66%	8.433%
65	8.896	2347	2350	2352	rBV3	388	243	0.02%	0.002%
66	9.124	2416	2421	2424	rBV2	258	233	0.01%	0.002%
67	9.298	2473	2475	2480	rBV2	286	201	0.01%	0.002%
68	9.417	2499	2512	2546	rBV	537879	913565	58.78%	8.596%
69	9.607	2568	2571	2574	rVB2	445	275	0.02%	0.003%
70	9.665	2586	2589	2592	rBV	278	206	0.01%	0.002%
71	9.713	2601	2604	2607	rBV2	267	206	0.01%	0.002%
72	9.739	2610	2612	2617	rVB2	290	190	0.01%	0.002%
73	9.938	2671	2674	2677	rBV	289	207	0.01%	0.002%
74	9.989	2687	2690	2693	rBV2	351	254	0.02%	0.002%
75	10.092	2719	2722	2725	rBV2	226	182	0.01%	0.002%
76	10.137	2731	2736	2741	rVB2	225	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050485.D
 Acq On : 29 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4399-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.301	2784	2787	2792	rVB2	225	184	0.01%	0.002%
78	10.401	2815	2818	2821	rBV	226	161	0.01%	0.002%
79	10.501	2845	2849	2853	rBV	205	186	0.01%	0.002%
80	10.758	2916	2929	2952	rBV	526676	863627	55.56%	8.126%
81	10.986	2997	3000	3003	rBV2	229	138	0.01%	0.001%
82	11.028	3010	3013	3018	rBV3	371	255	0.02%	0.002%
83	11.246	3078	3081	3087	rBV	278	248	0.02%	0.002%
84	11.324	3102	3105	3109	rBV	228	170	0.01%	0.002%
85	11.391	3121	3126	3130	rBV2	296	372	0.02%	0.004%
86	11.697	3219	3221	3225	rVB2	258	154	0.01%	0.001%
87	11.748	3234	3237	3243	rVB2	294	234	0.02%	0.002%
88	11.812	3244	3257	3279	rBV	402019	655260	42.16%	6.165%
89	12.124	3351	3354	3356	rBV2	283	154	0.01%	0.001%
90	12.192	3361	3375	3402	rBV	509080	846326	54.45%	7.963%
91	12.365	3426	3429	3431	rBV3	374	296	0.02%	0.003%
92	12.446	3450	3454	3459	rVB2	633	660	0.04%	0.006%
93	12.481	3460	3465	3468	rBV3	406	402	0.03%	0.004%
94	12.655	3517	3519	3523	rVB2	280	190	0.01%	0.002%
95	12.677	3524	3526	3529	rVB3	538	272	0.02%	0.003%
96	12.697	3529	3532	3535	rBV3	449	356	0.02%	0.003%
97	13.008	3626	3629	3633	rVB3	267	206	0.01%	0.002%
98	13.198	3684	3688	3691	rBV	372	296	0.02%	0.003%
99	13.349	3732	3735	3737	rBV	338	221	0.01%	0.002%
100	15.192	4305	4308	4311	rBV3	651	376	0.02%	0.004%




Sum of corrected areas: 10628238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050485.D
Acq On : 29 Aug 2022 15:24
Operator : SY/MD
Sample : N4399-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

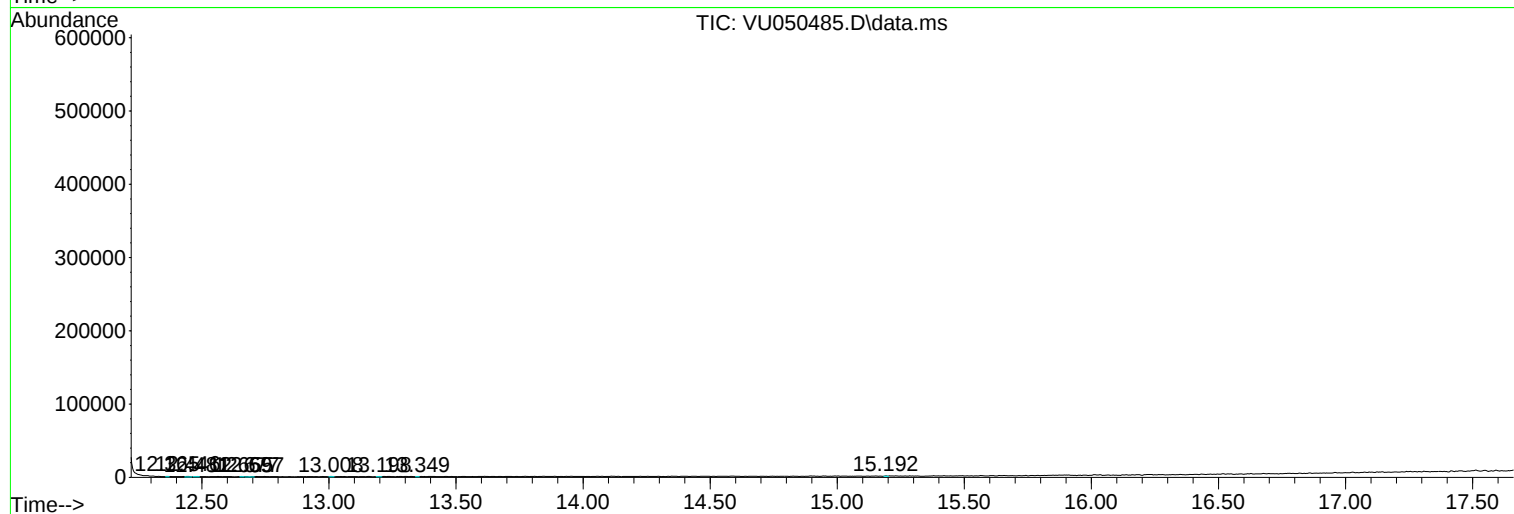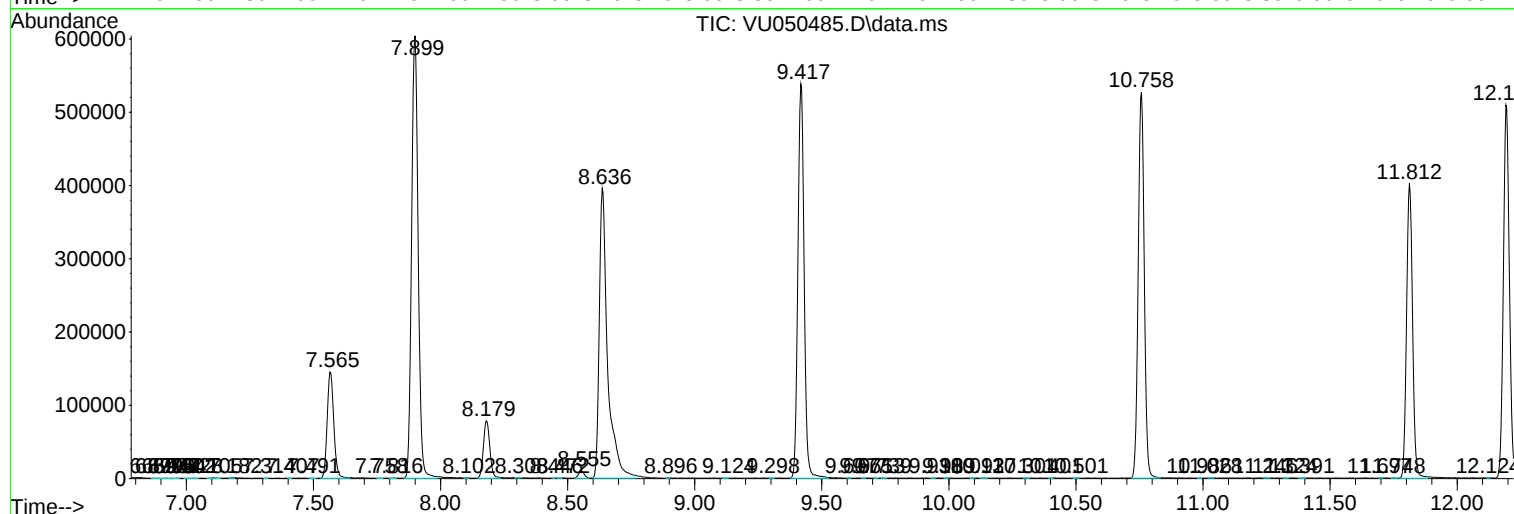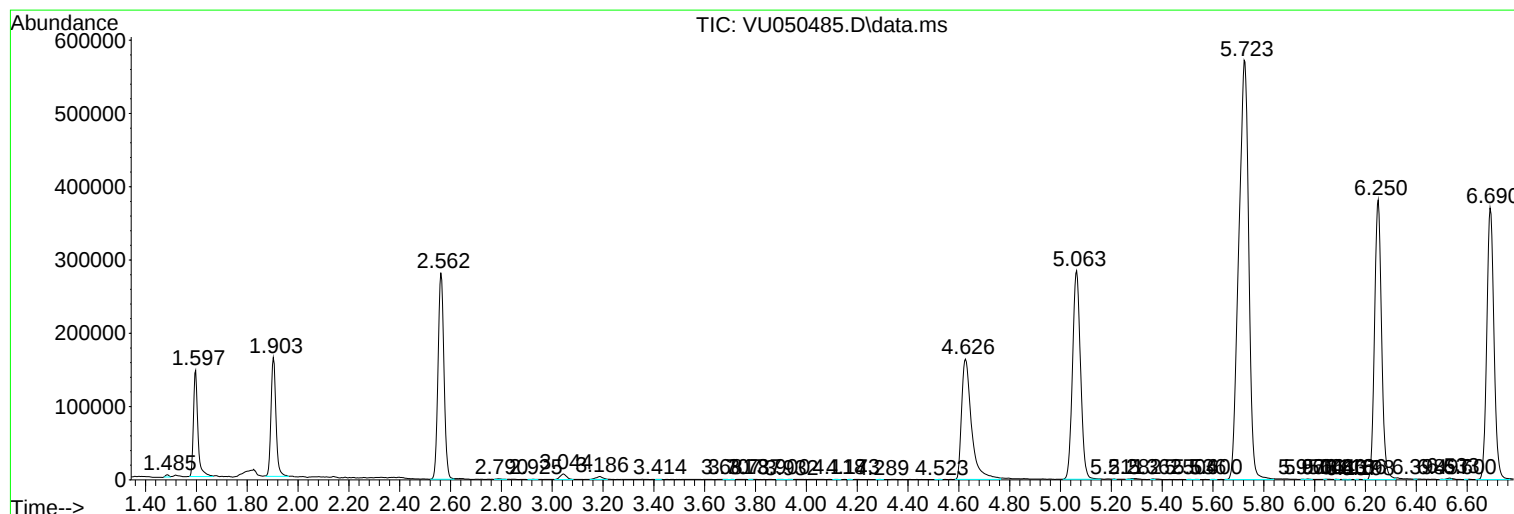

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050485.D
Acq On : 29 Aug 2022 15:24
Operator : SY/MD
Sample : N4399-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050485.D
Acq On : 29 Aug 2022 15:24
Operator : SY/MD
Sample : N4399-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------