

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050486.D
 Acq On : 29 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

Signal : TIC: VU050486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV3	3033	2839	0.19%	0.028%
2	1.597	72	80	102	rBV	159796	203069	13.45%	1.982%
3	1.899	165	174	197	rVB	150697	205487	13.61%	2.006%
4	2.562	367	380	395	rBV	259212	416692	27.60%	4.068%
5	2.758	437	441	443	rBV2	368	284	0.02%	0.003%
6	2.790	443	451	456	rBV5	1377	2110	0.14%	0.021%
7	2.877	475	478	480	rBV	377	238	0.02%	0.002%
8	3.038	522	528	529	rBV3	1673	1263	0.08%	0.012%
9	3.089	539	544	546	rBV	248	205	0.01%	0.002%
10	3.186	561	574	588	rBV2	3434	8460	0.56%	0.083%
11	3.276	596	602	604	rBV2	189	157	0.01%	0.002%
12	3.462	658	660	664	rVB	245	154	0.01%	0.002%
13	3.488	664	668	673	rBV	221	218	0.01%	0.002%
14	3.610	703	706	709	rBV	239	160	0.01%	0.002%
15	3.668	720	724	728	rBV2	218	174	0.01%	0.002%
16	3.977	814	820	823	rBV2	225	225	0.01%	0.002%
17	4.134	863	869	872	rVB	274	267	0.02%	0.003%
18	4.163	872	878	882	rBV2	261	329	0.02%	0.003%
19	4.189	882	886	891	rBV2	334	315	0.02%	0.003%
20	4.292	916	918	922	rVB2	272	170	0.01%	0.002%
21	4.472	970	974	978	rBV	195	168	0.01%	0.002%
22	4.626	1008	1022	1060	rBV	159599	428990	28.41%	4.188%
23	4.912	1107	1111	1115	rVB2	374	324	0.02%	0.003%
24	5.063	1141	1158	1183	rBV	281283	614807	40.72%	6.002%
25	5.208	1199	1203	1205	rBV2	353	299	0.02%	0.003%
26	5.298	1221	1231	1239	rVB3	1721	2857	0.19%	0.028%
27	5.369	1244	1253	1254	rBV3	708	744	0.05%	0.007%
28	5.449	1273	1278	1283	rVB	219	183	0.01%	0.002%
29	5.478	1283	1287	1292	rBV	242	212	0.01%	0.002%
30	5.507	1292	1296	1300	rBV3	293	237	0.02%	0.002%
31	5.549	1307	1309	1315	rVB	312	184	0.01%	0.002%
32	5.584	1316	1320	1323	rBV2	247	168	0.01%	0.002%
33	5.603	1323	1326	1329	rVB2	252	182	0.01%	0.002%
34	5.722	1342	1363	1382	rBV2	560264	1509731	100.00%	14.738%
35	6.041	1456	1462	1467	rVB4	302	421	0.03%	0.004%
36	6.079	1471	1474	1478	rBV2	288	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050486.D
 Acq On : 29 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.108	1481	1483	1487	rVV3	299	217	0.01%	0.002%
38	6.250	1512	1527	1548	rBV	362122	687445	45.53%	6.711%
39	6.407	1574	1576	1579	rBV	311	164	0.01%	0.002%
40	6.533	1607	1615	1622	rVB8	1470	2462	0.16%	0.024%
41	6.594	1630	1634	1641	rVB3	428	487	0.03%	0.005%
42	6.629	1641	1645	1649	rBV2	372	253	0.02%	0.002%
43	6.690	1649	1664	1688	rBV	363197	711773	47.15%	6.949%
44	6.845	1708	1712	1715	rVB3	532	437	0.03%	0.004%
45	6.915	1730	1734	1738	rBV2	206	169	0.01%	0.002%
46	7.050	1770	1776	1778	rBV2	217	243	0.02%	0.002%
47	7.134	1797	1802	1804	rVB2	262	230	0.02%	0.002%
48	7.153	1804	1808	1811	rBV2	271	209	0.01%	0.002%
49	7.182	1811	1817	1818	rBV3	926	769	0.05%	0.008%
50	7.269	1839	1844	1847	rBV2	229	205	0.01%	0.002%
51	7.501	1914	1916	1924	rVB	283	252	0.02%	0.002%
52	7.565	1924	1936	1955	rBV	168884	302837	20.06%	2.956%
53	7.716	1982	1983	1987	rVB2	370	206	0.01%	0.002%
54	7.748	1990	1993	1996	rVB3	245	157	0.01%	0.002%
55	7.899	2026	2040	2062	rBV	588460	1029904	68.22%	10.054%
56	8.179	2115	2127	2149	rBV2	113513	198361	13.14%	1.936%
57	8.301	2163	2165	2170	rVB3	458	397	0.03%	0.004%
58	8.481	2217	2221	2225	rVB2	321	271	0.02%	0.003%
59	8.542	2238	2240	2245	rVB2	444	242	0.02%	0.002%
60	8.636	2256	2269	2315	rBV2	388642	875211	57.97%	8.544%
61	8.912	2352	2355	2360	rBV	320	312	0.02%	0.003%
62	8.944	2360	2365	2371	rVB3	359	466	0.03%	0.005%
63	9.005	2378	2384	2388	rBV2	273	332	0.02%	0.003%
64	9.050	2394	2398	2401	rBV3	236	182	0.01%	0.002%
65	9.166	2433	2434	2442	rVB2	251	198	0.01%	0.002%
66	9.250	2455	2460	2463	rBV	607	483	0.03%	0.005%
67	9.269	2463	2466	2469	rVB2	326	204	0.01%	0.002%
68	9.308	2475	2478	2482	rVB	282	189	0.01%	0.002%
69	9.349	2488	2491	2497	rVB2	220	216	0.01%	0.002%
70	9.417	2497	2512	2530	rBV	498332	841512	55.74%	8.215%
71	9.607	2566	2571	2575	rVB3	472	418	0.03%	0.004%
72	9.635	2576	2580	2585	rVB3	336	339	0.02%	0.003%
73	9.664	2585	2589	2591	rBV	284	237	0.02%	0.002%
74	9.947	2672	2677	2679	rBV	352	317	0.02%	0.003%
75	10.115	2723	2729	2731	rBV	240	251	0.02%	0.002%
76	10.398	2814	2817	2822	rVB2	341	260	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050486.D
 Acq On : 29 Aug 2022 15:48
 Operator : SY/MD
 Sample : N4365-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.758	2915	2929	2953	rBV	511372	836192	55.39%	8.163%
78	10.896	2969	2972	2975	rVB	291	162	0.01%	0.002%
79	10.954	2986	2990	2993	rBV2	297	207	0.01%	0.002%
80	11.079	3028	3029	3035	rVB2	479	298	0.02%	0.003%
81	11.111	3035	3039	3044	rVB2	395	368	0.02%	0.004%
82	11.516	3161	3165	3167	rBV2	316	251	0.02%	0.002%
83	11.629	3195	3200	3204	rBV	242	264	0.02%	0.003%
84	11.812	3244	3257	3286	rBV	354434	570297	37.77%	5.567%
85	11.976	3305	3308	3309	rBV2	334	203	0.01%	0.002%
86	12.041	3324	3328	3331	rBV2	248	240	0.02%	0.002%
87	12.073	3331	3338	3344	rBV6	939	1525	0.10%	0.015%
88	12.192	3362	3375	3403	rBV	463309	768568	50.91%	7.503%
89	12.314	3411	3413	3416	rVB3	610	256	0.02%	0.002%
90	12.481	3461	3465	3466	rBV2	276	192	0.01%	0.002%
91	12.581	3494	3496	3498	rBV	273	169	0.01%	0.002%
92	12.619	3505	3508	3513	rVB2	433	254	0.02%	0.002%
93	12.684	3523	3528	3529	rBV2	395	373	0.02%	0.004%
94	12.774	3553	3556	3560	rBV2	410	389	0.03%	0.004%
95	12.825	3570	3572	3579	rVB2	368	262	0.02%	0.003%
96	12.902	3594	3596	3599	rBV	347	252	0.02%	0.002%
97	13.169	3677	3679	3682	rVB2	337	162	0.01%	0.002%
98	13.327	3725	3728	3734	rBV3	352	395	0.03%	0.004%
99	13.587	3806	3809	3814	rBV2	333	417	0.03%	0.004%
100	13.880	3896	3900	3908	rBV	424	477	0.03%	0.005%




Sum of corrected areas: 10243526

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050486.D
Acq On : 29 Aug 2022 15:48
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

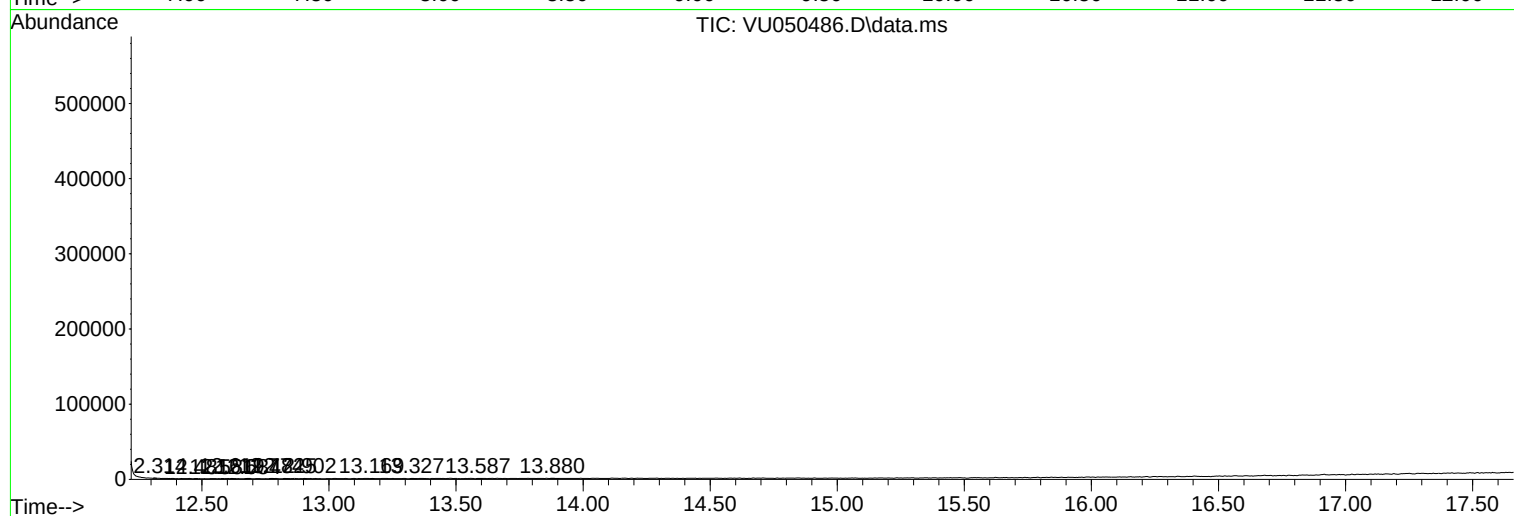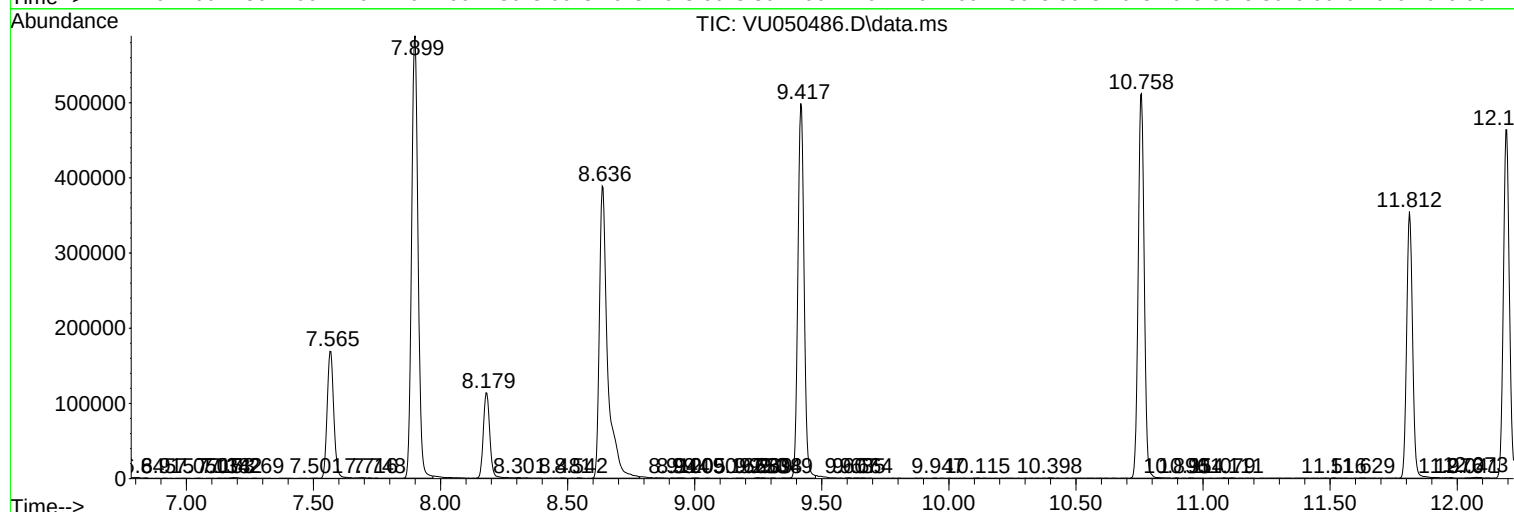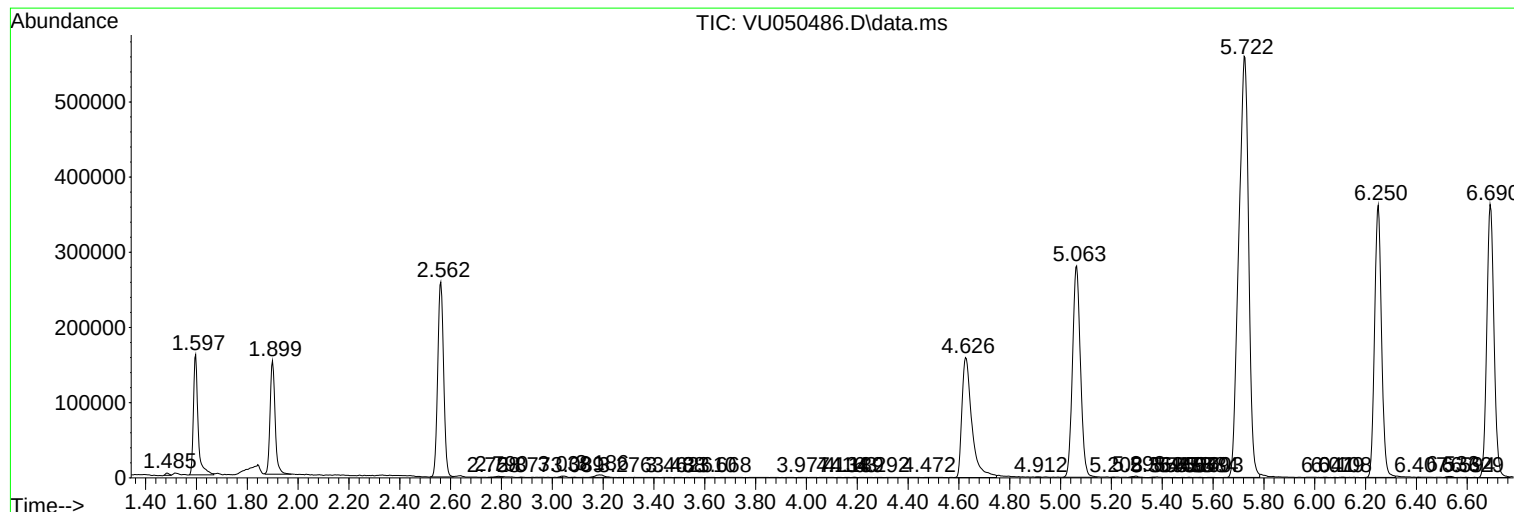

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050486.D
Acq On : 29 Aug 2022 15:48
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050486.D
Acq On : 29 Aug 2022 15:48
Operator : SY/MD
Sample : N4365-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------