

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050488.D
 Acq On : 29 Aug 2022 16:47
 Operator : SY/MD
 Sample : N4365-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M

Title : VOC Analysis

Signal : TIC: VU050488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rBV	188952	228658	14.27%	2.052%
2	1.903	167	175	191	rVB	166714	223672	13.96%	2.007%
3	2.562	368	380	398	rVB	308397	492066	30.71%	4.415%
4	2.633	398	402	403	rBV3	953	571	0.04%	0.005%
5	2.684	416	418	421	rBV3	364	189	0.01%	0.002%
6	2.909	484	488	491	rBV2	373	347	0.02%	0.003%
7	2.967	503	506	512	rBV3	304	337	0.02%	0.003%
8	3.044	517	530	541	rBV2	6978	12481	0.78%	0.112%
9	3.186	559	574	590	rBV2	4087	9592	0.60%	0.086%
10	3.247	591	593	598	rVV2	284	181	0.01%	0.002%
11	3.353	619	626	637	rVB4	911	1379	0.09%	0.012%
12	3.475	661	664	667	rVB2	260	180	0.01%	0.002%
13	3.517	674	677	685	rVB	222	239	0.01%	0.002%
14	3.562	685	691	695	rBV3	286	347	0.02%	0.003%
15	3.755	746	751	755	rVB2	312	301	0.02%	0.003%
16	3.990	820	824	827	rBV2	194	171	0.01%	0.002%
17	4.012	828	831	841	rVB2	276	283	0.02%	0.003%
18	4.092	850	856	859	rBV2	161	194	0.01%	0.002%
19	4.128	863	867	870	rVV	156	170	0.01%	0.002%
20	4.147	870	873	880	rVV2	346	412	0.03%	0.004%
21	4.240	896	902	910	rBV2	158	185	0.01%	0.002%
22	4.507	982	985	990	rVB2	192	201	0.01%	0.002%
23	4.536	990	994	999	rBV2	176	182	0.01%	0.002%
24	4.562	999	1002	1005	rBV	209	184	0.01%	0.002%
25	4.629	1010	1023	1065	rBV	153904	434380	27.11%	3.897%
26	4.970	1126	1129	1133	rBV2	253	189	0.01%	0.002%
27	5.063	1141	1158	1181	rBV	292329	640630	39.99%	5.748%
28	5.189	1194	1197	1202	rVB4	356	349	0.02%	0.003%
29	5.256	1215	1218	1222	rVB4	314	193	0.01%	0.002%
30	5.292	1222	1229	1231	rBV3	933	1307	0.08%	0.012%
31	5.372	1247	1254	1259	rBV2	1016	1262	0.08%	0.011%
32	5.491	1287	1291	1295	rVB2	244	203	0.01%	0.002%
33	5.555	1307	1311	1315	rVB2	218	178	0.01%	0.002%
34	5.726	1342	1364	1396	rBV2	593164	1602166	100.00%	14.375%
35	5.922	1423	1425	1429	rVB3	412	283	0.02%	0.003%
36	6.073	1469	1472	1475	rVB2	260	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050488.D
 Acq On : 29 Aug 2022 16:47
 Operator : SY/MD
 Sample : N4365-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

37	6.115	1482	1485	1488	rBV	373	317	0.02%	0.003%
38	6.250	1513	1527	1556	rBV	403053	771618	48.16%	6.923%
39	6.536	1607	1616	1623	rVB6	1844	3241	0.20%	0.029%
40	6.594	1631	1634	1636	rBV2	492	296	0.02%	0.003%
41	6.690	1651	1664	1694	rVV	379807	741373	46.27%	6.652%
42	6.841	1709	1711	1715	rVB3	585	345	0.02%	0.003%
43	6.870	1718	1720	1726	rBV2	245	164	0.01%	0.001%
44	6.896	1726	1728	1733	rVB2	244	165	0.01%	0.001%
45	7.157	1802	1809	1812	rBV2	176	175	0.01%	0.002%
46	7.195	1813	1821	1822	rBV2	673	633	0.04%	0.006%
47	7.346	1861	1868	1870	rBV	180	191	0.01%	0.002%
48	7.423	1887	1892	1899	rVB2	325	430	0.03%	0.004%
49	7.465	1899	1905	1906	rBV	284	308	0.02%	0.003%
50	7.507	1914	1918	1921	rBV	264	186	0.01%	0.002%
51	7.568	1924	1937	1954	rBV	177540	316468	19.75%	2.839%
52	7.690	1972	1975	1977	rBV	248	182	0.01%	0.002%
53	7.739	1988	1990	2000	rVB3	214	245	0.02%	0.002%
54	7.780	2000	2003	2004	rBV3	287	179	0.01%	0.002%
55	7.803	2004	2010	2019	rVB5	1462	2170	0.14%	0.019%
56	7.899	2023	2040	2061	rBV	646003	1131990	70.65%	10.157%
57	8.182	2115	2128	2150	rBV	120360	211799	13.22%	1.900%
58	8.314	2165	2169	2175	rVB4	474	491	0.03%	0.004%
59	8.359	2180	2183	2188	rBV3	428	382	0.02%	0.003%
60	8.475	2217	2219	2224	rVB2	317	187	0.01%	0.002%
61	8.513	2228	2231	2234	rBV2	231	167	0.01%	0.001%
62	8.558	2238	2245	2249	rBV3	1318	1574	0.10%	0.014%
63	8.584	2249	2253	2256	rVB2	376	304	0.02%	0.003%
64	8.639	2256	2270	2317	rBV2	388457	887261	55.38%	7.961%
65	8.880	2340	2345	2348	rBV2	299	227	0.01%	0.002%
66	8.957	2366	2369	2372	rBV3	338	239	0.01%	0.002%
67	8.996	2378	2381	2386	rVB2	204	169	0.01%	0.002%
68	9.025	2386	2390	2393	rBV	235	234	0.01%	0.002%
69	9.124	2415	2421	2428	rBV3	281	406	0.03%	0.004%
70	9.160	2428	2432	2440	rVB4	382	441	0.03%	0.004%
71	9.420	2497	2513	2532	rBV	576364	962240	60.06%	8.634%
72	9.571	2556	2560	2566	rVB4	1518	1695	0.11%	0.015%
73	9.857	2644	2649	2652	rBV	154	170	0.01%	0.002%
74	10.201	2748	2756	2759	rBV	265	304	0.02%	0.003%
75	10.275	2776	2779	2783	rBV	320	255	0.02%	0.002%
76	10.327	2790	2795	2798	rBV2	303	297	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050488.D
 Acq On : 29 Aug 2022 16:47
 Operator : SY/MD
 Sample : N4365-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis

77	10.349	2798	2802	2811	rBV2	697	948	0.06%	0.009%
78	10.475	2838	2841	2846	rBV2	236	225	0.01%	0.002%
79	10.758	2916	2929	2955	rBV	544362	879126	54.87%	7.888%
80	10.909	2966	2976	2991	rVB2	8527	13200	0.82%	0.118%
81	11.176	3056	3059	3062	rVB	348	193	0.01%	0.002%
82	11.382	3120	3123	3129	rBV2	348	398	0.02%	0.004%
83	11.574	3179	3183	3186	rVB3	365	329	0.02%	0.003%
84	11.636	3199	3202	3208	rVB	313	270	0.02%	0.002%
85	11.812	3245	3257	3277	rBV	423957	685298	42.77%	6.149%
86	12.137	3356	3358	3362	rBV	236	198	0.01%	0.002%
87	12.195	3363	3376	3395	rBV	525689	867822	54.17%	7.786%
88	12.439	3446	3452	3458	rBV4	629	738	0.05%	0.007%
89	12.549	3483	3486	3488	rBV2	243	179	0.01%	0.002%
90	12.619	3505	3508	3510	rBV2	409	270	0.02%	0.002%
91	12.777	3555	3557	3560	rBV2	339	226	0.01%	0.002%
92	12.848	3576	3579	3583	rBV	485	362	0.02%	0.003%
93	12.951	3609	3611	3618	rVB3	520	380	0.02%	0.003%
94	12.983	3618	3621	3623	rBV2	384	257	0.02%	0.002%
95	13.070	3646	3648	3652	rBV	232	178	0.01%	0.002%
96	13.140	3666	3670	3673	rBV2	494	418	0.03%	0.004%
97	13.266	3705	3709	3712	rBV3	263	279	0.02%	0.003%
98	13.352	3733	3736	3741	rBV3	270	257	0.02%	0.002%
99	13.533	3789	3792	3793	rBV2	274	164	0.01%	0.001%
100	14.089	3963	3965	3967	rBV	317	163	0.01%	0.001%

Sum of corrected areas: 11145242




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050488.D
Acq On : 29 Aug 2022 16:47
Operator : SY/MD
Sample : N4365-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

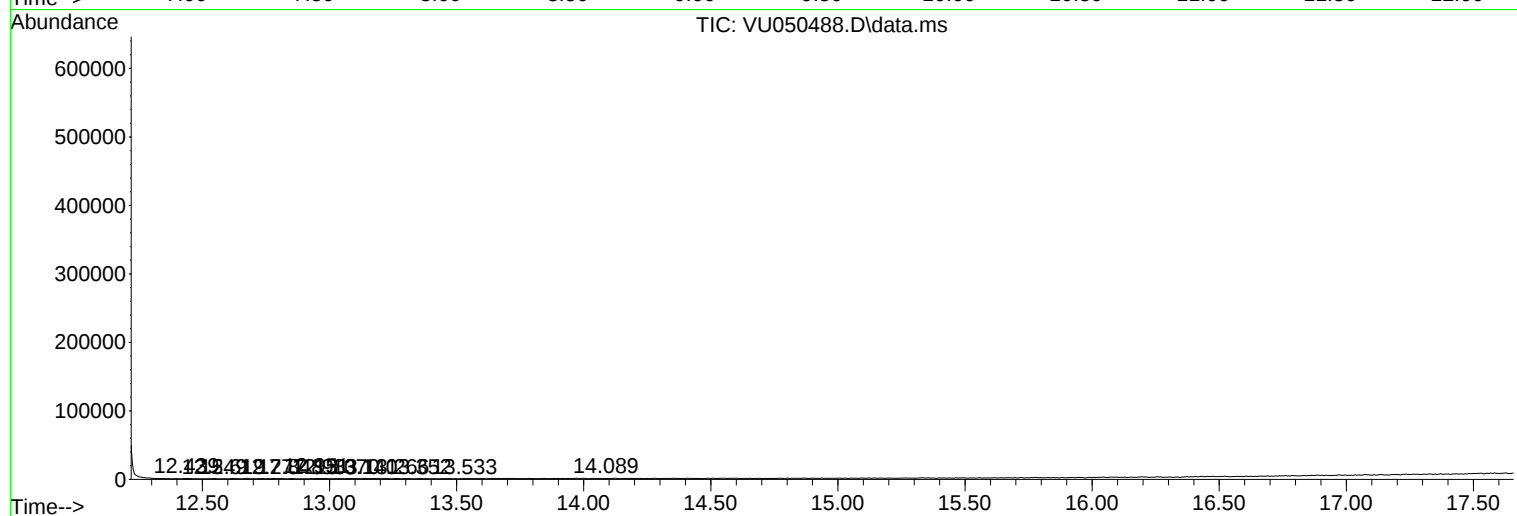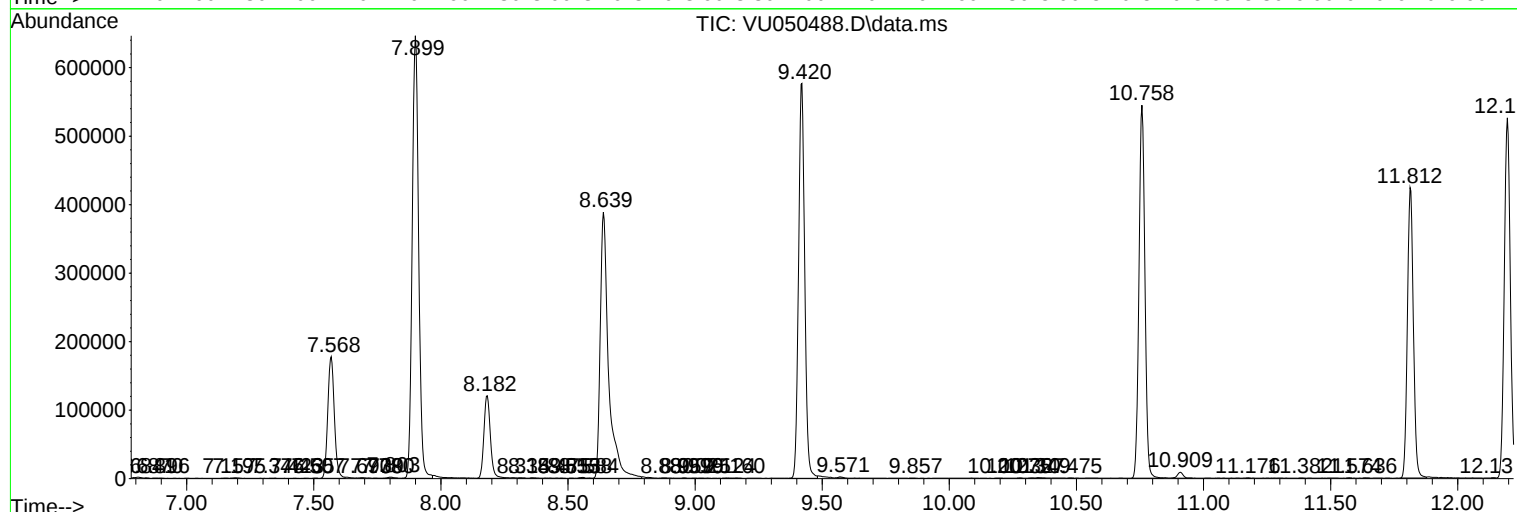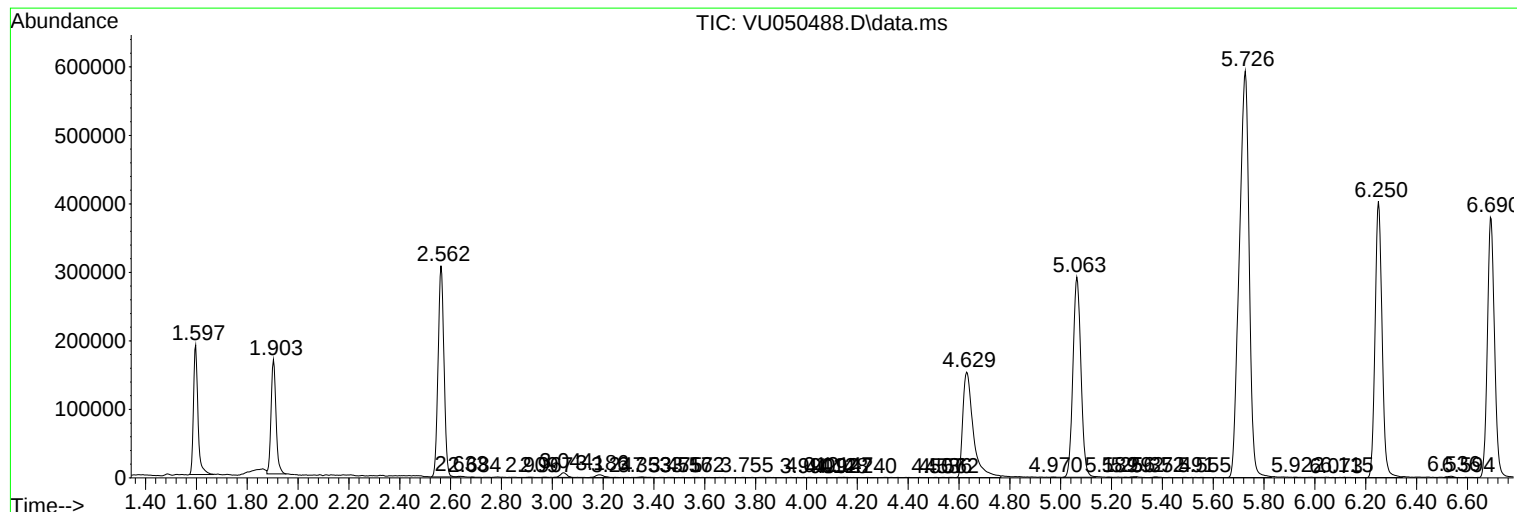

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050488.D
Acq On : 29 Aug 2022 16:47
Operator : SY/MD
Sample : N4365-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
Data File : VU050488.D
Acq On : 29 Aug 2022 16:47
Operator : SY/MD
Sample : N4365-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------