
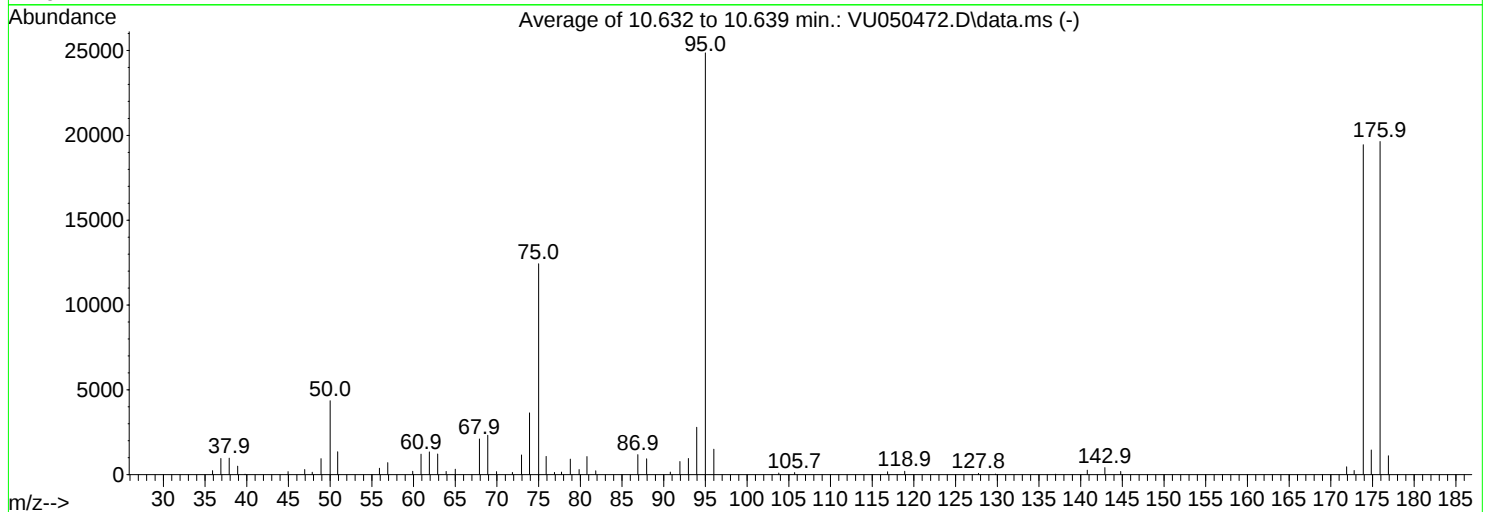


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082922\
 Data File : VU050472.D
 Acq On : 29 Aug 2022 09:45
 Operator : SY/MD
 Sample : BFB114
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB114

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM082422WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 30 05:29:53 2022

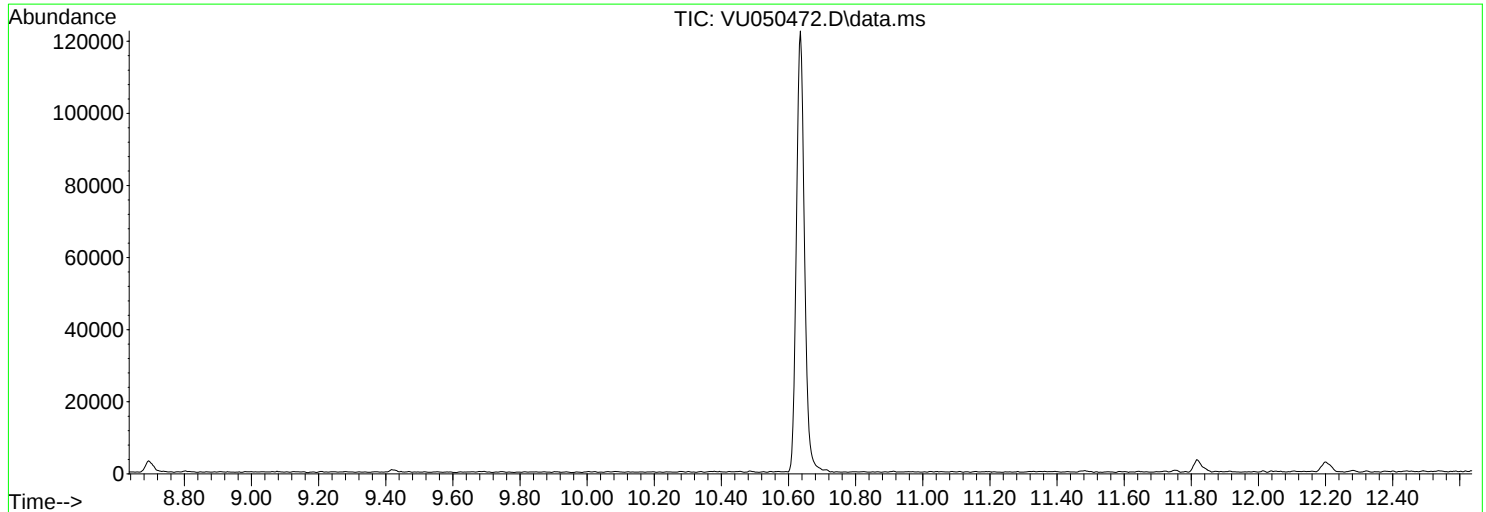

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4355	PASS
75	95	30	80	50.0	12432	PASS
95	95	100	100	100.0	24864	PASS
96	95	5	9	6.0	1497	PASS
173	174	0.00	2	1.2	242	PASS
174	95	50	120	78.2	19453	PASS
175	174	5	9	7.5	1455	PASS
176	174	95	101	100.9	19635	PASS
177	176	5	9	5.7	1112	PASS

m/z	Abundance
39.90	149.0
43.90	439.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.90	243.0
36.90	1000.0
37.90	988.0
38.90	566.0
39.80	139.0
44.00	523.0
44.90	210.0
47.00	225.0
47.90	119.0
48.90	977.0
50.00	4388.0
50.90	1344.0
55.90	371.0
56.90	707.0
59.90	203.0
60.90	1205.0
61.90	1318.0
62.90	1192.0
63.90	196.0
65.00	341.0
67.90	2156.0
68.90	2359.0
70.00	190.0
71.80	133.0
72.90	1240.0
73.90	3711.0
75.00	12742.0
75.90	1204.0
76.90	120.0
77.80	182.0
78.80	923.0
79.80	290.0
80.80	1084.0
81.90	219.0
86.90	1158.0
87.90	1024.0
90.80	115.0
91.90	749.0
92.90	883.0
93.90	2742.0
95.00	24944.0
96.00	1611.0
105.70	103.0
116.90	184.0
118.90	146.0
127.70	115.0
140.80	234.0
142.90	388.0
144.80	193.0
171.90	437.0
172.80	213.0
173.90	18992.0
174.80	1516.0
175.90	19464.0
176.90	1085.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.90	242.0
36.90	990.0
37.90	999.0
38.90	507.0
39.80	169.0
43.90	411.0
45.00	177.0
46.90	307.0
47.80	153.0
48.90	988.0
50.00	4515.0
50.90	1416.0
55.90	390.0
56.90	729.0
59.90	207.0
60.90	1265.0
61.90	1388.0
62.90	1256.0
63.90	191.0
65.00	339.0
67.90	2094.0
68.90	2347.0
69.90	192.0
71.90	132.0
72.90	1204.0
73.90	3737.0
75.00	12868.0
75.90	1110.0
76.90	129.0
77.80	142.0
78.80	945.0
79.90	311.0
80.80	1126.0
81.90	223.0
86.90	1233.0
88.00	949.0
90.80	155.0
92.00	818.0
93.00	1000.0
93.90	2899.0
95.00	25648.0
96.00	1542.0
103.80	135.0
105.70	133.0
116.90	165.0
118.90	205.0
127.80	121.0
137.00	100.0
140.80	278.0
142.90	428.0
144.80	202.0
171.90	500.0
172.80	244.0
173.90	19880.0
174.80	1498.0
175.90	20352.0
176.90	1129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114

m/z	Abundance
35.90	229.0
36.90	880.0
37.90	928.0
38.90	429.0
39.80	217.0
43.80	343.0
45.00	149.0
46.90	361.0
47.80	166.0
48.90	878.0
50.00	4161.0
50.90	1288.0
55.90	383.0
56.90	678.0
59.90	183.0
60.90	1163.0
61.90	1306.0
62.90	1197.0
63.90	180.0
65.00	295.0
67.90	2061.0
68.90	2247.0
69.90	163.0
71.90	126.0
73.00	1039.0
73.90	3475.0
75.00	11686.0
75.90	923.0
76.90	156.0
77.70	120.0
78.80	876.0
79.90	305.0
80.80	995.0
81.80	238.0
86.90	1151.0
88.00	838.0
90.80	194.0
92.00	757.0
93.00	972.0
94.00	2744.0
95.00	24000.0
96.00	1338.0
103.80	146.0
105.70	131.0
116.80	153.0
118.90	231.0
129.80	110.0
140.80	286.0
142.90	426.0
144.80	173.0
171.90	458.0
172.80	268.0
173.90	19488.0
174.90	1350.0
175.90	19088.0
176.90	1122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB114