




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
 Data File : VU054986.D
 Acq On : 30 Aug 2023 04:07
 Operator : MD/SY
 Sample : 04173-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Quant Time: Aug 30 04:26:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 30 01:18:16 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

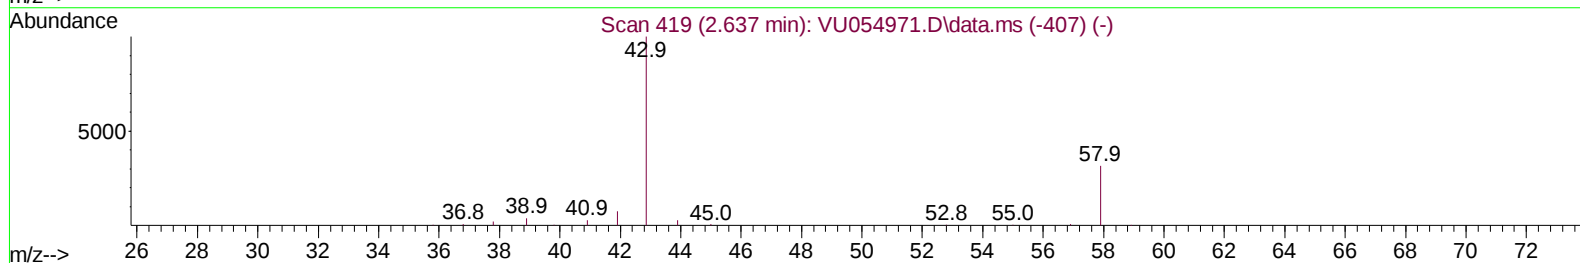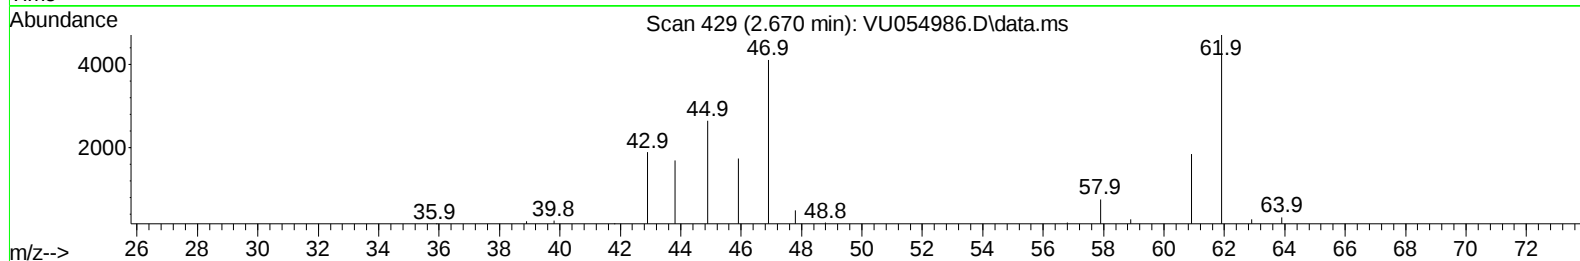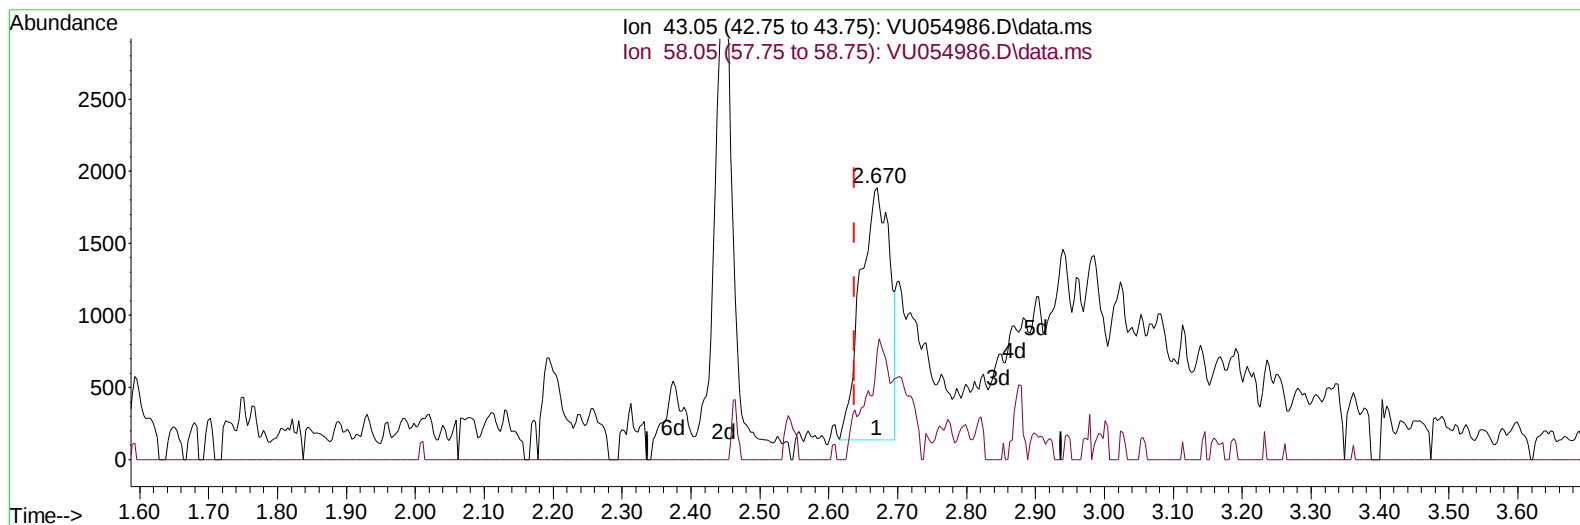

TIC: VU054986.D\data.ms

(13) Acetone (T)

2.670min (+ 0.033) 3.51 ug/L

response 5165

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	17.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
 Data File : VU054986.D
 Acq On : 30 Aug 2023 04:07
 Operator : MD/SY
 Sample : 04173-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Quant Time: Aug 30 04:26:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 30 01:18:16 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

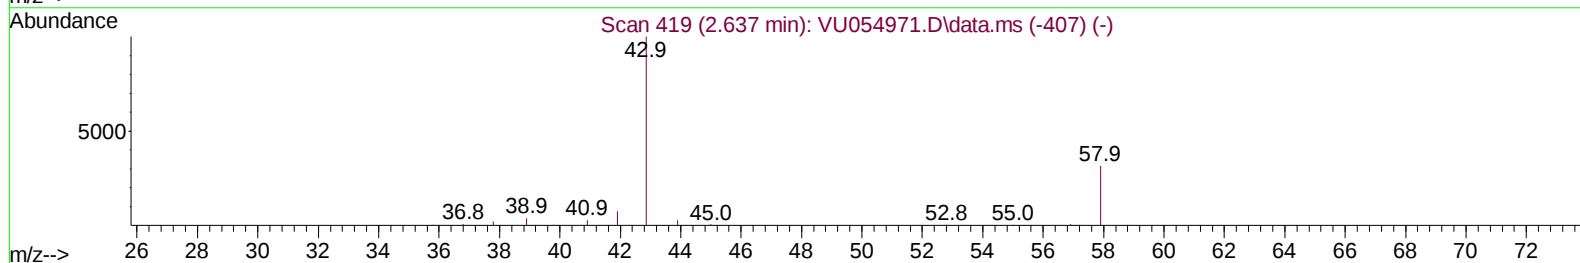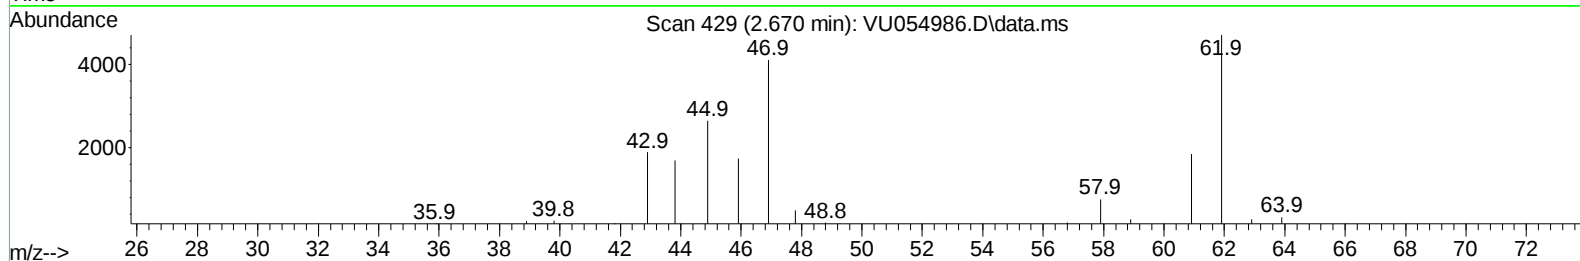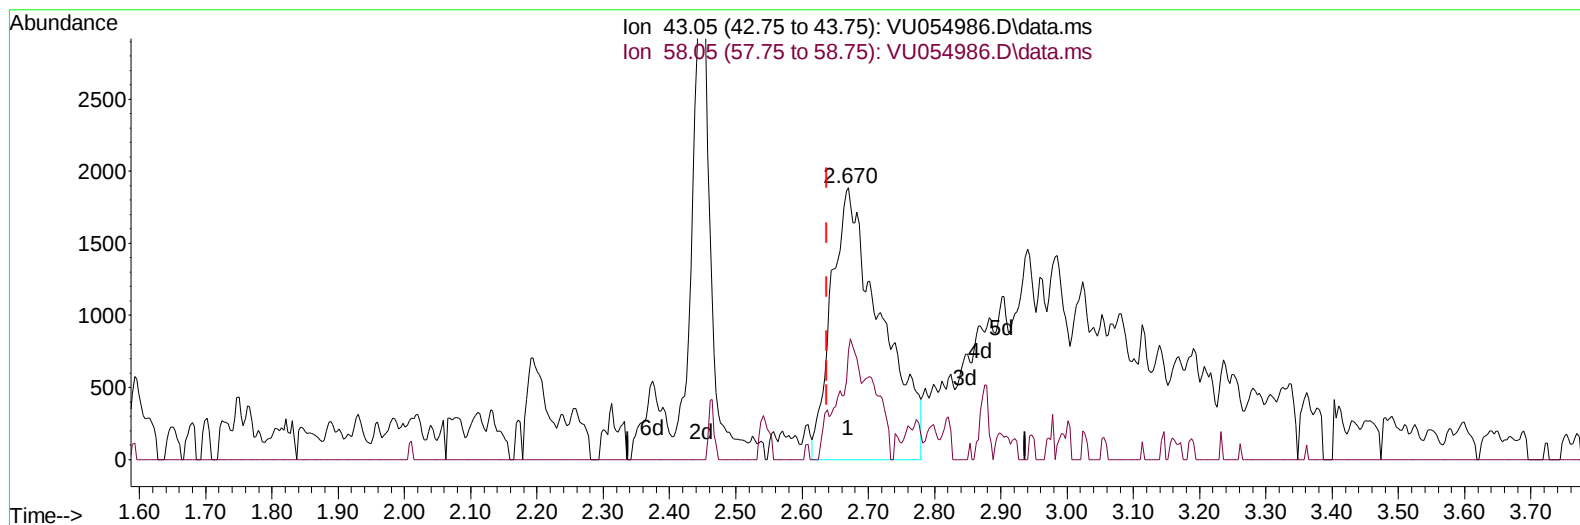

TIC: VU054986.D\data.ms

(13) Acetone (T)

2.670min (+ 0.033) 6.61 ug/L m

response 9721

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	9.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
 Data File : VU054986.D
 Acq On : 30 Aug 2023 04:07
 Operator : MD/SY
 Sample : 04173-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

Quant Time: Aug 30 04:26:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 30 01:18:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	159759	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.416	117	152794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	78659	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.593	65	25467	5.051	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 101.000%			
7) Chloroethane-d5	1.908	69	30492	4.681	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 93.600%			
11) 1,1-Dichloroethene-d2	2.561	65	14784	5.188	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 103.800%			
20) 2-Butanone-d5	4.651	46	160195	58.857	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery = 117.720%			
24) Chloroform-d	5.062	84	93868	5.018	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 100.400%			
26) 1,2-Dichloroethane-d4	5.702	65	53083	5.333	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 106.600%			
32) Benzene-d6	5.724	84	169872	4.946	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 99.000%			
36) 1,2-Dichloropropane-d6	6.689	67	60162	4.980	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 99.600%			
41) Toluene-d8	7.895	98	147094	4.472	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 89.400%			
43) trans-1,3-Dichloroprop...	8.181	79	16804	4.227	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 84.600%			
46) 2-Hexanone-d5	8.638	63	109544	58.057	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 116.120%			
56) 1,1,2,2-Tetrachloroeth...	10.753	84	57411	5.542	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 110.800%			
66) 1,2-Dichlorobenzene-d4	12.194	152	64864	5.165	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 103.200%			
Target Compounds						
3) Chloromethane	1.516	50	5518	0.534	ug/L	91
13) Acetone	2.670	43	9721m	6.607	ug/L	
14) Carbon disulfide	2.789	76	5602	0.280	ug/L #	89
18) trans-1,2-Dichloroethene	3.355	96	3036	0.385	ug/L	82
21) 2-Butanone	4.741	43	20174	8.949	ug/L	74
22) cis-1,2-Dichloroethene	4.667	96	9605	1.022	ug/L	96
34) Trichloroethene	6.541	95	8241	0.825	ug/L	87
42) Toluene	7.969	91	31369	0.784	ug/L	97
51) Chlorobenzene	9.448	112	3418	0.131	ug/L #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054986.D
Acq On : 30 Aug 2023 04:07
Operator : MD/SY
Sample : 04173-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 08/31/2023

Quant Time: Aug 30 04:26:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 30 01:18:16 2023
Response via : Initial Calibration

