

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
 Data File : VU054957.D
 Acq On : 29 Aug 2023 15:20
 Operator : MD/SY
 Sample : 04158-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	102	rBV	33818	38889	5.00%	0.742%
2	1.911	185	193	207	rVB	47963	63973	8.22%	1.220%
3	2.563	384	396	412	rVB	78180	126881	16.30%	2.420%
4	3.042	532	545	557	rBV4	9929	18896	2.43%	0.360%
5	4.631	1024	1039	1078	rBV	108328	313668	40.31%	5.984%
6	5.061	1155	1173	1196	rVB2	103557	239847	30.82%	4.575%
7	5.724	1360	1379	1398	rBV2	200847	531745	68.33%	10.144%
8	6.248	1529	1542	1563	rBV	228686	442743	56.89%	8.446%
9	6.528	1619	1629	1643	rBV9	4263	8562	1.10%	0.163%
10	6.688	1666	1679	1694	rBV2	137009	277818	35.70%	5.300%
11	7.566	1941	1952	1970	rBV2	56140	103996	13.36%	1.984%
12	7.897	2041	2055	2074	rBV	243969	436522	56.09%	8.327%
13	8.180	2131	2143	2155	rBV	34842	61831	7.95%	1.179%
14	8.634	2272	2284	2322	rBV3	366233	778211	100.00%	14.845%
15	9.415	2515	2527	2555	rBV	320743	553085	71.07%	10.551%
16	10.756	2933	2944	2960	rBV	124143	203054	26.09%	3.873%
17	10.891	2977	2986	2996	rVB5	6573	10434	1.34%	0.199%
18	11.810	3261	3272	3290	rBV	352616	574423	73.81%	10.958%
19	12.193	3379	3391	3410	rBV	275942	457604	58.80%	8.729%




Sum of corrected areas: 5242182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054957.D
Acq On : 29 Aug 2023 15:20
Operator : MD/SY
Sample : 04158-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

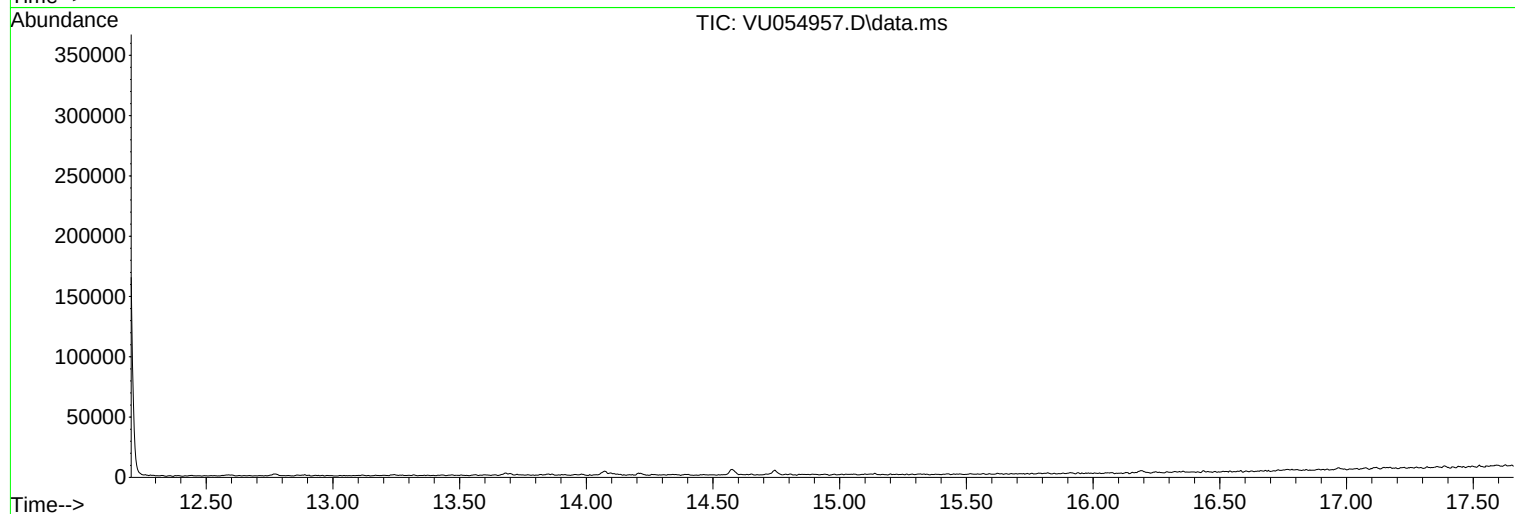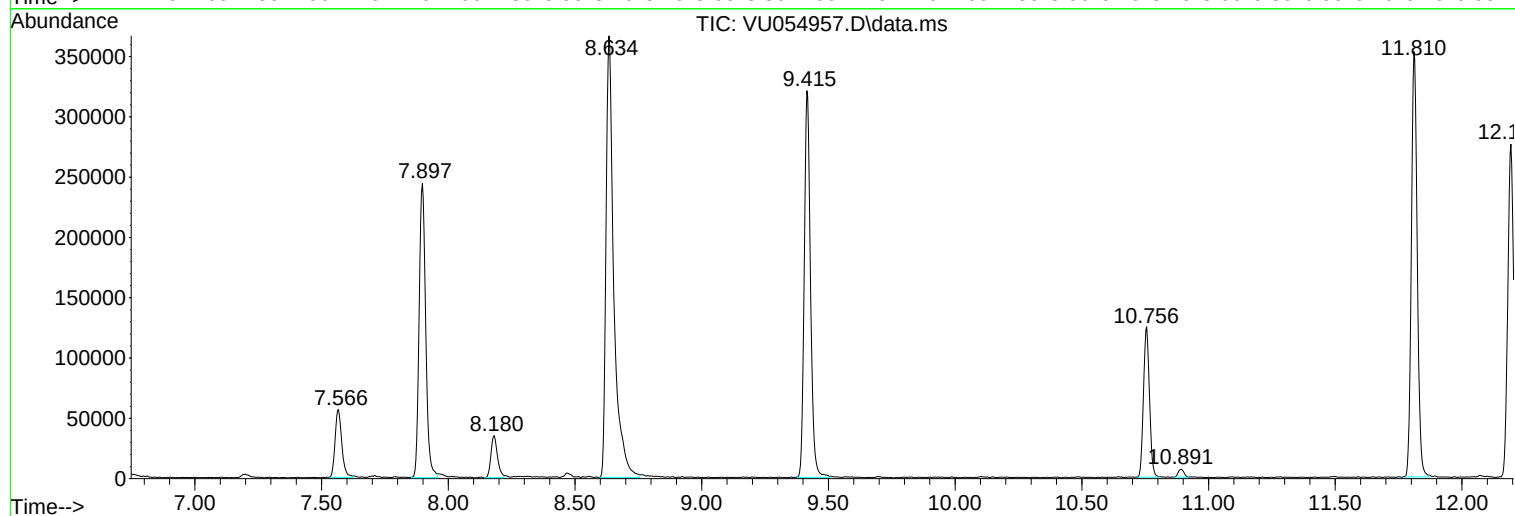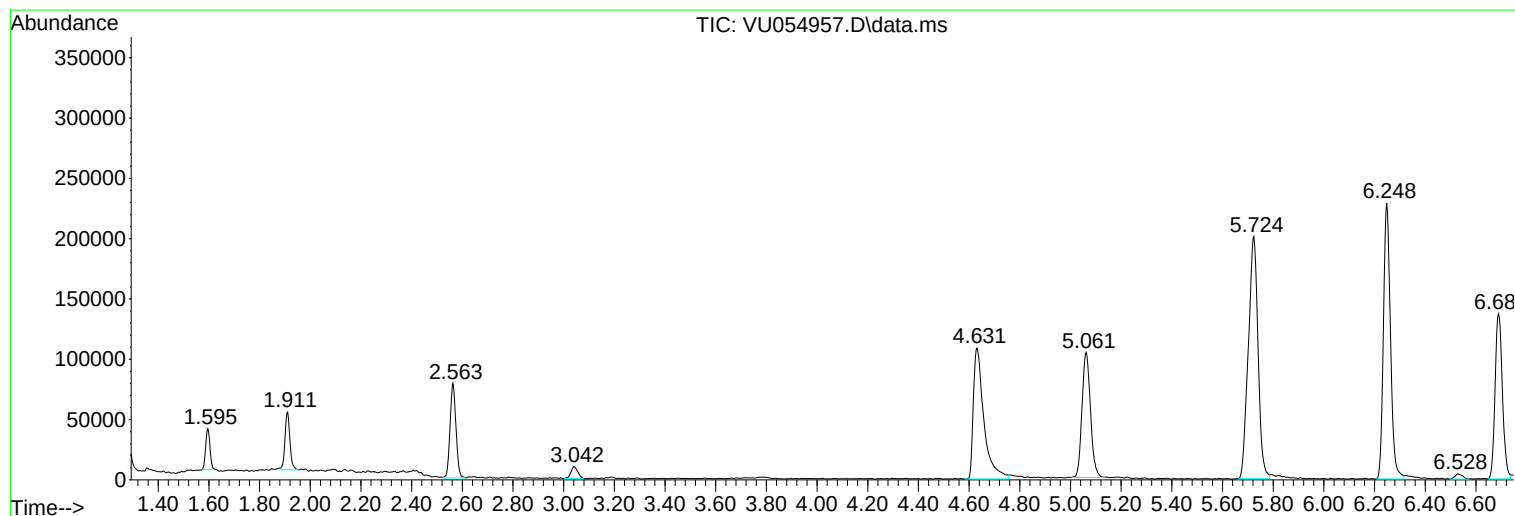

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054957.D
Acq On : 29 Aug 2023 15:20
Operator : MD/SY
Sample : 04158-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054957.D
Acq On : 29 Aug 2023 15:20
Operator : MD/SY
Sample : 04158-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc