

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
 Data File : VU054970.D
 Acq On : 29 Aug 2023 20:42
 Operator : MD/SY
 Sample : 04209-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH469

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.464	45	54	65	rVB	105470	110223	14.77%	2.149%
2	1.595	86	95	108	rVB	39127	50201	6.73%	0.979%
3	1.911	184	193	208	rVB	46861	63734	8.54%	1.243%
4	2.377	326	338	349	rBV3	13688	28512	3.82%	0.556%
5	2.563	384	396	410	rVB	76509	125336	16.79%	2.444%
6	4.631	1028	1039	1068	rBV	105313	292309	39.16%	5.699%
7	5.062	1158	1173	1198	rVB	105251	238916	32.01%	4.658%
8	5.724	1357	1379	1397	rBV2	190137	515766	69.10%	10.056%
9	6.248	1528	1542	1563	rBV	210130	412122	55.21%	8.035%
10	6.689	1663	1679	1698	rBV2	131645	264847	35.48%	5.164%
11	7.566	1940	1952	1966	rBV	53555	95570	12.80%	1.863%
12	7.897	2043	2055	2076	rBV	228893	409155	54.81%	7.977%
13	8.180	2132	2143	2159	rBV3	30394	56213	7.53%	1.096%
14	8.634	2271	2284	2319	rBV2	343080	746456	100.00%	14.554%
15	9.418	2515	2528	2548	rBV	294487	512285	68.63%	9.988%
16	10.756	2932	2944	2958	rBV	119109	192758	25.82%	3.758%
17	10.891	2976	2986	3000	rVB3	6751	11797	1.58%	0.230%
18	11.814	3261	3273	3292	rBV	314904	527161	70.62%	10.278%
19	12.061	3340	3350	3369	rBV	22445	44613	5.98%	0.870%
20	12.193	3378	3391	3411	rBV	258180	430990	57.74%	8.403%




Sum of corrected areas: 5128964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054970.D
Acq On : 29 Aug 2023 20:42
Operator : MD/SY
Sample : 04209-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH469

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

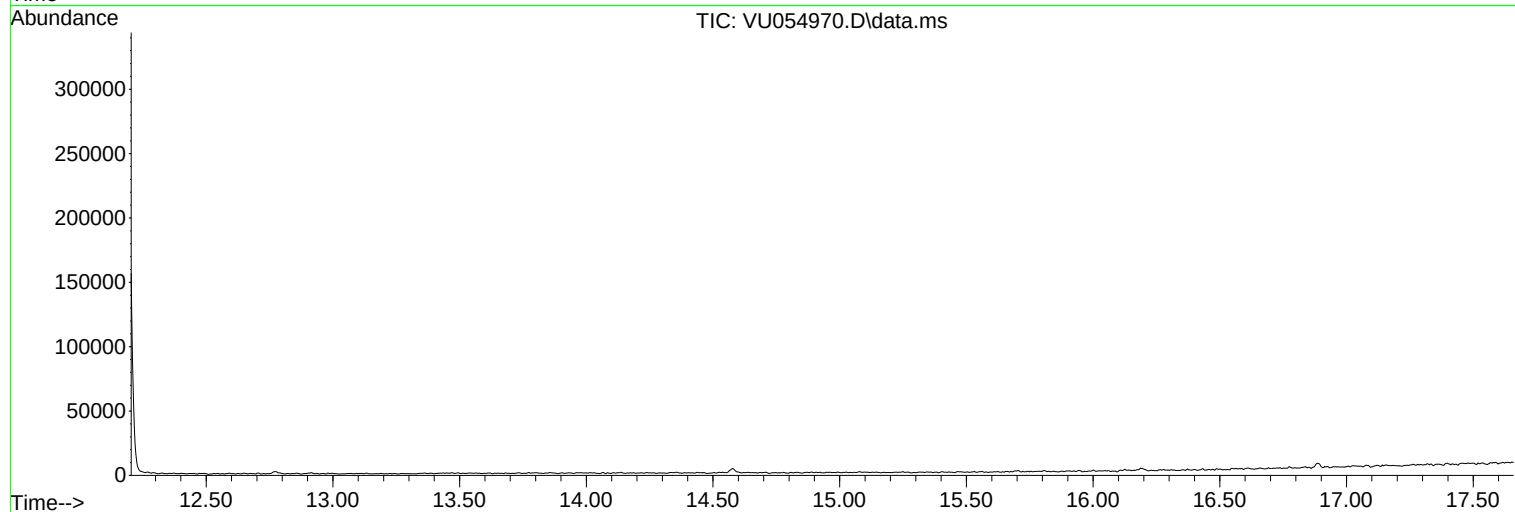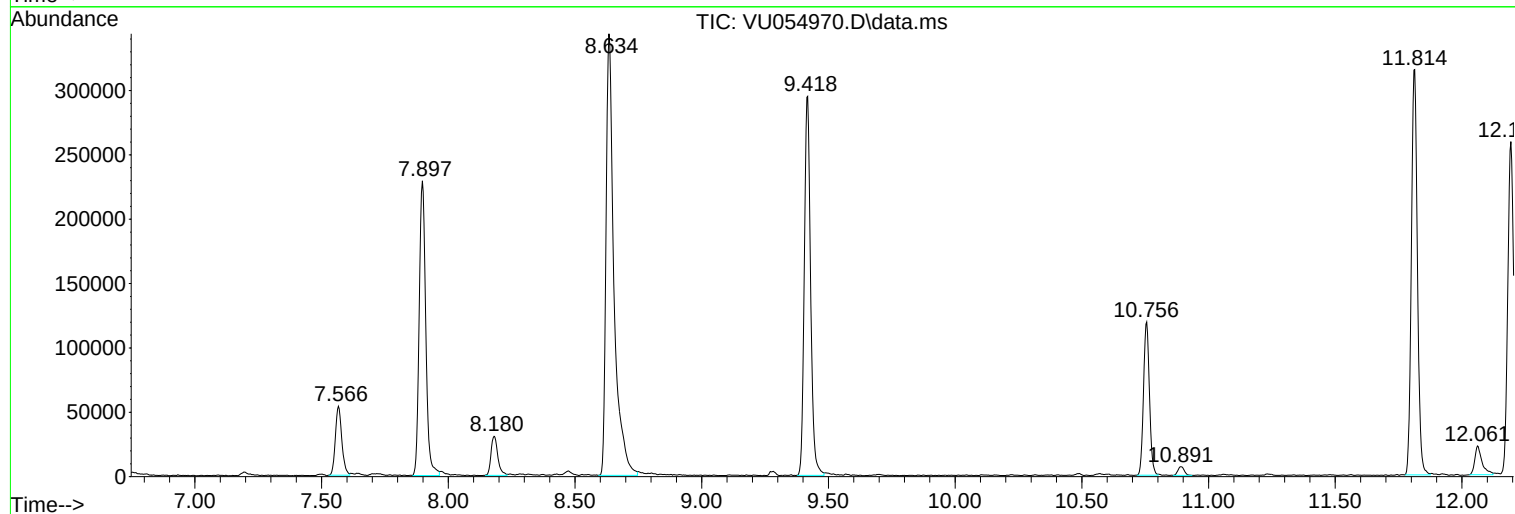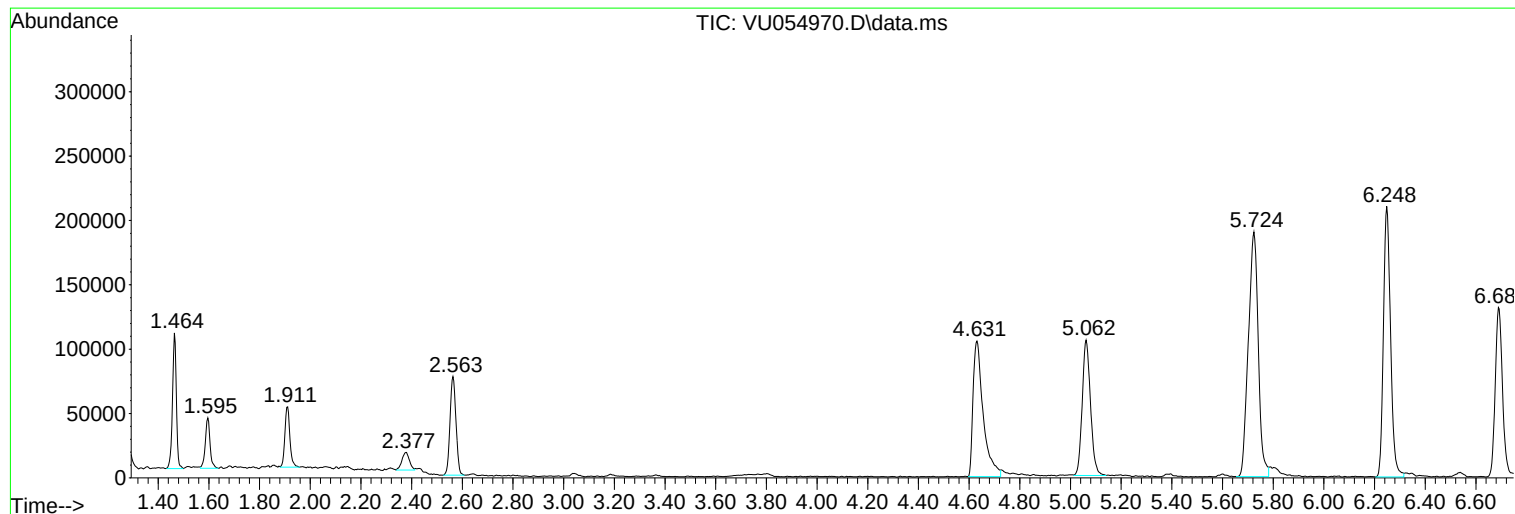

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054970.D
Acq On : 29 Aug 2023 20:42
Operator : MD/SY
Sample : 04209-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH469










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.464	1.34 ug/L	110223	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,1,1,4,4,4-Hexafluorobut-2-ene	164	C4H2F6	1010394-40-0	9		
2	3-Pyridinol	95	C5H5NO	000109-00-2	5		
3	4-Pyridinol	95	C5H5NO	000626-64-2	5		
4	4-Pyridazinamine	95	C4H5N3	020744-39-2	4		
5	Pyridine, 1-oxide	95	C5H5NO	000694-59-7	4		

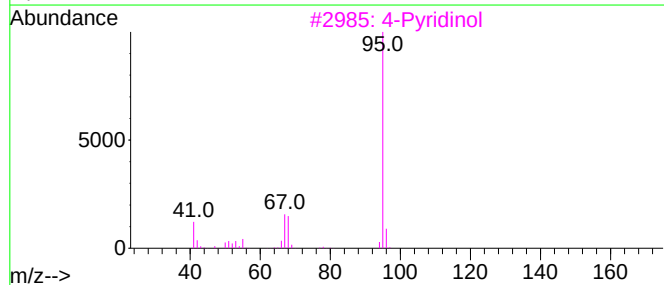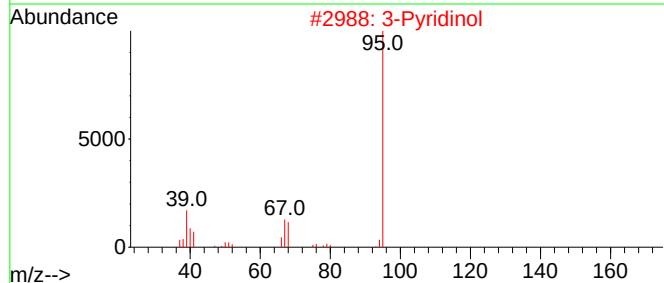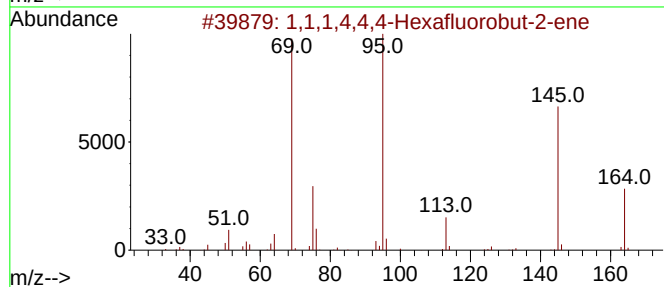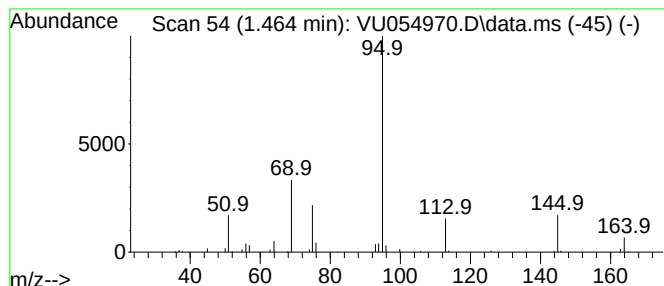

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054970.D
Acq On : 29 Aug 2023 20:42
Operator : MD/SY
Sample : 04209-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH469

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.464	1.3	ug/L	110223	1	6.248	412122	5.0