


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082923\
Data File : VU054943.D
Acq On : 29 Aug 2023 09:12
Operator : MD/SY
Sample : BFB035
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB035

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Aug 31 02:34:15 2023

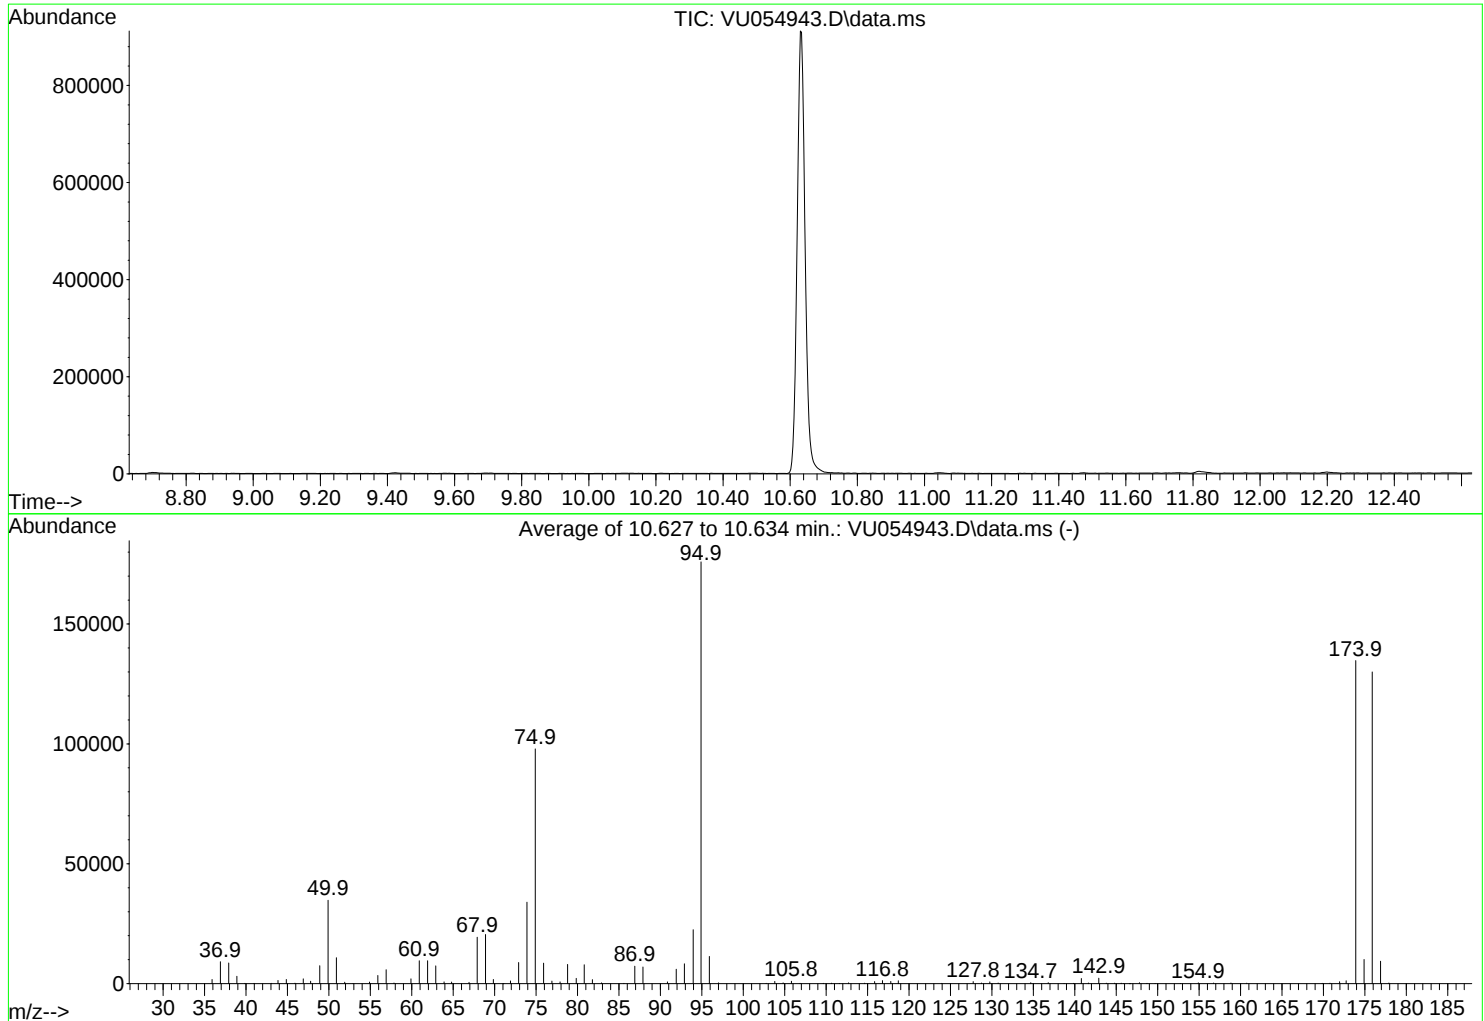

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	34781	PASS
75	95	30	80	55.6	97880	PASS
95	95	100	100	100.0	175936	PASS
96	95	5	9	6.4	11322	PASS
173	174	0.00	2	0.9	1235	PASS
174	95	50	120	76.6	134779	PASS
175	174	5	9	7.5	10078	PASS
176	174	95	101	96.4	129981	PASS
177	176	5	9	7.2	9326	PASS

m/z	Abundance
39.90	245.0
43.80	678.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	1668.0
36.90	8717.0
37.90	8026.0
38.90	3265.0
39.80	342.0
40.90	140.0
43.10	145.0
43.90	1880.0
44.90	1696.0
45.90	174.0
46.90	1998.0
47.80	905.0
48.90	7409.0
49.90	32888.0
50.90	10470.0
51.90	648.0
52.90	109.0
54.90	649.0
55.90	3468.0
56.90	5234.0
57.80	324.0
59.90	1848.0
60.90	8830.0
61.90	9140.0
62.90	7089.0
63.90	719.0
64.80	634.0
66.90	462.0
67.90	18768.0
68.90	19176.0
69.80	1630.0
71.00	108.0
71.90	1075.0
72.90	8333.0
73.90	31528.0
74.90	92296.0
75.90	8348.0
76.90	1253.0
77.90	798.0
78.80	7954.0
79.80	2164.0
80.80	7348.0
81.80	1580.0
82.90	308.0
85.60	210.0
86.90	6874.0
87.90	6634.0
90.80	680.0
91.90	5638.0
92.90	7427.0
94.00	21808.0
94.90	166272.0
95.90	11075.0
97.10	376.0
102.70	107.0
103.80	883.0
104.80	285.0
105.80	892.0
106.80	120.0
109.70	151.0
110.70	219.0
111.60	107.0
112.70	339.0
114.60	175.0
115.90	672.0
116.80	1155.0
117.80	845.0
118.70	1156.0
127.80	735.0
128.80	227.0
129.80	646.0
130.70	264.0
134.70	334.0
136.80	339.0
139.80	125.0
140.80	2105.0
141.60	189.0
142.90	2133.0
143.80	188.0
144.80	199.0
145.60	191.0
145.90	205.0
147.90	321.0
154.90	314.0
156.80	240.0
158.90	196.0
160.80	156.0
169.80	109.0
170.80	244.0
171.90	720.0
172.70	1138.0
173.90	122608.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

174.90	9235.0
175.90	119032.0
176.90	8575.0
177.90	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	1855.0
36.90	9567.0
37.90	8913.0
38.90	3201.0
39.80	359.0
40.90	126.0
43.10	145.0
43.90	2032.0
44.90	1806.0
45.90	178.0
46.90	2140.0
47.80	997.0
48.90	7688.0
49.90	35976.0
50.90	11094.0
51.90	633.0
52.90	117.0
54.90	665.0
55.90	3500.0
56.90	6085.0
57.90	284.0
59.90	2083.0
60.90	9848.0
61.90	9888.0
62.90	7641.0
63.90	772.0
64.80	720.0
66.90	531.0
67.90	20008.0
68.90	21104.0
69.90	1838.0
71.90	1213.0
72.90	9126.0
73.90	34968.0
74.90	101344.0
75.90	8784.0
76.90	1095.0
77.90	765.0
78.80	8257.0
79.90	2235.0
80.80	8187.0
81.80	1685.0
82.90	339.0
85.60	149.0
86.90	7522.0
87.90	7274.0
90.80	725.0
91.90	6232.0
92.90	8547.0
94.00	23032.0
94.90	182016.0
95.90	11660.0
97.00	368.0
102.70	119.0
103.80	1008.0
104.80	336.0
105.80	1035.0
106.80	110.0
109.60	132.0
110.70	240.0
111.60	110.0
112.70	322.0
114.70	178.0
115.90	866.0
116.80	1272.0
117.80	985.0
118.70	1226.0
124.00	133.0
127.70	856.0
128.80	254.0
129.70	816.0
130.80	277.0
134.70	472.0
136.80	439.0
138.70	117.0
139.90	146.0
140.80	2223.0
141.60	290.0
142.90	2391.0
143.80	237.0
144.80	243.0
145.60	204.0
146.60	100.0
147.80	404.0
148.70	142.0
152.70	106.0
154.90	351.0
156.70	269.0
158.90	313.0
160.70	207.0
169.90	130.0
170.80	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

171.90	833.0
172.80	1293.0
173.90	139328.0
174.90	10538.0
175.90	133632.0
176.90	9571.0
177.90	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	1726.0
36.90	9191.0
37.90	8934.0
38.90	2838.0
39.90	353.0
41.00	100.0
43.00	148.0
43.90	2122.0
44.80	1752.0
45.90	216.0
46.90	1813.0
47.80	1038.0
48.90	7261.0
49.90	35480.0
50.90	10813.0
51.90	595.0
54.90	608.0
55.90	3256.0
56.90	6062.0
57.90	210.0
59.90	2020.0
60.90	9964.0
61.90	9674.0
62.90	7473.0
63.90	727.0
64.80	722.0
66.90	547.0
67.90	19336.0
68.90	21112.0
69.90	1796.0
71.90	1217.0
72.90	9081.0
73.90	35344.0
74.90	100000.0
75.90	8446.0
76.90	952.0
77.90	652.0
78.80	7778.0
79.90	2140.0
80.80	8089.0
81.80	1753.0
82.90	315.0
86.90	7400.0
87.90	6911.0
90.90	747.0
91.90	6240.0
92.90	8915.0
93.90	22656.0
94.90	179520.0
95.90	11231.0
96.90	333.0
102.80	140.0
103.80	949.0
104.80	344.0
105.80	1046.0
106.90	121.0
109.60	100.0
110.60	203.0
112.70	284.0
114.70	178.0
115.80	990.0
116.80	1324.0
117.80	924.0
118.70	1162.0
123.90	183.0
127.70	961.0
128.70	260.0
129.70	800.0
130.80	290.0
134.70	482.0
136.80	495.0
138.70	112.0
139.90	154.0
140.80	2155.0
141.70	277.0
142.90	2364.0
143.80	291.0
144.80	261.0
145.60	209.0
147.70	413.0
148.70	197.0
149.70	131.0
152.80	110.0
154.90	362.0
156.70	272.0
158.80	351.0
160.70	203.0
169.90	116.0
170.80	123.0
172.00	819.0
172.80	1273.0
173.90	142400.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

174.90	10460.0
175.90	137280.0
176.90	9833.0
177.90	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035