


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082924\
Data File : VU060562.D
Acq On : 29 Aug 2024 09:24
Operator : MD/SY
Sample : BFB192
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB192

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Aug 29 23:12:56 2024

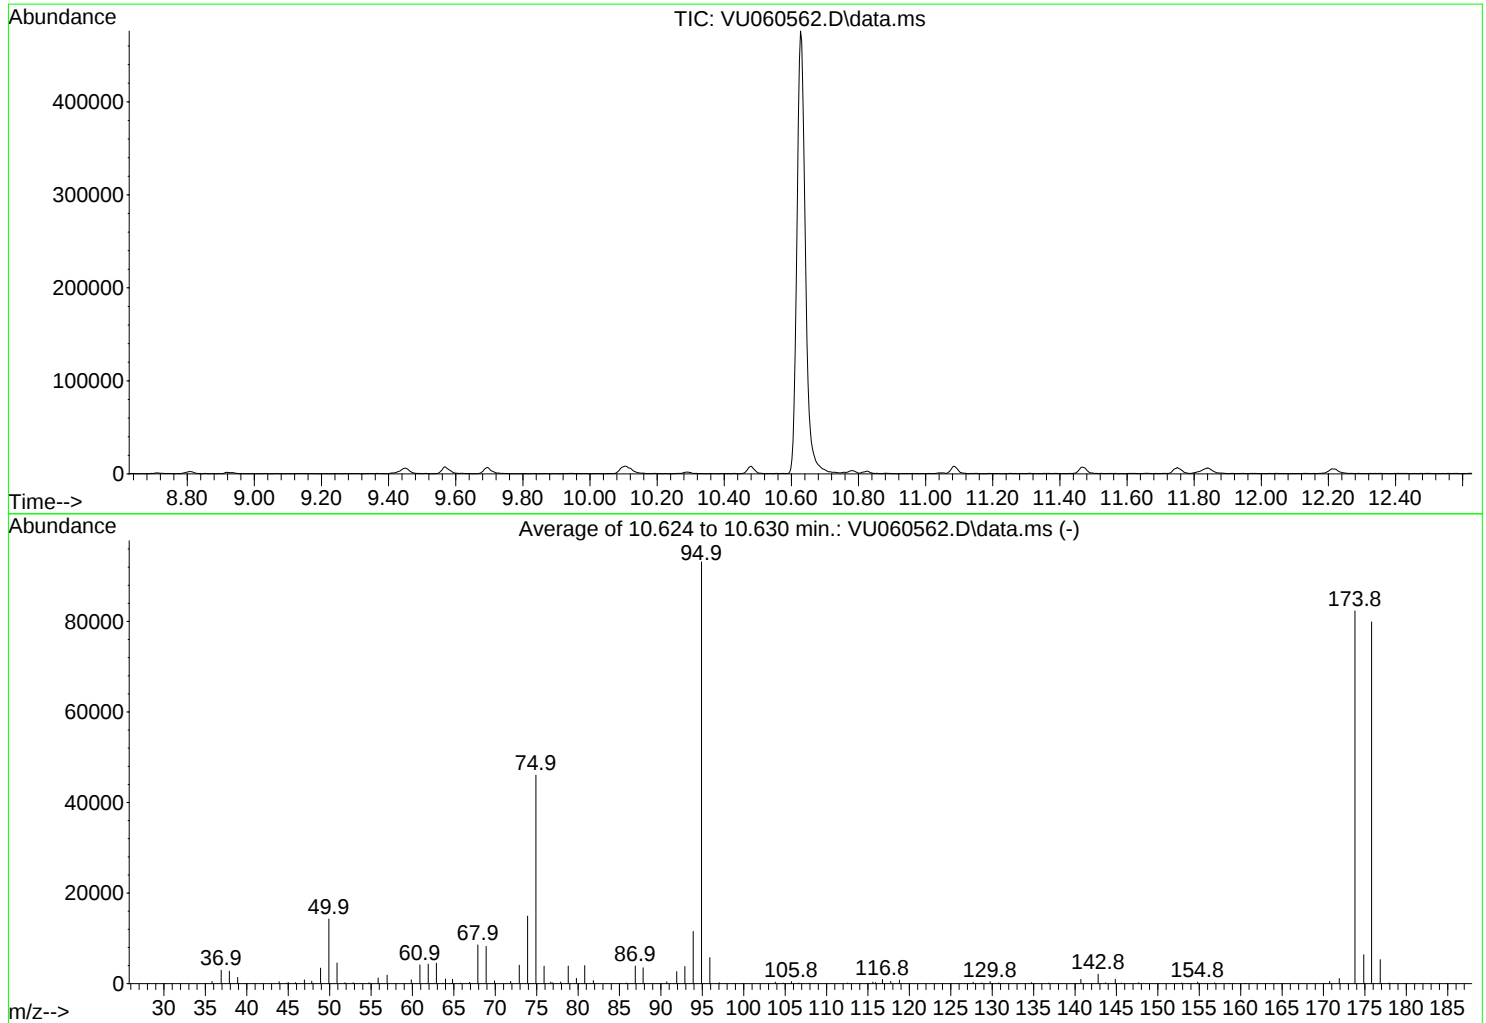

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	14278	PASS
75	95	30	80	49.4	46051	PASS
95	95	100	100	100.0	93155	PASS
96	95	5	9	6.2	5761	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.4	82352	PASS
175	174	5	9	7.7	6380	PASS
176	174	95	101	97.0	79896	PASS
177	176	5	9	6.6	5306	PASS

m/z	Abundance
39.80	122.0
43.90	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
35.80	456.0
36.90	2764.0
37.90	2711.0
38.90	1294.0
40.00	166.0
43.90	728.0
44.80	319.0
45.90	304.0
46.90	760.0
47.80	519.0
48.90	3162.0
49.90	14159.0
50.90	4483.0
51.90	218.0
52.90	140.0
54.80	199.0
55.90	1208.0
56.90	1725.0
59.80	829.0
60.90	3855.0
61.90	4052.0
62.90	4181.0
64.00	1056.0
64.80	778.0
65.80	175.0
66.90	259.0
67.90	8307.0
68.90	8227.0
69.90	620.0
71.90	585.0
72.90	3971.0
73.90	14554.0
74.90	44664.0
75.90	3751.0
76.70	507.0
77.90	337.0
78.80	3758.0
79.80	1182.0
80.80	3934.0
81.90	649.0
85.80	117.0
86.90	3718.0
87.90	3379.0
90.70	410.0
91.90	2520.0
92.90	3686.0
93.90	10486.0
94.90	90264.0
95.90	5823.0
97.00	218.0
103.80	330.0
104.70	117.0
105.80	446.0
106.70	105.0
112.50	140.0
115.70	419.0
116.80	949.0
117.70	453.0
118.80	719.0
127.70	338.0
128.70	152.0
129.70	425.0
130.80	152.0
134.80	272.0
136.80	127.0
140.70	1025.0
142.80	2058.0
143.70	190.0
144.90	971.0
145.60	130.0
147.70	179.0
152.90	146.0
154.80	294.0
156.80	188.0
158.70	127.0
160.60	149.0
170.80	533.0
171.90	1066.0
173.80	78600.0
174.90	5929.0
175.80	76552.0
176.90	5055.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
35.80	530.0
36.90	3040.0
37.90	2843.0
38.90	1435.0
40.00	196.0
43.90	716.0
45.00	342.0
45.90	241.0
46.90	831.0
47.90	537.0
48.90	3566.0
49.90	14726.0
50.90	4681.0
51.90	197.0
52.90	228.0
54.80	205.0
55.80	1323.0
56.90	1890.0
59.80	862.0
60.90	4283.0
61.90	4371.0
62.90	4703.0
64.00	1083.0
64.80	942.0
65.80	178.0
66.90	297.0
67.90	8825.0
68.90	8416.0
69.90	643.0
71.90	482.0
72.90	4209.0
73.90	15349.0
74.90	47688.0
75.90	3933.0
76.70	523.0
77.90	376.0
78.80	4021.0
79.80	1216.0
80.80	4133.0
81.90	680.0
85.80	147.0
86.90	4012.0
87.90	3579.0
90.70	435.0
91.90	2765.0
92.90	3839.0
93.90	12008.0
94.90	95800.0
95.90	5891.0
97.10	221.0
103.80	362.0
104.80	143.0
105.70	489.0
106.70	176.0
107.90	122.0
112.60	142.0
114.90	112.0
115.60	370.0
115.90	371.0
116.70	915.0
117.80	506.0
118.80	803.0
127.70	306.0
128.80	173.0
129.80	489.0
130.80	166.0
134.70	256.0
136.80	153.0
140.70	1030.0
142.80	2156.0
143.70	224.0
144.80	999.0
145.60	136.0
147.70	219.0
152.90	140.0
153.60	106.0
154.80	368.0
156.80	166.0
158.70	128.0
160.60	114.0
170.80	491.0
171.90	1144.0
173.80	84336.0
174.90	6654.0
175.80	82496.0
176.80	5555.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
35.80	552.0
36.90	3125.0
37.90	2709.0
38.90	1373.0
40.00	186.0
43.90	620.0
45.00	411.0
45.90	206.0
47.00	877.0
47.90	505.0
48.90	3565.0
49.90	13949.0
50.90	4573.0
51.80	237.0
52.80	240.0
53.70	119.0
54.70	194.0
55.80	1308.0
57.00	1983.0
59.90	841.0
60.90	4266.0
61.90	4493.0
62.90	4741.0
64.00	985.0
64.90	1134.0
65.80	100.0
66.90	274.0
67.90	8477.0
68.90	8097.0
69.90	562.0
71.80	374.0
72.90	4034.0
73.90	14874.0
74.90	45800.0
75.90	3881.0
76.90	551.0
77.90	384.0
78.80	3889.0
79.80	1081.0
80.80	3880.0
81.80	677.0
85.80	159.0
86.90	3932.0
87.80	3509.0
90.70	382.0
91.90	2657.0
92.90	3810.0
93.90	12059.0
94.90	93400.0
95.90	5569.0
97.10	219.0
103.80	369.0
104.70	151.0
105.70	486.0
106.60	173.0
107.90	173.0
112.60	108.0
114.90	106.0
115.50	326.0
115.90	349.0
116.70	852.0
117.80	532.0
118.80	824.0
127.70	291.0
128.80	186.0
129.80	437.0
130.80	195.0
134.70	205.0
136.80	172.0
140.70	855.0
142.80	2067.0
143.70	226.0
144.80	1009.0
145.60	121.0
145.90	125.0
147.70	242.0
152.80	114.0
154.80	371.0
156.90	148.0
170.70	416.0
171.90	1175.0
173.80	84120.0
174.80	6557.0
175.80	80640.0
176.80	5307.0
177.90	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192