

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026443.D
 Acq On : 30 Aug 2018 13:49
 Operator : MD/SY
 Sample : J4691-09 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 31 04:24:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 31 04:22:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	149186	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	138795	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	59904	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	46621	50.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.88%
7) Chloroethane-d5	1.68	69	40546	48.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.14%
11) 1,1-Dichloroethene-d2	2.27	63	72791	34.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.94%
21) 2-Butanone-d5	4.18	46	68628	95.66	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.66%
24) Chloroform-d	4.65	84	79091	45.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	5.31	65	55331	47.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.22%
32) Benzene-d6	5.34	84	160767	50.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.50%
36) 1,2-Dichloropropane-d6	6.33	67	55269	50.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.58%
41) Toluene-d8	7.57	98	144799	46.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.78%
43) trans-1,3-Dichloropropene-	7.85	79	23404	46.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.28%
47) 2-Hexanone-d5	8.31	63	49070	97.36	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	75583	46.68	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.36%
64) 1,2-Dichlorobenzene-d4	11.86	152	58114	53.47	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.94%

Target Compounds


					Ovalue
35) Methylcyclohexane	6.34	83	12331	7.912 ug/L #	18
37) 1,2-Dichloropropane	6.33	63	5954	5.405 ug/L #	88
46) Tetrachloroethene	8.23	164	7350	9.007 ug/L	95
49) Dibromochloromethane	8.23	129	6773	5.957 ug/L #	10
59) 1,2,3-Trichloropropane	11.48	75	7030	5.115 ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026443.D
Acq On : 30 Aug 2018 13:49
Operator : MD/SY
Sample : J4691-09 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 31 04:24:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 31 04:22:30 2018
Response via : Initial Calibration

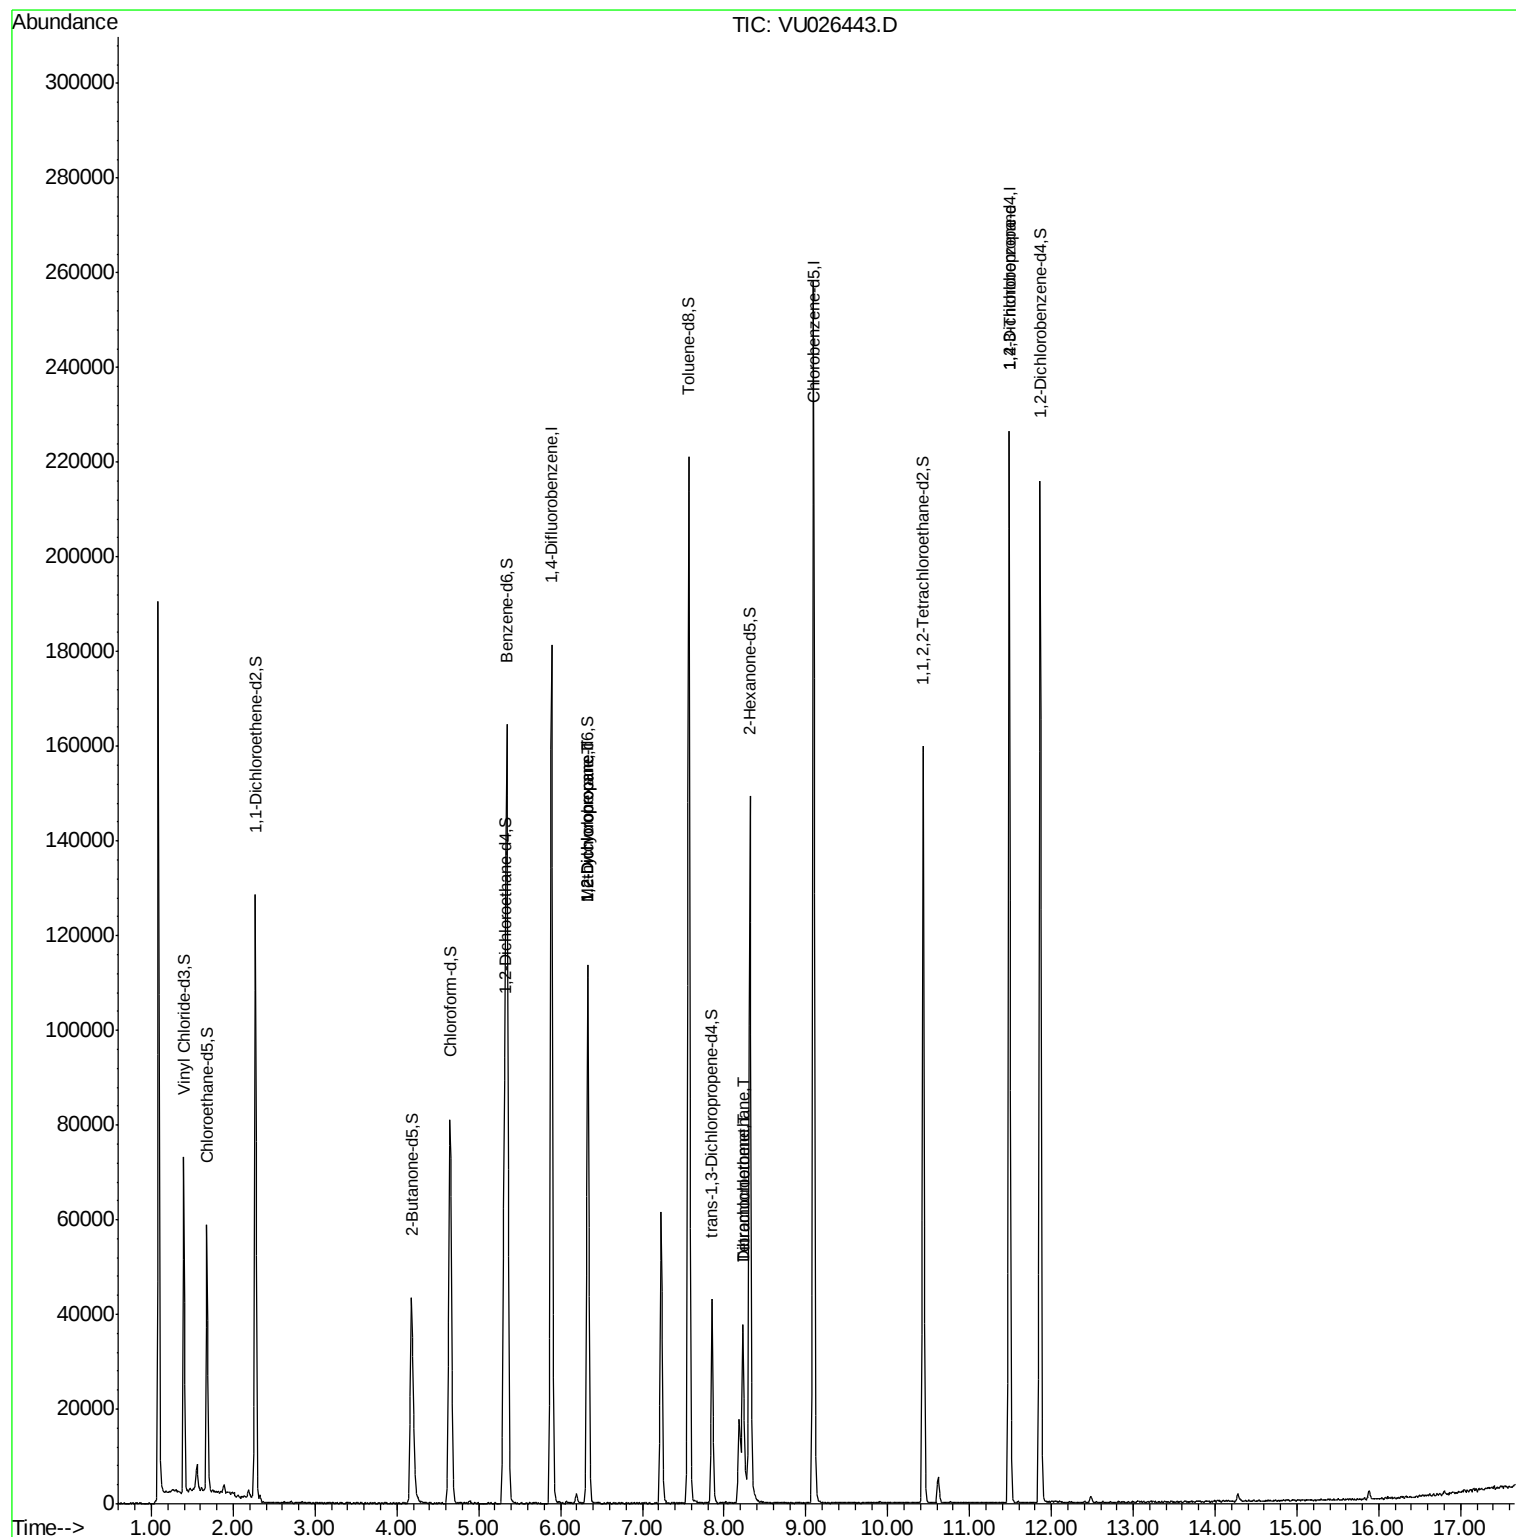


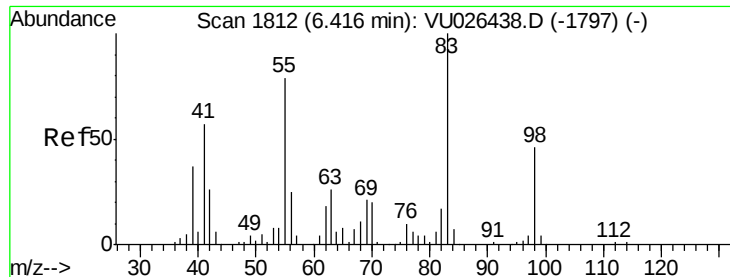




#35
Methvlcvclohexane
Concen: 7.912 ug/L
RT: 6.34 min Scan# 1787
Delta R.T. -0.08 min
Lab File: VU026443.D
Acq: 30 Aug 2018 13:49

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion	83	Resp	12331
Ion Ratio	Lower	Upper	
83	100		
55	0.0	63.3	94.9#
98	0.8	36.7	55.1#

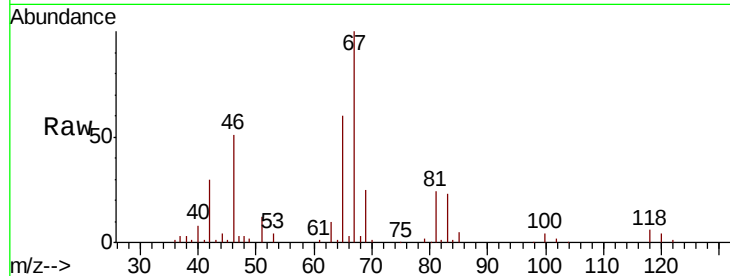


Abundance Ion 83.00 (82.70 to 83.70): VU0
Ion 55.00 (54.70 to 55.70): VU0
Ion 98.00 (97.70 to 98.70): VU0

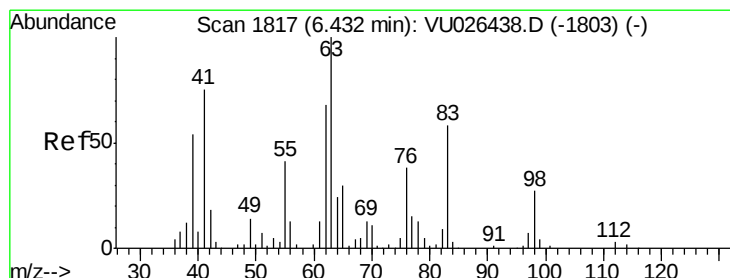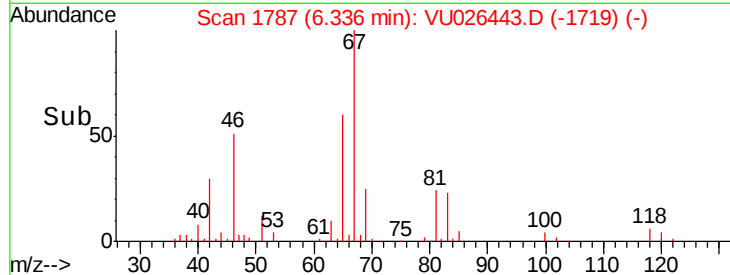
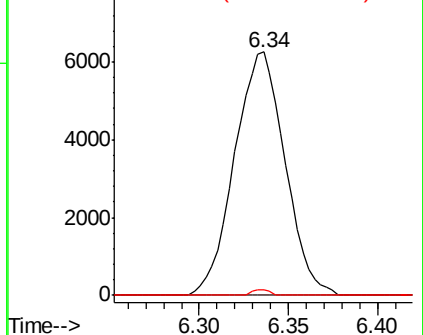



#37
1,2-Dichloropropane
Concen: 5.405 ug/L
RT: 6.33 min Scan# 1786
Delta R.T. -0.10 min
Lab File: VU026443.D
Acq: 30 Aug 2018 13:49

Tgt Ion	63	Resp	5954
Ion Ratio	Lower	Upper	
63	100		
112	0.0	3.0	4.6#

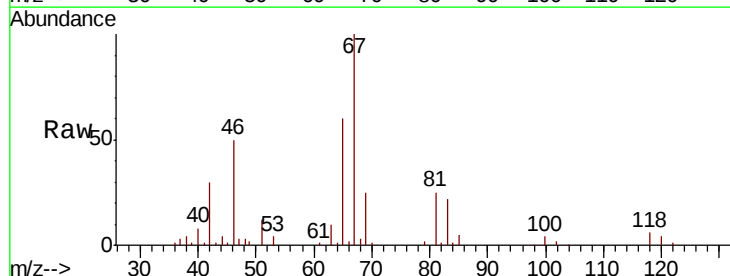

Abundance Ion 63.00 (62.70 to 63.70): VU0
Ion 112.00 (111.70 to 112.70): V

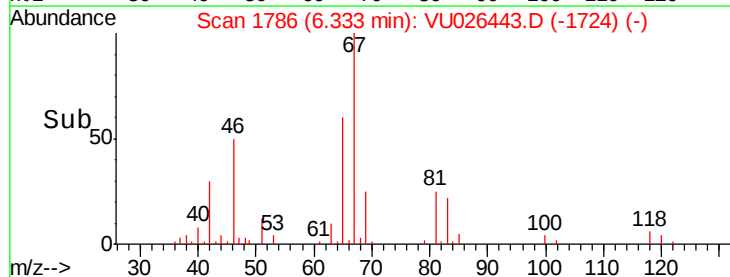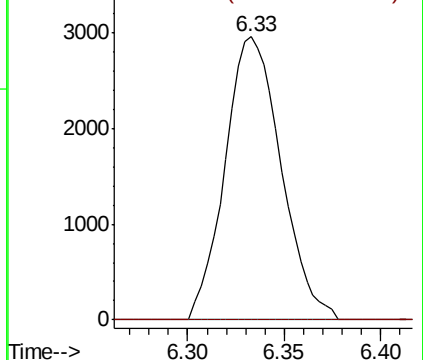


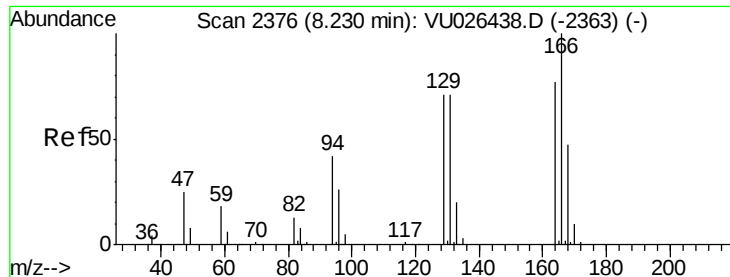




#46
Tetrachloroethene
Concen: 9.007 ug/L
RT: 8.23 min Scan# 2376
Delta R.T. 0.00 min
Lab File: VU026443.D
Acq: 30 Aug 2018 13:49

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion:164 Resp: 7350
Ion Ratio Lower Upper
164 100
129 89.2 67.3 125.1
131 87.7 65.3 121.3
166 133.2 90.9 168.7

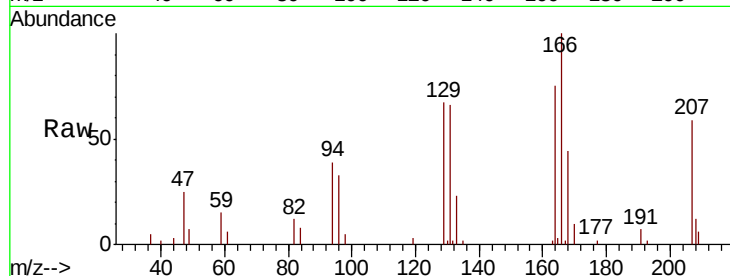


Abundance Ion 164.00 (163.70 to 164.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V
Ion 166.00 (165.70 to 166.70): V

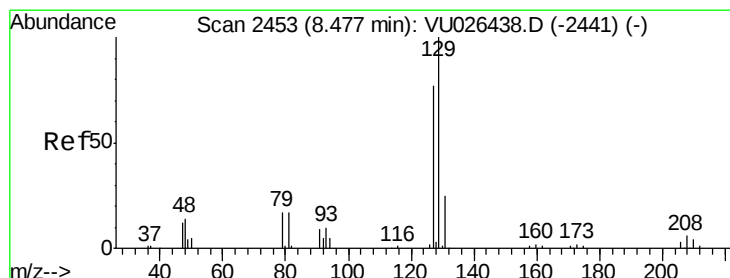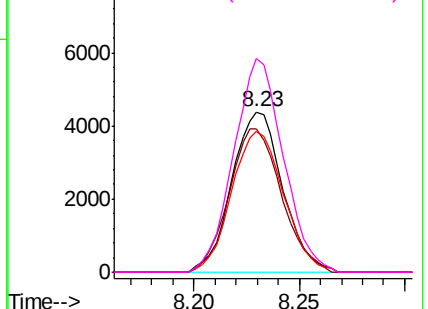
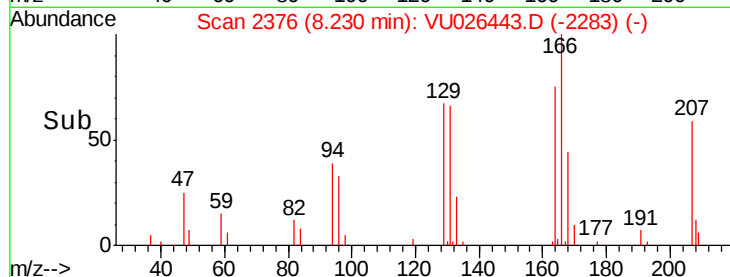



#49
Dibromochloromethane
Concen: 5.957 ug/L
RT: 8.23 min Scan# 2375
Delta R.T. -0.25 min
Lab File: VU026443.D
Acq: 30 Aug 2018 13:49

Tgt Ion:129 Resp: 6773
Ion Ratio Lower Upper
129 100
127 0.0 55.0 102.2#

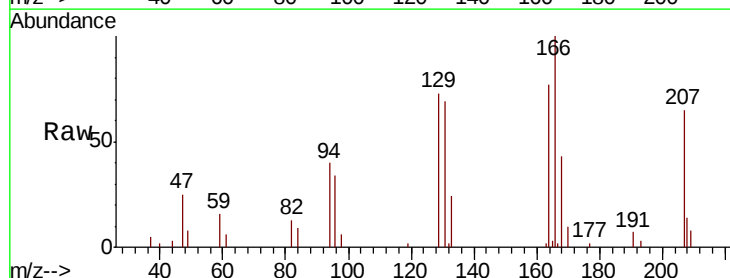

Abundance Ion 129.00 (128.70 to 129.70): V
Ion 127.00 (126.70 to 127.70): V

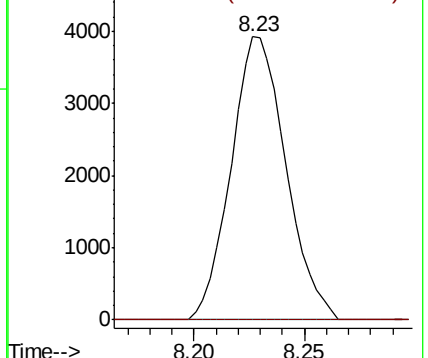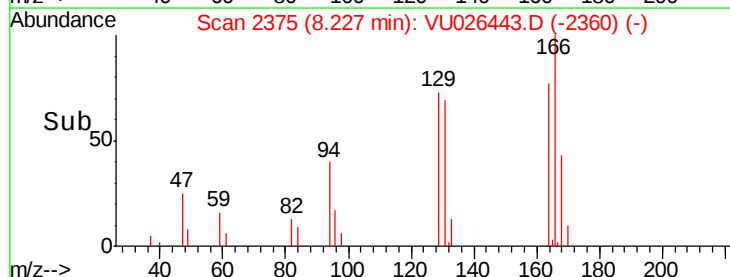

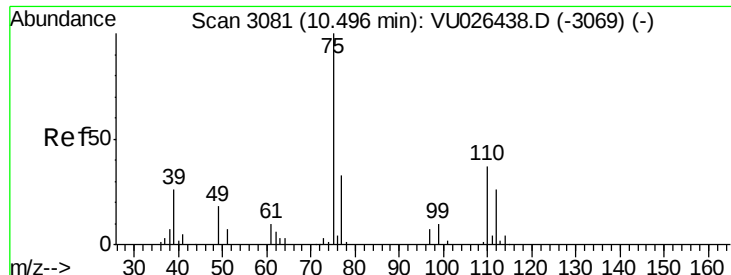

#59

1,2,3-Trichloropropane

Concen: 5.115 ug/L

RT: 11.48 min Scan# 3388

Delta R.T. 0.99 min

Lab File: VU026443.D

Acq: 30 Aug 2018 13:49

Instrument :

MSVOA_U

ClientSampleId :

Tot Ion: 75 Resp: 7030

Ion Ratio Lower Upper

75 100

77 38.4 25.0 37.6#

