

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026454.D
 Acq On : 30 Aug 2018 18:07
 Operator : MD/SY
 Sample : J4691-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE17

Quant Time: Aug 31 05:16:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 31 04:22:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	140686	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	132468	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	56114	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	42603	48.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.76%
7) Chloroethane-d5	1.68	69	37786	48.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.27	63	61128	31.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.28%
21) 2-Butanone-d5	4.18	46	67470	99.73	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.73%
24) Chloroform-d	4.65	84	76094	46.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.44%
26) 1,2-Dichloroethane-d4	5.31	65	51443	46.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.86%
32) Benzene-d6	5.35	84	151724	49.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.38%
36) 1,2-Dichloropropane-d6	6.33	67	51391	49.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.00%
41) Toluene-d8	7.57	98	136412	46.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.56%
43) trans-1,3-Dichloropropene-	7.85	79	22278	46.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.02%
47) 2-Hexanone-d5	8.31	63	47662	99.08	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.08%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	73449	47.53	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.06%
64) 1,2-Dichlorobenzene-d4	11.86	152	53572	52.62	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.24%


Target Compounds					Ovalue
46) Tetrachloroethene	8.23	164	3968	5.09 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026454.D
Acq On : 30 Aug 2018 18:07
Operator : MD/SY
Sample : J4691-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE17

Quant Time: Aug 31 05:16:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 31 04:22:30 2018
Response via : Initial Calibration

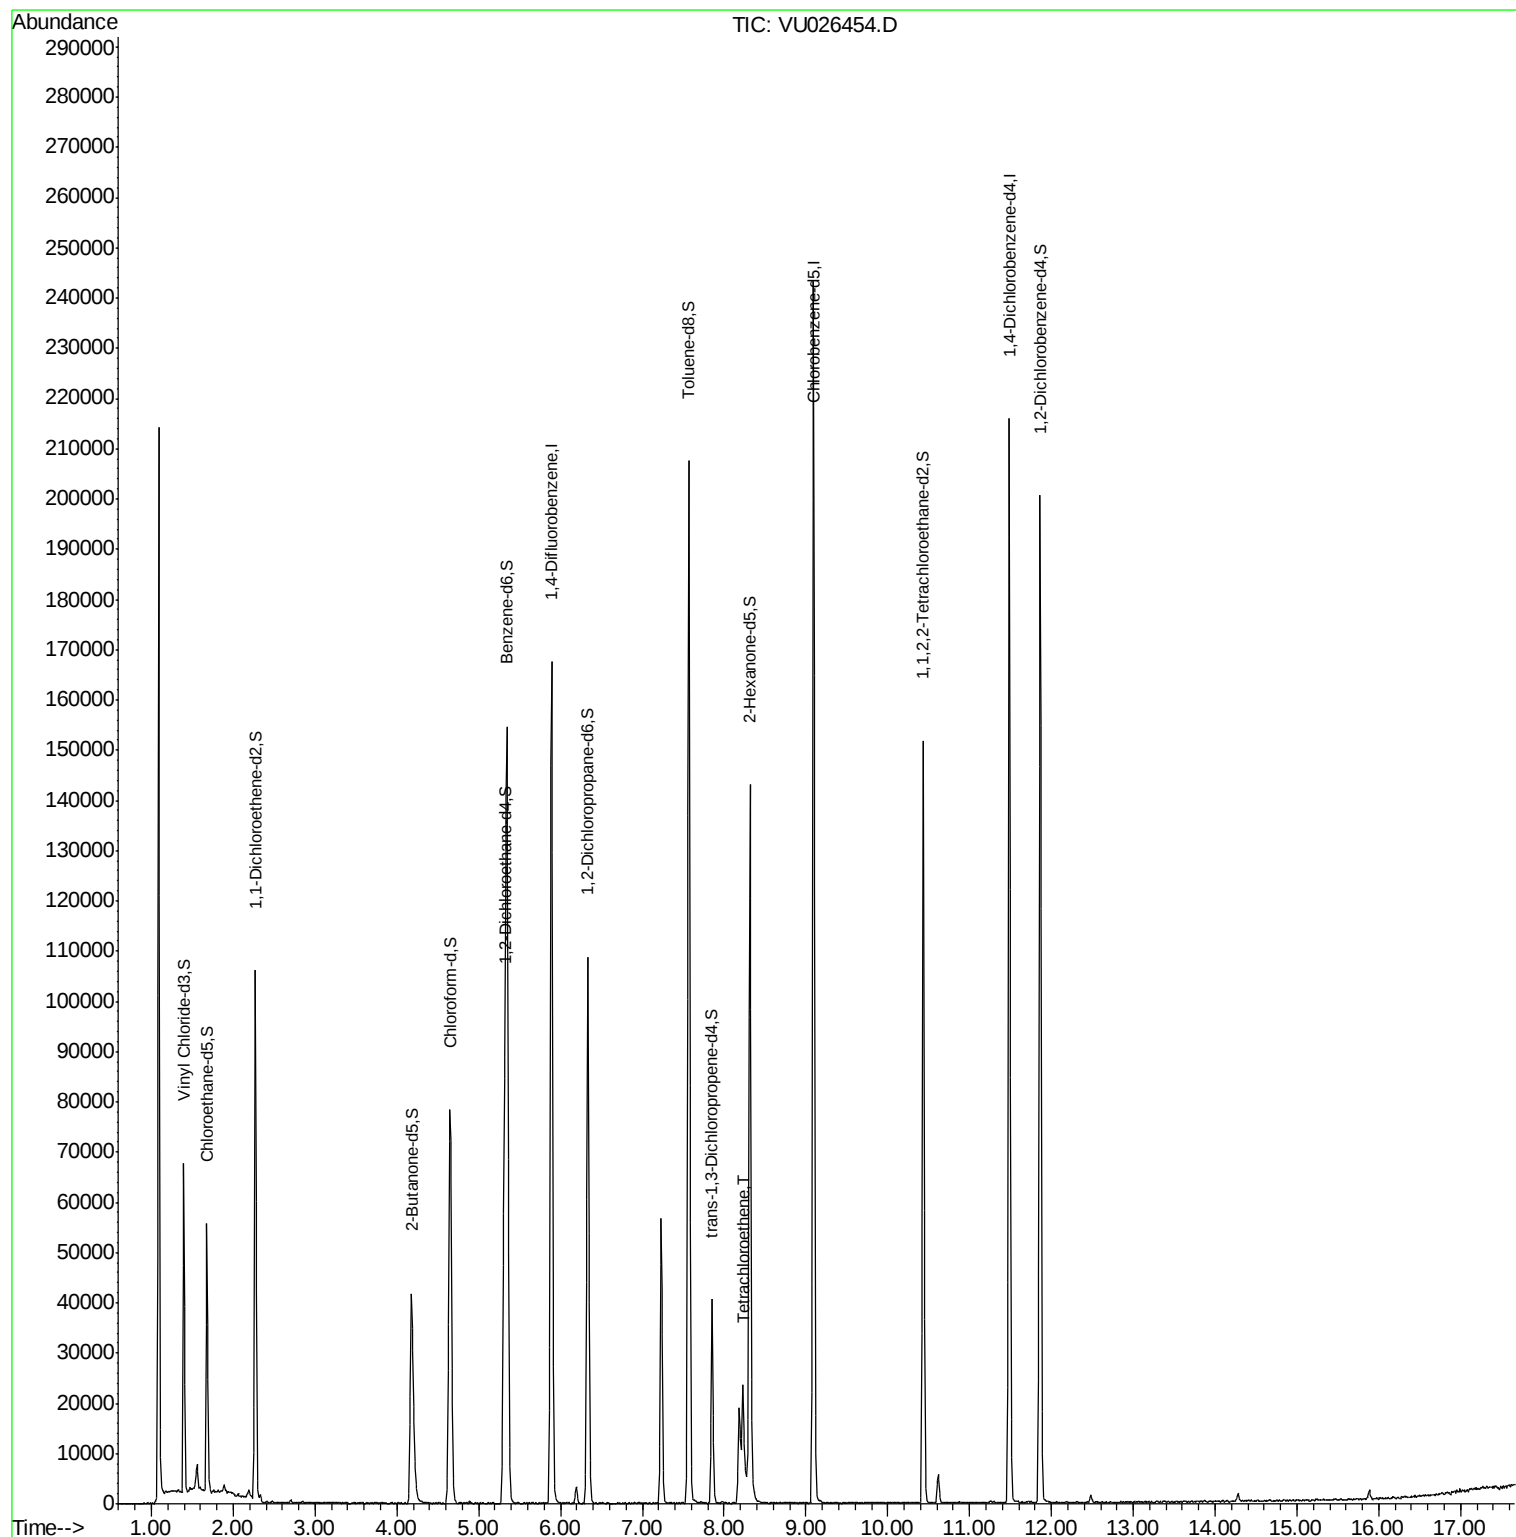

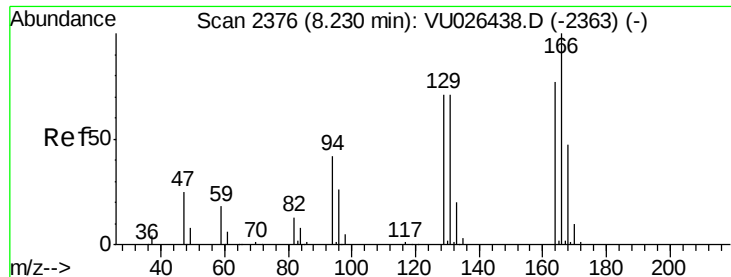

#46

Tetrachloroethene

Concen: 5.09 ug/L


RT: 8.23 min Scan# 2376

Delta R.T. -0.00 min

Lab File: VU026454.D

Acq: 30 Aug 2018 18:07

Instrument :
MSVOA_U
ClientSampleId :
BEE17

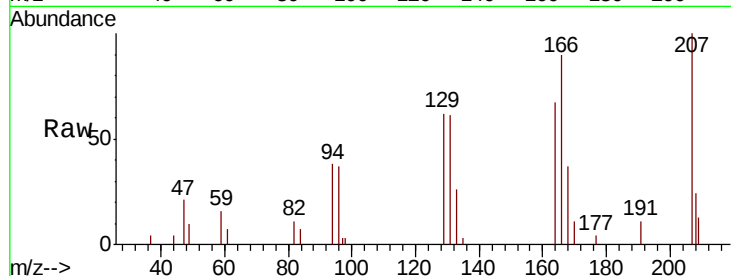

Tot Ion:164 Resp: 3968

Ion Ratio Lower Upper

164 100

129 92.1 67.3 125.1

131 90.7 65.3 121.3

166 134.3 90.9 168.7

Abundance Ion 164.00 (163.70 to 164.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V
Ion 166.00 (165.70 to 166.70): V

