

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026460.D
 Acq On : 30 Aug 2018 20:26
 Operator : MD/SY
 Sample : J4694-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.802	63	66	69	rBB	123	112	0.002%	0.0002%
2	0.979	119	121	124	rVV	143	122	0.003%	0.0003%
3	1.085	140	154	177	rBV	187432	214788	45.03%	4.752%
4	1.397	244	251	263	rBV	63743	67025	14.05%	1.483%
5	1.677	330	338	351	rVB	51715	68490	14.36%	1.515%
6	2.268	512	522	536	rVV	97783	149078	31.25%	3.298%
7	2.329	536	541	547	rVB4	1273	1679	0.35%	0.0037%
8	2.436	571	574	576	rBV	178	110	0.002%	0.0002%
9	2.474	584	586	592	rVB	220	151	0.003%	0.0003%
10	2.616	627	630	635	rVB2	229	208	0.004%	0.0005%
11	2.699	649	656	662	rVB2	721	1006	0.21%	0.0022%
12	2.834	690	698	710	rBV3	1214	2687	0.56%	0.0059%
13	3.252	821	828	832	rBV	152	270	0.006%	0.0006%
14	3.278	832	836	839	rBV2	333	311	0.007%	0.0007%
15	3.513	906	909	912	rVB2	281	228	0.005%	0.0005%
16	3.548	917	920	926	rVB	196	113	0.002%	0.0003%
17	3.635	943	947	949	rBV	198	107	0.002%	0.0002%
18	3.789	992	995	998	rBV	139	145	0.003%	0.0003%
19	4.001	1058	1061	1065	rVB	158	98	0.002%	0.0002%
20	4.178	1101	1116	1148	rBV2	44268	137236	28.77%	3.036%
21	4.355	1168	1171	1175	rVV2	235	194	0.004%	0.0004%
22	4.423	1190	1192	1195	rVB	200	131	0.003%	0.0003%
23	4.439	1195	1197	1201	rBB	147	119	0.002%	0.0003%
24	4.461	1201	1204	1207	rBV	129	135	0.003%	0.0003%
25	4.535	1223	1227	1228	rBV	222	134	0.003%	0.0003%
26	4.648	1245	1262	1283	rBV	76263	182087	38.17%	4.029%
27	4.789	1300	1306	1308	rBV2	182	224	0.005%	0.0005%
28	4.879	1331	1334	1336	rVV	246	160	0.003%	0.0004%
29	4.892	1336	1338	1342	rVB2	260	170	0.004%	0.0004%
30	4.940	1350	1353	1355	rBV	126	113	0.002%	0.0003%
31	4.972	1361	1363	1365	rVB	237	96	0.002%	0.0002%
32	5.040	1381	1384	1388	rBV	149	180	0.004%	0.0004%
33	5.085	1396	1398	1403	rBV	141	168	0.004%	0.0004%
34	5.207	1433	1436	1438	rBV	171	134	0.003%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026460.D
 Acq On : 30 Aug 2018 20:26
 Operator : MD/SY
 Sample : J4694-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.342	1454	1478	1496	rBV2	155070	453462	95.06%	10.033%
36	5.516	1526	1532	1537	rBV	182	302	0.06%	0.007%
37	5.812	1622	1624	1630	rVB	108	94	0.02%	0.002%
38	5.889	1633	1648	1669	rBV	178687	344497	72.22%	7.622%
39	6.001	1680	1683	1685	rBV	107	96	0.02%	0.002%
40	6.088	1707	1710	1711	rBV	210	105	0.02%	0.002%
41	6.188	1730	1741	1758	rVB	31150	58411	12.25%	1.292%
42	6.332	1772	1786	1804	rBV	108842	212565	44.56%	4.703%
43	6.455	1822	1824	1830	rVB	262	200	0.04%	0.004%
44	6.487	1831	1834	1836	rBV	121	109	0.02%	0.002%
45	6.670	1887	1891	1893	rBV	163	161	0.03%	0.004%
46	6.985	1986	1989	1994	rBV	157	199	0.04%	0.004%
47	7.230	2053	2065	2082	rBV2	56574	99283	20.81%	2.197%
48	7.310	2088	2090	2094	rVB	183	114	0.02%	0.003%
49	7.442	2128	2131	2132	rBV	134	96	0.02%	0.002%
50	7.513	2150	2153	2155	rBV	161	131	0.03%	0.003%
51	7.567	2156	2170	2186	rVV	209457	357128	74.87%	7.902%
52	7.786	2235	2238	2239	rBV	147	108	0.02%	0.002%
53	7.850	2247	2258	2276	rBV	40918	66839	14.01%	1.479%
54	7.950	2284	2289	2292	rBV2	263	265	0.06%	0.006%
55	7.982	2298	2299	2302	rVB	260	121	0.03%	0.003%
56	8.184	2349	2362	2365	rVV	19163	31281	6.56%	0.692%
57	8.230	2366	2376	2391	rVV	274290	477013	100.00%	10.554%
58	8.313	2392	2402	2419	rVB	141643	240774	50.48%	5.327%
59	8.458	2446	2447	2450	rBV	221	94	0.02%	0.002%
60	8.615	2491	2496	2499	rBV2	294	315	0.07%	0.007%
61	8.757	2536	2540	2543	rBV	193	122	0.03%	0.003%
62	8.934	2593	2595	2600	rVB2	134	94	0.02%	0.002%
63	9.091	2632	2644	2665	rBV	256601	414304	86.85%	9.167%
64	9.426	2746	2748	2752	rVB	176	116	0.02%	0.003%
65	9.895	2889	2894	2897	rBV	114	129	0.03%	0.003%
66	9.982	2916	2921	2924	rBV2	221	199	0.04%	0.004%
67	10.432	3049	3061	3079	rBV	148687	237170	49.72%	5.248%
68	10.512	3082	3086	3087	rBV	207	127	0.03%	0.003%
69	10.615	3107	3118	3130	rBV2	5607	10808	2.27%	0.239%
70	10.879	3196	3200	3203	rVB2	168	185	0.04%	0.004%
71	10.924	3211	3214	3220	rBV	108	131	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026460.D
 Acq On : 30 Aug 2018 20:26
 Operator : MD/SY
 Sample : J4694-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	11.168	3286	3290	3293	rBV	156	127	0.03%	0.003%
73	11.483	3377	3388	3403	rBV	228339	353675	74.14%	7.825%
74	11.715	3457	3460	3463	rVB2	170	101	0.02%	0.002%
75	11.799	3483	3486	3489	rBV2	166	131	0.03%	0.003%
76	11.863	3494	3506	3521	rBV	205494	321386	67.37%	7.111%
77	12.017	3550	3554	3558	rVB2	316	193	0.04%	0.004%
78	12.397	3669	3672	3673	rBV	140	95	0.02%	0.002%
79	12.480	3690	3698	3707	rVB3	1385	2179	0.46%	0.048%
80	12.651	3748	3751	3754	rVB	227	132	0.03%	0.003%
81	12.689	3760	3763	3766	rBV	207	173	0.04%	0.004%
82	12.725	3771	3774	3777	rBV2	208	172	0.04%	0.004%
83	13.020	3862	3866	3869	rBV2	330	224	0.05%	0.005%
84	13.075	3879	3883	3887	rVB2	291	267	0.06%	0.006%
85	13.216	3924	3927	3931	rVB2	199	155	0.03%	0.003%
86	13.316	3954	3958	3963	rVB3	261	255	0.05%	0.006%
87	13.560	4032	4034	4036	rBV	204	103	0.02%	0.002%
88	13.676	4068	4070	4076	rBV	211	123	0.03%	0.003%
89	13.737	4087	4089	4096	rVB2	239	248	0.05%	0.005%
90	13.782	4096	4103	4106	rBV2	360	417	0.09%	0.009%
91	13.811	4109	4112	4118	rVV3	270	255	0.05%	0.006%
92	13.837	4118	4120	4122	rBV	203	115	0.02%	0.003%
93	13.850	4122	4124	4126	rVB	283	139	0.03%	0.003%
94	13.869	4126	4130	4134	rBV2	259	251	0.05%	0.006%
95	13.905	4136	4141	4143	rBV	235	223	0.05%	0.005%
96	13.995	4166	4169	4171	rBV2	230	179	0.04%	0.004%
97	14.059	4188	4189	4193	rBV3	241	199	0.04%	0.004%
98	14.281	4252	4258	4266	rVB3	1644	2402	0.50%	0.053%
99	14.480	4317	4320	4323	rBV2	231	228	0.05%	0.005%
100	16.123	4829	4831	4837	rBV	429	314	0.07%	0.007%


Sum of corrected areas: 4519618

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026460.D
Acq On : 30 Aug 2018 20:26
Operator : MD/SY
Sample : J4694-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

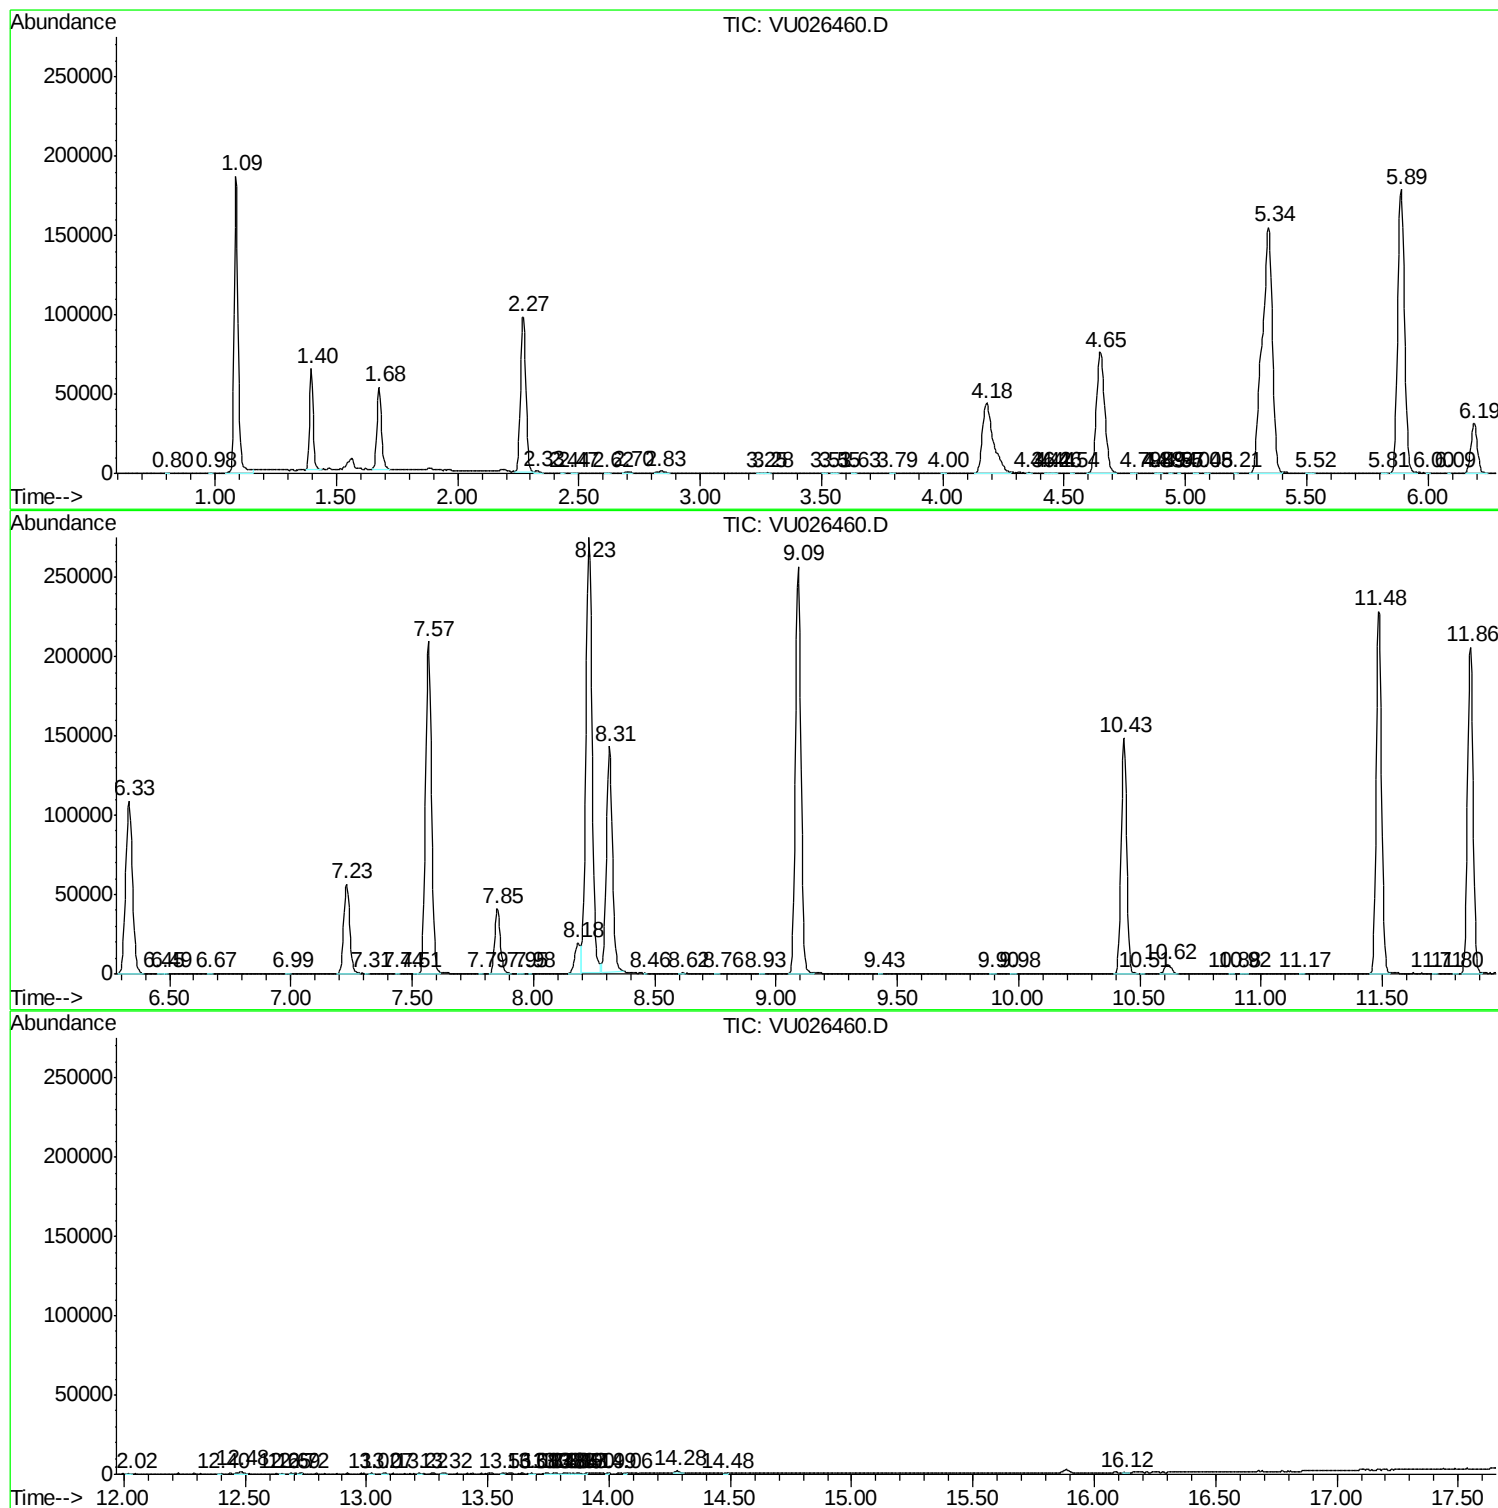

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026460.D
Acq On : 30 Aug 2018 20:26
Operator : MD/SY
Sample : J4694-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026460.D
Acq On : 30 Aug 2018 20:26
Operator : MD/SY
Sample : J4694-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc