

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026481.D
 Acq On : 31 Aug 2018 04:56
 Operator : MD/SY
 Sample : J4694-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.731	41	44	47	rBB	136	117	0.003%	0.0003%
2	0.757	51	52	55	rVB	220	104	0.002%	0.0003%
3	1.027	133	136	138	rBV	129	113	0.003%	0.0003%
4	1.088	138	155	179	rBV	171928	201151	44.78%	4.960%
5	1.397	244	251	262	rBV	60981	62795	13.98%	1.548%
6	1.680	331	339	354	rVB	51203	65745	14.63%	1.621%
7	2.272	512	523	536	rVB	99247	151229	33.66%	3.729%
8	2.481	585	588	591	rBV2	176	107	0.002%	0.0003%
9	2.587	619	621	624	rVV2	188	114	0.003%	0.0003%
10	2.616	628	630	636	rVB2	262	280	0.006%	0.0007%
11	2.706	651	658	664	rVB3	907	1243	0.28%	0.0031%
12	2.773	676	679	682	rBV	177	115	0.003%	0.0003%
13	2.841	690	700	710	rBV3	1047	2110	0.47%	0.0052%
14	3.120	782	787	791	rBV	317	315	0.007%	0.0008%
15	3.796	994	997	1001	rBV	148	180	0.004%	0.0004%
16	3.850	1010	1014	1015	rBV	248	173	0.004%	0.0004%
17	4.178	1101	1116	1151	rBV3	42307	140708	31.32%	3.470%
18	4.352	1168	1170	1173	rVB	226	113	0.003%	0.0003%
19	4.477	1206	1209	1212	rVB	195	149	0.003%	0.0004%
20	4.506	1212	1218	1225	rBB	175	339	0.008%	0.0008%
21	4.548	1226	1231	1233	rBV	146	171	0.004%	0.0004%
22	4.651	1246	1263	1290	rBV2	75603	182262	40.57%	4.494%
23	4.802	1307	1310	1313	rVV2	244	180	0.004%	0.0004%
24	4.821	1314	1316	1324	rVB2	170	239	0.005%	0.0006%
25	4.886	1332	1336	1338	rBV3	228	155	0.003%	0.0004%
26	4.921	1345	1347	1349	rBV	231	127	0.003%	0.0003%
27	5.133	1410	1413	1416	rBB	131	116	0.003%	0.0003%
28	5.159	1417	1421	1424	rBV	141	166	0.004%	0.0004%
29	5.217	1434	1439	1442	rBV	149	189	0.004%	0.0005%
30	5.342	1455	1478	1498	rBV3	153435	449241	100.00%	11.078%
31	5.413	1499	1500	1505	rVB2	334	208	0.005%	0.0005%
32	5.628	1564	1567	1572	rBB	168	184	0.004%	0.0005%
33	5.654	1572	1575	1578	rBV	149	143	0.003%	0.0004%
34	5.805	1618	1622	1627	rBV	165	253	0.006%	0.0006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026481.D
 Acq On : 31 Aug 2018 04:56
 Operator : MD/SY
 Sample : J4694-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.841	1630	1633	1634	rBV	151	108	0.02%	0.003%
36	5.889	1634	1648	1671	rBV	187587	362099	80.60%	8.929%
37	6.082	1705	1708	1710	rBV	173	140	0.03%	0.003%
38	6.095	1710	1712	1717	rVB2	250	222	0.05%	0.005%
39	6.188	1731	1741	1756	rBV2	23298	42690	9.50%	1.053%
40	6.332	1771	1786	1807	rBB	108365	210735	46.91%	5.196%
41	6.551	1852	1854	1860	rBV	169	204	0.05%	0.005%
42	6.648	1881	1884	1886	rBV	261	211	0.05%	0.005%
43	6.680	1890	1894	1896	rBV	137	142	0.03%	0.004%
44	6.783	1922	1926	1930	rBV	172	214	0.05%	0.005%
45	6.988	1987	1990	1992	rBV	146	122	0.03%	0.003%
46	7.059	2008	2012	2013	rBV	154	126	0.03%	0.003%
47	7.130	2032	2034	2036	rBV	145	105	0.02%	0.003%
48	7.230	2054	2065	2080	rVV	54910	94995	21.15%	2.342%
49	7.567	2157	2170	2189	rVV	205308	351507	78.24%	8.668%
50	7.850	2248	2258	2275	rBV	39214	63700	14.18%	1.571%
51	7.940	2283	2286	2289	rBV2	133	108	0.02%	0.003%
52	7.988	2298	2301	2304	rVB	283	166	0.04%	0.004%
53	8.069	2324	2326	2329	rVB	290	144	0.03%	0.004%
54	8.098	2329	2335	2338	rBV	162	250	0.06%	0.006%
55	8.184	2346	2362	2369	rBV	24651	50256	11.19%	1.239%
56	8.313	2392	2402	2428	rVB	136351	234270	52.15%	5.777%
57	8.451	2443	2445	2448	rVB2	275	146	0.03%	0.004%
58	8.561	2476	2479	2482	rVB	154	110	0.02%	0.003%
59	9.091	2631	2644	2661	rBV	270362	435970	97.05%	10.750%
60	9.184	2671	2673	2677	rVB2	327	143	0.03%	0.004%
61	10.210	2988	2992	2999	rBV	91	118	0.03%	0.003%
62	10.432	3050	3061	3078	rBV	147043	232344	51.72%	5.729%
63	10.538	3090	3094	3096	rBV2	167	149	0.03%	0.004%
64	10.615	3106	3118	3130	rBV	6954	12960	2.88%	0.320%
65	10.663	3130	3133	3135	rBV2	245	182	0.04%	0.004%
66	10.754	3157	3161	3164	rBV	142	141	0.03%	0.003%
67	10.808	3175	3178	3184	rVB2	285	201	0.04%	0.005%
68	10.840	3184	3188	3191	rBV	222	248	0.06%	0.006%
69	10.876	3196	3199	3200	rBV	215	141	0.03%	0.003%
70	10.991	3230	3235	3238	rBV	203	190	0.04%	0.005%
71	11.059	3253	3256	3257	rBV	182	108	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026481.D
 Acq On : 31 Aug 2018 04:56
 Operator : MD/SY
 Sample : J4694-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	11.123	3274	3276	3280	rVV2	177	111	0.02%	0.003%
73	11.155	3283	3286	3293	rVB	197	148	0.03%	0.004%
74	11.220	3303	3306	3308	rBV	142	109	0.02%	0.003%
75	11.377	3350	3355	3356	rBV	209	167	0.04%	0.004%
76	11.393	3358	3360	3365	rVB2	207	182	0.04%	0.004%
77	11.487	3376	3389	3404	rBV	238074	372437	82.90%	9.184%
78	11.599	3421	3424	3425	rBV	207	124	0.03%	0.003%
79	11.609	3425	3427	3431	rVB	213	120	0.03%	0.003%
80	11.676	3446	3448	3451	rVB	166	115	0.03%	0.003%
81	11.789	3481	3483	3489	rVB2	159	138	0.03%	0.003%
82	11.863	3494	3506	3524	rBV	199039	317045	70.57%	7.818%
83	11.966	3533	3538	3541	rBV3	263	227	0.05%	0.006%
84	12.017	3551	3554	3556	rBV	354	219	0.05%	0.005%
85	12.117	3583	3585	3588	rBV2	179	111	0.02%	0.003%
86	12.316	3645	3647	3654	rVB	203	132	0.03%	0.003%
87	12.480	3688	3698	3708	rVV2	1544	2774	0.62%	0.068%
88	12.554	3717	3721	3725	rBV2	224	203	0.05%	0.005%
89	13.429	3990	3993	3994	rBV	205	122	0.03%	0.003%
90	13.519	4018	4021	4023	rBV	165	105	0.02%	0.003%
91	13.612	4047	4050	4053	rVB2	181	127	0.03%	0.003%
92	13.769	4097	4099	4102	rVB	204	112	0.02%	0.003%
93	13.789	4102	4105	4108	rBV2	181	123	0.03%	0.003%
94	13.831	4115	4118	4122	rBV	168	192	0.04%	0.005%
95	13.876	4130	4132	4137	rVB2	294	182	0.04%	0.004%
96	13.924	4144	4147	4151	rBV	196	184	0.04%	0.005%
97	14.277	4251	4257	4268	rVB2	1426	2378	0.53%	0.059%
98	14.554	4338	4343	4345	rBV	358	278	0.06%	0.007%
99	16.319	4888	4892	4893	rBV	556	353	0.08%	0.009%
100	16.445	4929	4931	4934	rBV3	535	346	0.08%	0.009%


Sum of corrected areas: 4055363

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026481.D
Acq On : 31 Aug 2018 04:56
Operator : MD/SY
Sample : J4694-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

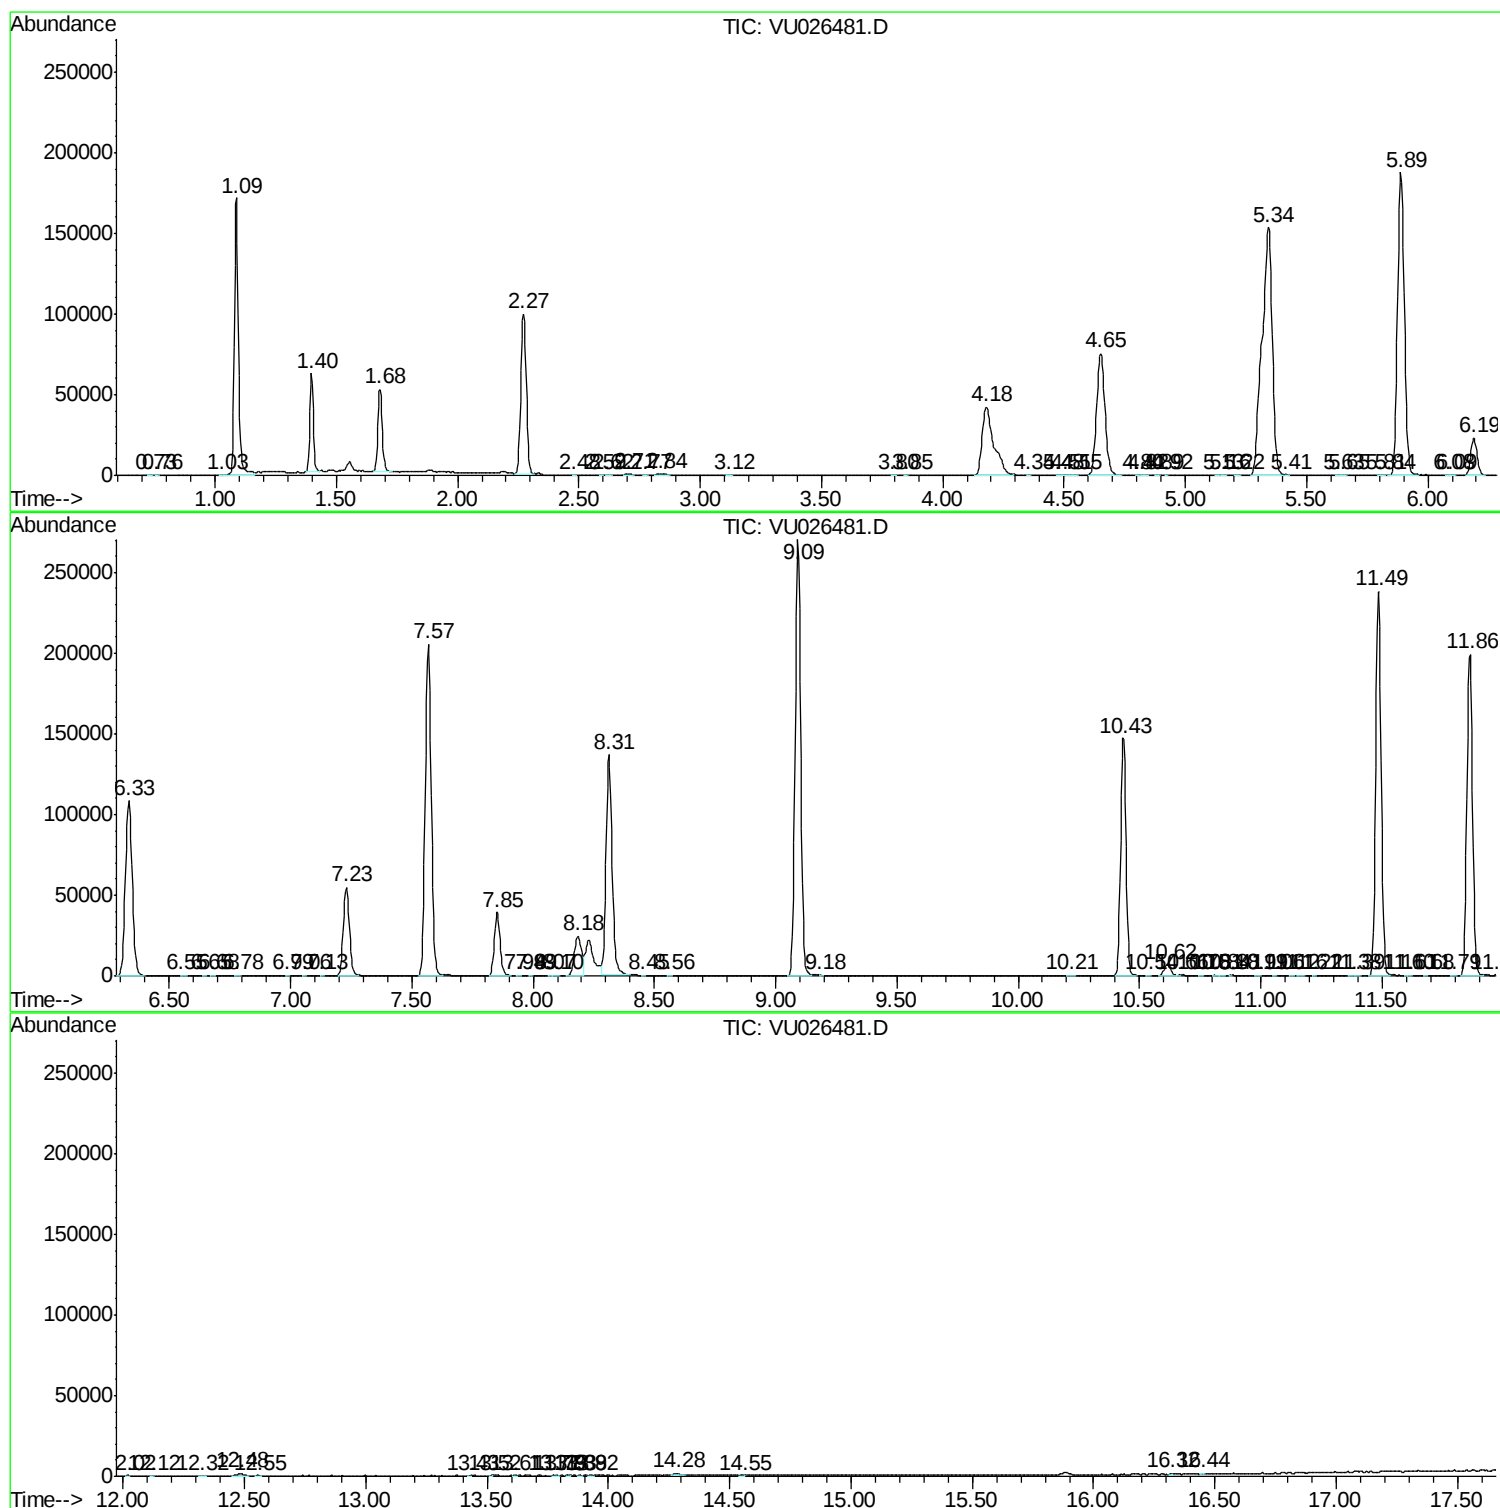

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026481.D
Acq On : 31 Aug 2018 04:56
Operator : MD/SY
Sample : J4694-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026481.D
Acq On : 31 Aug 2018 04:56
Operator : MD/SY
Sample : J4694-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc