

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026482.D
 Acq On : 31 Aug 2018 05:19
 Operator : MD/SY
 Sample : J4691-05DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.642	14	16	18	rBB	125	65	0.00%	0.001%
2	0.738	44	46	49	rBB	136	92	0.00%	0.001%
3	0.764	52	54	55	rBB	209	61	0.00%	0.001%
4	0.780	56	59	60	rBV	111	62	0.00%	0.001%
5	0.809	67	68	69	rBV	206	60	0.00%	0.001%
6	0.838	75	77	79	rBB	137	72	0.00%	0.001%
7	0.896	93	95	97	rBB	118	65	0.00%	0.001%
8	0.912	98	100	102	rBB	131	70	0.00%	0.001%
9	0.934	103	107	111	rBB	141	142	0.00%	0.001%
10	1.089	135	155	179	rBV	485780	545975	8.48%	5.014%
11	1.397	244	251	262	rBV	60737	62375	0.97%	0.573%
12	1.680	332	339	357	rVB	51451	66643	1.04%	0.612%
13	2.272	513	523	537	rVB	96141	145142	2.26%	1.333%
14	2.413	564	567	570	rBV2	204	173	0.00%	0.002%
15	2.584	617	620	623	rBV	309	259	0.00%	0.002%
16	2.699	651	656	659	rBV2	531	596	0.01%	0.005%
17	2.838	695	699	702	rBV2	295	227	0.00%	0.002%
18	2.953	732	735	739	rVV	159	84	0.00%	0.001%
19	2.976	740	742	746	rVB2	156	112	0.00%	0.001%
20	3.085	772	776	779	rBV2	169	144	0.00%	0.001%
21	3.159	798	799	802	rBB	129	66	0.00%	0.001%
22	3.381	866	868	871	rVB	262	130	0.00%	0.001%
23	3.407	872	876	879	rBV	218	227	0.00%	0.002%
24	3.452	887	890	894	rVB2	253	212	0.00%	0.002%
25	3.474	894	897	899	rBV	128	111	0.00%	0.001%
26	3.796	994	997	998	rBV	118	67	0.00%	0.001%
27	3.883	1021	1024	1025	rBV	132	92	0.00%	0.001%
28	3.969	1048	1051	1053	rBV	140	124	0.00%	0.001%
29	4.088	1085	1088	1089	rBB	209	60	0.00%	0.001%
30	4.117	1092	1097	1100	rBV	144	204	0.00%	0.002%
31	4.178	1101	1116	1156	rVV	40198	111924	1.74%	1.028%
32	4.375	1170	1177	1183	rBV2	180	247	0.00%	0.002%
33	4.481	1207	1210	1212	rBV	132	118	0.00%	0.001%
34	4.539	1224	1228	1232	rBB	199	203	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026482.D
 Acq On : 31 Aug 2018 05:19
 Operator : MD/SY
 Sample : J4691-05DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	4.564	1233	1236	1237	rBV	130	92	0.00%	0.001%
36	4.574	1237	1239	1241	rVV	139	61	0.00%	0.001%
37	4.651	1246	1263	1283	rVV	75261	181466	2.82%	1.667%
38	4.796	1307	1308	1310	rVB	248	92	0.00%	0.001%
39	4.815	1311	1314	1316	rVB2	332	155	0.00%	0.001%
40	4.870	1329	1331	1333	rBV	134	92	0.00%	0.001%
41	4.883	1333	1335	1336	rBV	240	119	0.00%	0.001%
42	4.928	1346	1349	1352	rBV	162	157	0.00%	0.001%
43	4.979	1363	1365	1366	rBV	116	65	0.00%	0.001%
44	5.018	1375	1377	1380	rBV	138	117	0.00%	0.001%
45	5.053	1385	1388	1389	rBV	228	117	0.00%	0.001%
46	5.117	1402	1408	1411	rBV	167	244	0.00%	0.002%
47	5.207	1434	1436	1438	rVB	245	115	0.00%	0.001%
48	5.233	1439	1444	1447	rBB	127	158	0.00%	0.001%
49	5.252	1447	1450	1454	rBB	143	118	0.00%	0.001%
50	5.342	1455	1478	1499	rBV2	153584	452063	7.03%	4.152%
51	5.471	1516	1518	1520	rVB	214	102	0.00%	0.001%
52	5.487	1521	1523	1526	rBB	126	89	0.00%	0.001%
53	5.535	1536	1538	1543	rBB	163	151	0.00%	0.001%
54	5.567	1544	1548	1551	rBB	159	151	0.00%	0.001%
55	5.600	1552	1558	1560	rBV	140	170	0.00%	0.002%
56	5.645	1569	1572	1574	rBV	126	114	0.00%	0.001%
57	5.712	1591	1593	1596	rBV	160	130	0.00%	0.001%
58	5.748	1602	1604	1605	rBV	161	89	0.00%	0.001%
59	5.889	1633	1648	1668	rBV	188896	362795	5.64%	3.332%
60	6.018	1685	1688	1690	rBV	265	164	0.00%	0.002%
61	6.053	1697	1699	1701	rBB	118	63	0.00%	0.001%
62	6.072	1701	1705	1706	rBV	168	140	0.00%	0.001%
63	6.188	1729	1741	1759	rVB	59904	113455	1.76%	1.042%
64	6.333	1772	1786	1804	rBV	107441	211828	3.29%	1.945%
65	6.519	1841	1844	1847	rBV	148	152	0.00%	0.001%
66	6.590	1860	1866	1871	rBV	162	297	0.00%	0.003%
67	6.690	1892	1897	1898	rBV	253	189	0.00%	0.002%
68	6.767	1918	1921	1923	rBB	127	89	0.00%	0.001%
69	6.786	1923	1927	1931	rBB	154	178	0.00%	0.002%
70	6.812	1932	1935	1937	rBB	160	107	0.00%	0.001%
71	6.838	1937	1943	1946	rBV	160	224	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026482.D
 Acq On : 31 Aug 2018 05:19
 Operator : MD/SY
 Sample : J4691-05DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	6.937	1968	1974	1979	rBV	158	252	0.00%	0.002%
73	7.153	2038	2041	2042	rBV	145	102	0.00%	0.001%
74	7.230	2054	2065	2086	rBV	55722	95603	1.49%	0.878%
75	7.458	2134	2136	2138	rBV	130	93	0.00%	0.001%
76	7.567	2157	2170	2188	rBV	208483	356919	5.55%	3.278%
77	7.699	2209	2211	2217	rVB3	353	168	0.00%	0.002%
78	7.809	2244	2245	2248	rVB	222	67	0.00%	0.001%
79	7.850	2248	2258	2272	rBV	38676	63420	0.99%	0.582%
80	8.040	2315	2317	2320	rBV	150	67	0.00%	0.001%
81	8.095	2332	2334	2337	rVB	268	133	0.00%	0.001%
82	8.117	2338	2341	2343	rBV	175	148	0.00%	0.001%
83	8.230	2348	2376	2392	rBV	3835623	6434840	100.00%	59.095%
84	8.313	2395	2402	2426	rVB	143697	244280	3.80%	2.243%
85	8.619	2494	2497	2500	rVB	419	296	0.00%	0.003%
86	9.046	2628	2630	2632	rBV	169	86	0.00%	0.001%
87	9.091	2632	2644	2661	rBV	278593	449251	6.98%	4.126%
88	9.384	2731	2735	2737	rBV2	269	173	0.00%	0.002%
89	9.416	2742	2745	2747	rBV2	166	96	0.00%	0.001%
90	9.953	2909	2912	2914	rBV	162	92	0.00%	0.001%
91	10.169	2977	2979	2981	rBV	260	135	0.00%	0.001%
92	10.329	3026	3029	3032	rBV	146	65	0.00%	0.001%
93	10.432	3049	3061	3078	rBV	148150	233666	3.63%	2.146%
94	10.615	3108	3118	3131	rVB3	6768	12910	0.20%	0.119%
95	11.043	3245	3251	3258	rBV2	203	275	0.00%	0.003%
96	11.075	3258	3261	3268	rVB	253	187	0.00%	0.002%
97	11.484	3376	3388	3405	rBV	256537	397082	6.17%	3.647%
98	11.654	3439	3441	3445	rBB	270	130	0.00%	0.001%
99	11.860	3493	3505	3526	rBV	210852	336161	5.22%	3.087%
100	13.609	4047	4049	4053	rBV	336	177	0.00%	0.002%


Sum of corrected areas: 10888986

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026482.D
Acq On : 31 Aug 2018 05:19
Operator : MD/SY
Sample : J4691-05DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

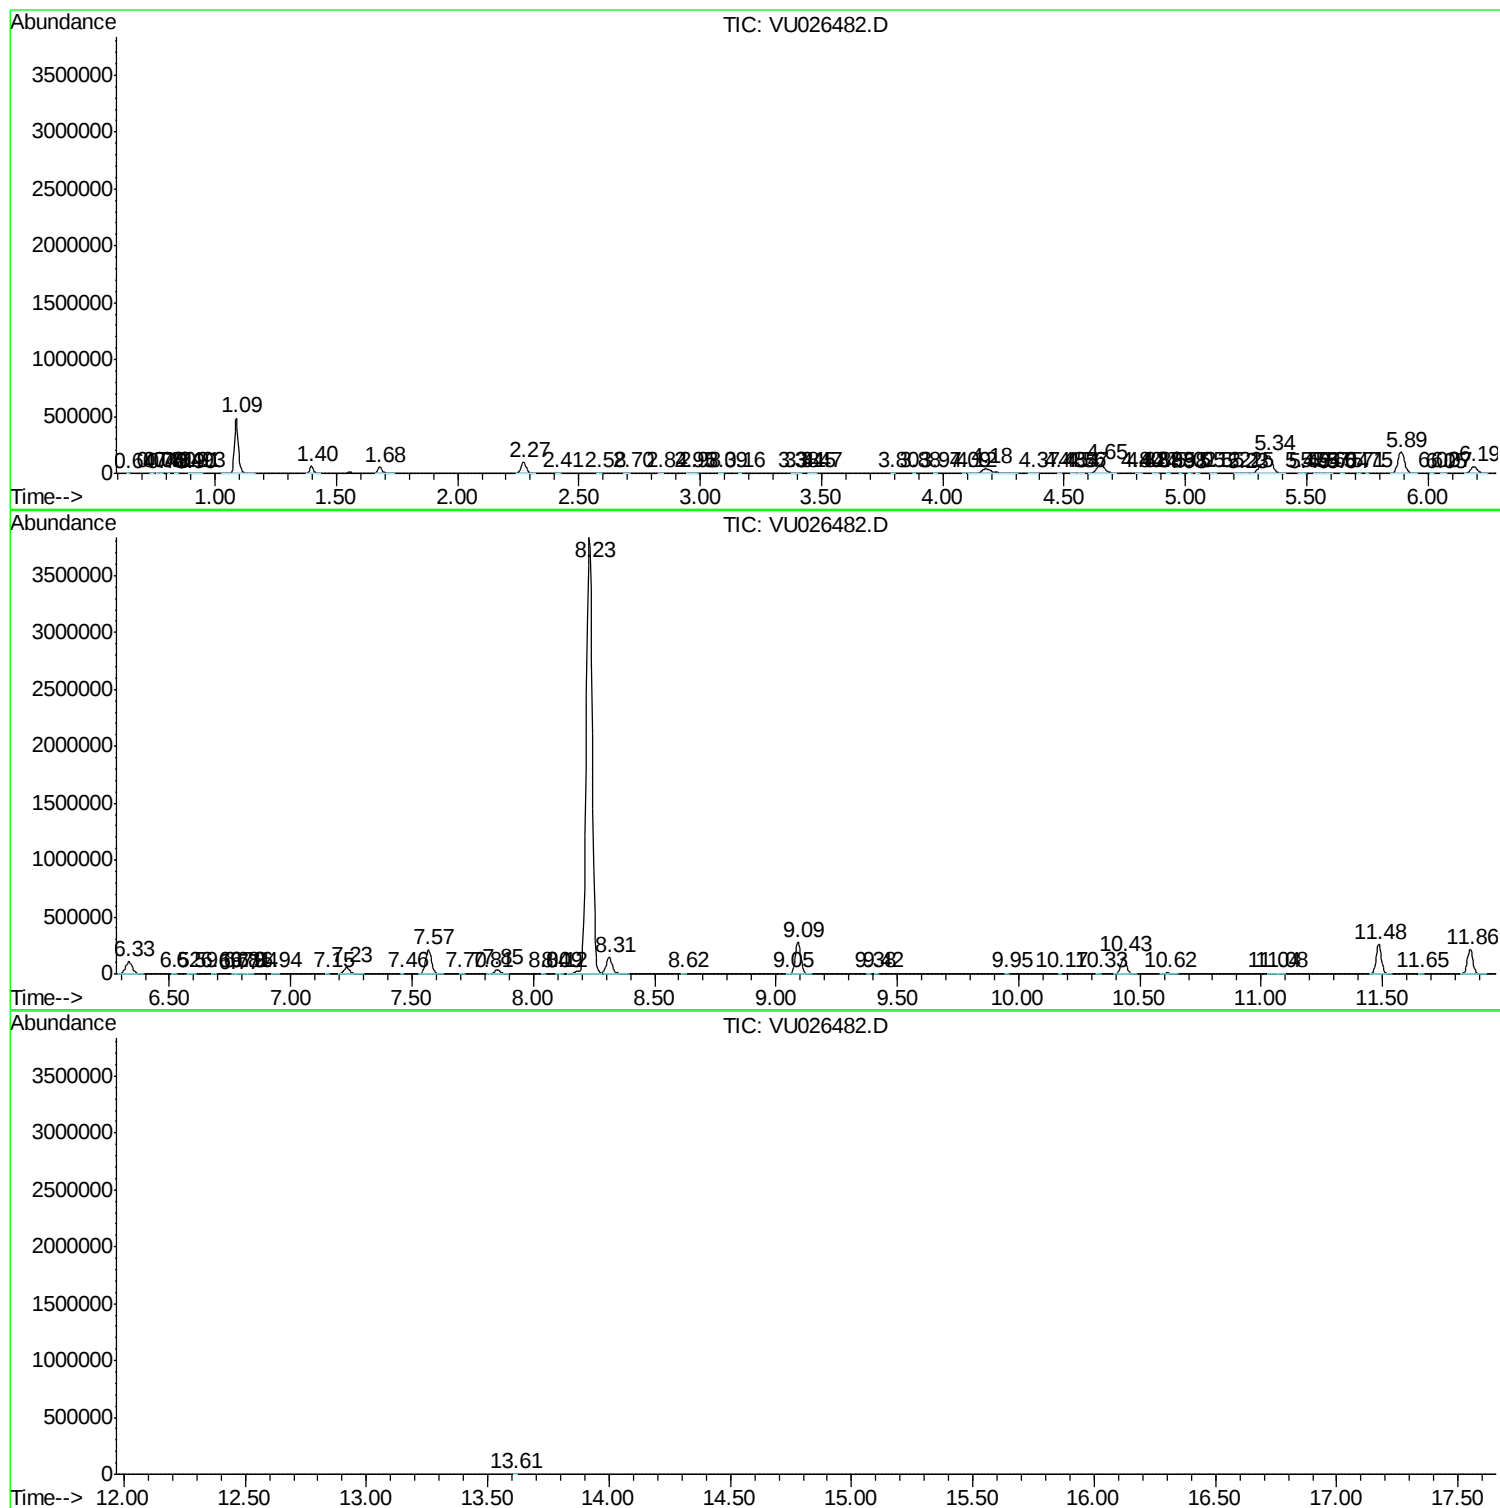

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026482.D
Acq On : 31 Aug 2018 05:19
Operator : MD/SY
Sample : J4691-05DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026482.D
Acq On : 31 Aug 2018 05:19
Operator : MD/SY
Sample : J4691-05DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc