

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026483.D
 Acq On : 31 Aug 2018 05:42
 Operator : MD/SY
 Sample : J4691-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.015	127	132	135	rBB	156	173	0.00%	0.002%
2	1.089	138	155	170	rBV	524709	584849	10.08%	5.633%
3	1.397	244	251	265	rBV	62477	64836	1.12%	0.624%
4	1.680	331	339	353	rVB	52083	68179	1.18%	0.657%
5	2.188	492	497	503	rVB3	1176	1632	0.03%	0.016%
6	2.272	512	523	537	rVB	102251	156072	2.69%	1.503%
7	2.330	537	541	547	rVB4	1077	1062	0.02%	0.010%
8	2.461	578	582	586	rVB	225	137	0.00%	0.001%
9	2.699	650	656	668	rBV2	1075	1700	0.03%	0.016%
10	2.838	691	699	707	rVB3	654	1240	0.02%	0.012%
11	3.059	765	768	772	rVB	176	119	0.00%	0.001%
12	3.101	776	781	785	rBV2	190	176	0.00%	0.002%
13	3.304	841	844	845	rBV	234	119	0.00%	0.001%
14	3.429	880	883	886	rVB	269	178	0.00%	0.002%
15	3.564	922	925	927	rBV	194	154	0.00%	0.001%
16	3.635	945	947	952	rBV	168	199	0.00%	0.002%
17	3.670	955	958	963	rBV	165	227	0.00%	0.002%
18	3.728	972	976	978	rBV	297	268	0.00%	0.003%
19	3.915	1032	1034	1038	rBB	264	177	0.00%	0.002%
20	3.995	1057	1059	1063	rBB	150	125	0.00%	0.001%
21	4.024	1063	1068	1072	rBB	171	223	0.00%	0.002%
22	4.182	1102	1117	1144	rBV	43110	120810	2.08%	1.164%
23	4.365	1171	1174	1178	rVB2	320	273	0.00%	0.003%
24	4.387	1178	1181	1183	rBV	254	183	0.00%	0.002%
25	4.403	1183	1186	1188	rBV	250	149	0.00%	0.001%
26	4.484	1207	1211	1216	rBV	174	234	0.00%	0.002%
27	4.651	1247	1263	1287	rVB	77114	184511	3.18%	1.777%
28	4.741	1287	1291	1293	rBV	167	170	0.00%	0.002%
29	4.780	1299	1303	1307	rVB2	304	333	0.01%	0.003%
30	4.805	1308	1311	1312	rBV	184	130	0.00%	0.001%
31	4.863	1325	1329	1333	rVB	296	325	0.01%	0.003%
32	4.883	1333	1335	1339	rBB2	459	299	0.01%	0.003%
33	4.908	1339	1343	1349	rBV	126	219	0.00%	0.002%
34	5.040	1382	1384	1387	rBV	132	114	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026483.D
 Acq On : 31 Aug 2018 05:42
 Operator : MD/SY
 Sample : J4691-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.095	1397	1401	1405	rBV	174	219	0.00%	0.002%
36	5.342	1455	1478	1498	rBV2	157527	460003	7.93%	4.430%
37	5.474	1517	1519	1522	rBB	248	117	0.00%	0.001%
38	5.686	1580	1585	1589	rBV	161	226	0.00%	0.002%
39	5.799	1618	1620	1623	rBV	144	120	0.00%	0.001%
40	5.889	1634	1648	1668	rBV	186967	363397	6.27%	3.500%
41	6.008	1682	1685	1689	rVB2	230	164	0.00%	0.002%
42	6.188	1728	1741	1759	rVB2	58847	111686	1.93%	1.076%
43	6.333	1771	1786	1808	rBV	109470	216311	3.73%	2.083%
44	6.445	1818	1821	1823	rBV	147	122	0.00%	0.001%
45	6.471	1825	1829	1830	rVV	224	170	0.00%	0.002%
46	6.490	1833	1835	1839	rVV	193	131	0.00%	0.001%
47	6.535	1843	1849	1853	rBV	181	270	0.00%	0.003%
48	6.606	1867	1871	1873	rBV	178	167	0.00%	0.002%
49	6.686	1890	1896	1900	rBV	155	258	0.00%	0.002%
50	6.767	1913	1921	1924	rBV	181	285	0.00%	0.003%
51	6.854	1945	1948	1951	rBV	134	134	0.00%	0.001%
52	6.908	1963	1965	1968	rBV	260	168	0.00%	0.002%
53	7.027	1999	2002	2005	rBB	145	121	0.00%	0.001%
54	7.230	2052	2065	2083	rBV2	56128	97190	1.68%	0.936%
55	7.567	2157	2170	2190	rBV	213000	363212	6.26%	3.498%
56	7.770	2229	2233	2240	rVV	190	239	0.00%	0.002%
57	7.854	2248	2259	2279	rVV	39772	66317	1.14%	0.639%
58	7.931	2280	2283	2288	rVB2	309	287	0.00%	0.003%
59	7.960	2288	2292	2294	rBV2	187	161	0.00%	0.002%
60	8.082	2328	2330	2333	rVB	283	158	0.00%	0.002%
61	8.107	2333	2338	2343	rBV	193	311	0.01%	0.003%
62	8.230	2347	2376	2392	rBV	3506499	5799596	100.00%	55.857%
63	8.313	2393	2402	2424	rVB	153145	263705	4.55%	2.540%
64	8.619	2491	2497	2505	rVB	907	1272	0.02%	0.012%
65	9.091	2632	2644	2672	rBV	276510	448815	7.74%	4.323%
66	10.098	2953	2957	2963	rBV2	308	445	0.01%	0.004%
67	10.271	3009	3011	3015	rBV2	155	125	0.00%	0.001%
68	10.432	3049	3061	3078	rBV	152299	241343	4.16%	2.324%
69	10.615	3105	3118	3130	rVV2	7269	13698	0.24%	0.132%
70	10.747	3155	3159	3163	rBV	153	133	0.00%	0.001%
71	10.869	3193	3197	3200	rBV2	240	196	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
 Data File : VU026483.D
 Acq On : 31 Aug 2018 05:42
 Operator : MD/SY
 Sample : J4691-06DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEE03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	11.439	3370	3374	3376	rBV	194	154	0.00%	0.001%
73	11.484	3376	3388	3408	rVV	253394	392306	6.76%	3.778%
74	11.606	3423	3426	3430	rVV2	229	134	0.00%	0.001%
75	11.631	3431	3434	3437	rVB2	213	150	0.00%	0.001%
76	11.860	3493	3505	3525	rBV	210517	336969	5.81%	3.245%
77	11.988	3543	3545	3547	rBV	351	197	0.00%	0.002%
78	12.307	3641	3644	3646	rBV	226	119	0.00%	0.001%
79	12.336	3649	3653	3659	rVB2	199	193	0.00%	0.002%
80	12.377	3663	3666	3669	rBV	183	134	0.00%	0.001%
81	12.484	3688	3699	3708	rVV2	1620	2754	0.05%	0.027%
82	12.551	3716	3720	3723	rVB3	287	233	0.00%	0.002%
83	12.609	3735	3738	3743	rVB	254	177	0.00%	0.002%
84	12.648	3748	3750	3754	rVV	233	149	0.00%	0.001%
85	12.754	3781	3783	3785	rVB	242	115	0.00%	0.001%
86	12.786	3790	3793	3796	rBV	247	193	0.00%	0.002%
87	12.828	3803	3806	3809	rVB	281	169	0.00%	0.002%
88	13.024	3864	3867	3870	rBV	144	115	0.00%	0.001%
89	13.467	4004	4005	4012	rBV	221	158	0.00%	0.002%
90	13.635	4054	4057	4061	rBV2	231	188	0.00%	0.002%
91	13.686	4071	4073	4076	rBV	247	168	0.00%	0.002%
92	13.712	4079	4081	4084	rVB2	226	149	0.00%	0.001%
93	13.998	4165	4170	4175	rBV2	353	472	0.01%	0.005%
94	14.062	4188	4190	4194	rVB2	327	196	0.00%	0.002%
95	14.159	4217	4220	4222	rBV2	228	191	0.00%	0.002%
96	14.274	4251	4256	4269	rVB2	1627	2485	0.04%	0.024%
97	14.522	4330	4333	4342	rVB2	274	223	0.00%	0.002%
98	15.879	4750	4755	4765	rVB4	1697	3068	0.05%	0.030%
99	16.162	4841	4843	4845	rBV	444	194	0.00%	0.002%
100	16.461	4934	4936	4938	rBV2	445	226	0.00%	0.002%


Sum of corrected areas: 10382846

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026483.D
Acq On : 31 Aug 2018 05:42
Operator : MD/SY
Sample : J4691-06DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

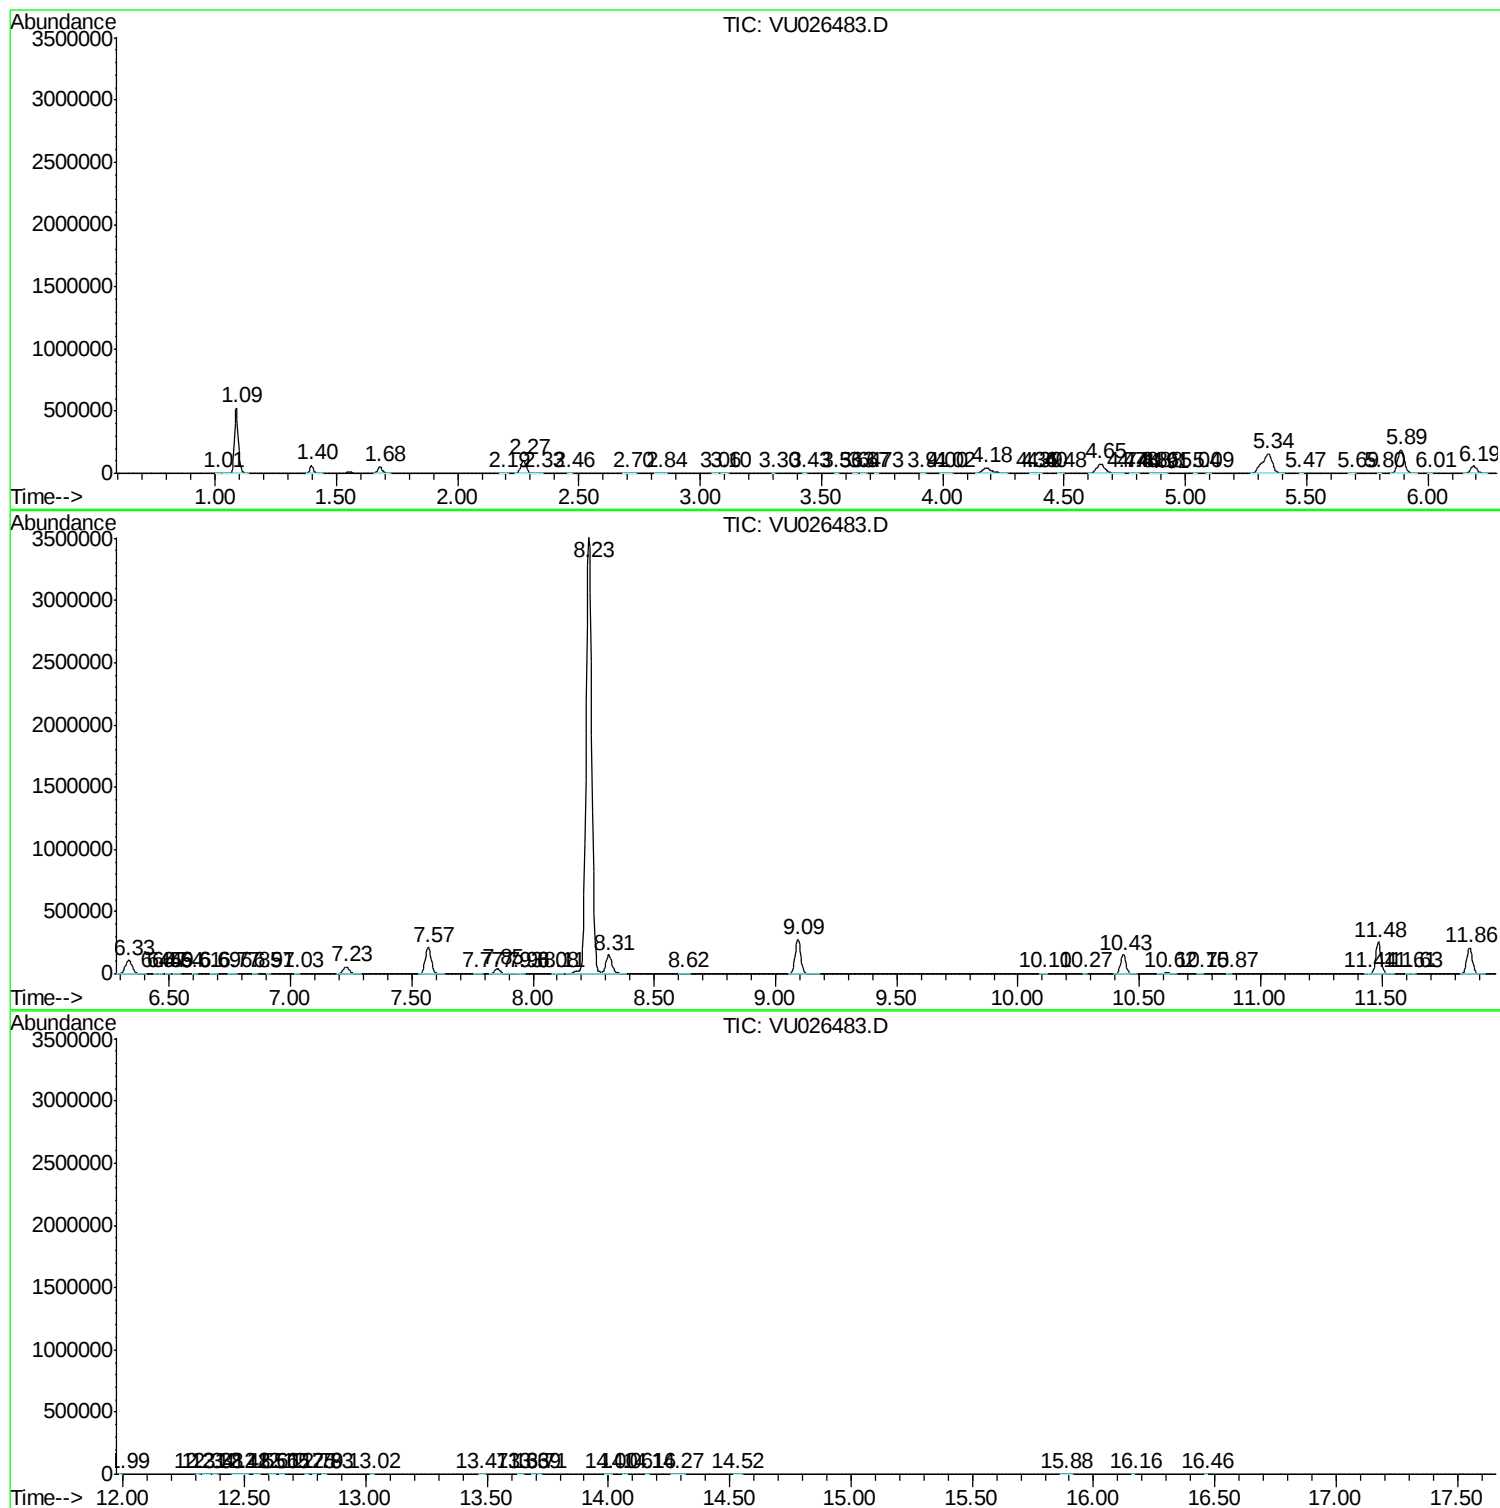

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026483.D
Acq On : 31 Aug 2018 05:42
Operator : MD/SY
Sample : J4691-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083018\
Data File : VU026483.D
Acq On : 31 Aug 2018 05:42
Operator : MD/SY
Sample : J4691-06DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEE03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc