


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083018\
Data File : VU026437.D
Acq On : 30 Aug 2018 10:01
Operator : MD/SY
Sample : BFB44
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Title : VOC Analysis
Last Update : Sat Sep 01 06:27:57 2018

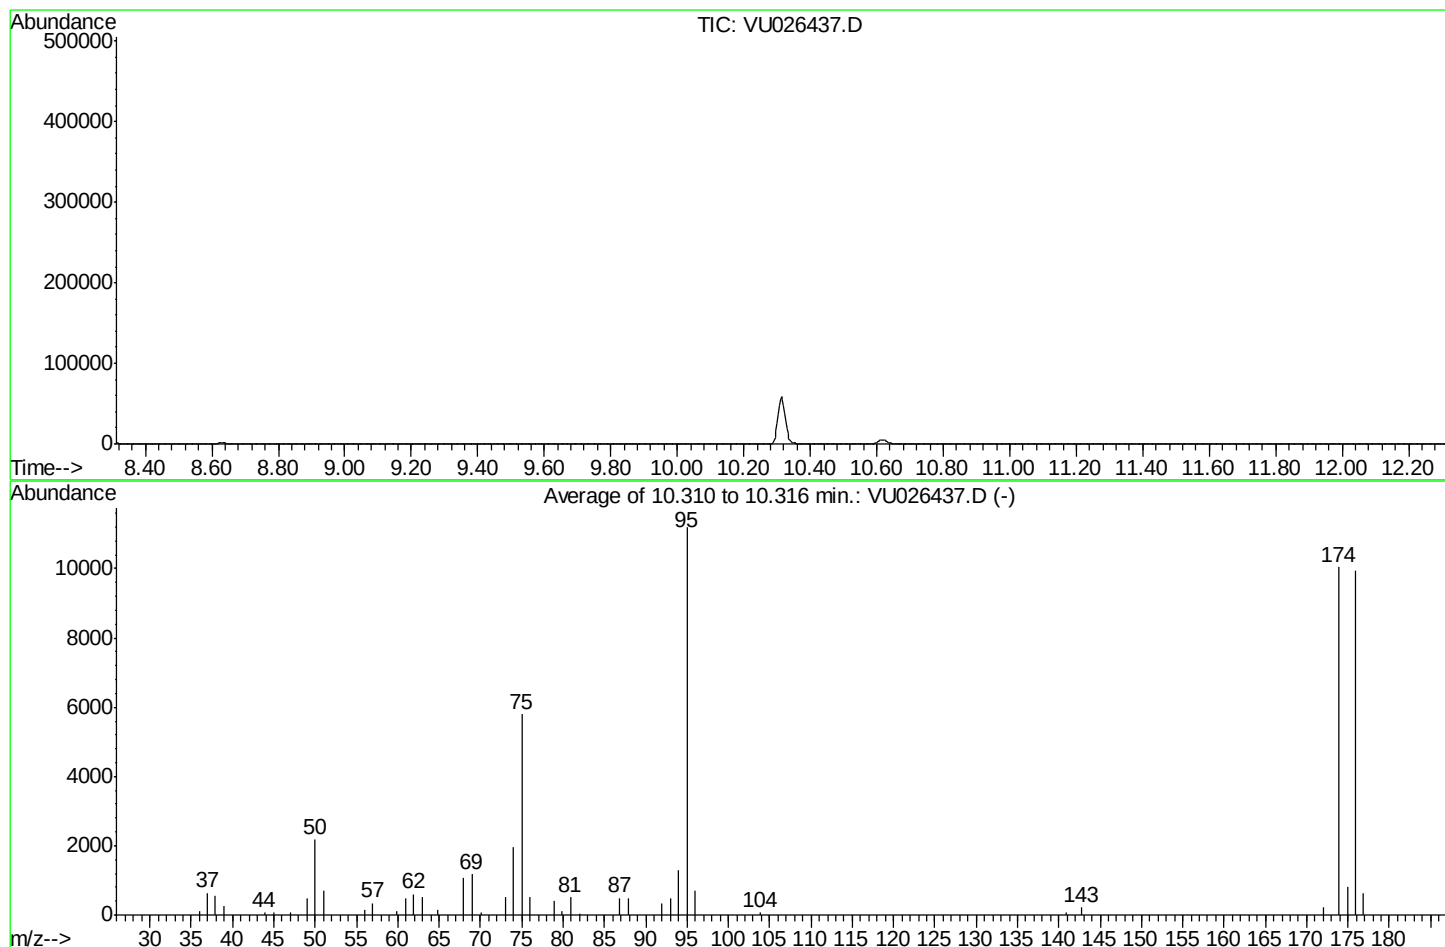

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3013

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	2165	PASS
75	95	30	80	51.8	5795	PASS
95	95	100	100	100.0	11194	PASS
96	95	5	9	6.1	688	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.7	10044	PASS
175	174	5	9	8.0	800	PASS
176	174	95	101	99.1	9953	PASS
177	176	5	9	6.2	622	PASS

m/z	Abundance
43.90	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	126.0
37.00	624.0
37.90	558.0
39.00	247.0
43.90	240.0
44.90	103.0
49.00	532.0
50.00	2142.0
51.00	653.0
56.00	150.0
57.00	340.0
59.90	123.0
60.90	485.0
62.00	518.0
63.00	509.0
64.90	112.0
68.00	1017.0
69.00	1200.0
70.10	102.0
73.00	558.0
74.00	1944.0
75.00	5785.0
76.00	533.0
78.90	431.0
79.90	106.0
80.90	490.0
82.00	100.0
86.80	483.0
88.00	448.0
92.00	306.0
93.00	447.0
94.00	1303.0
95.00	10928.0
96.00	696.0
142.80	192.0
171.90	212.0
173.90	9836.0
174.90	804.0
175.90	9564.0
176.90	640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	117.0
37.00	672.0
38.00	571.0
39.00	275.0
43.90	269.0
45.00	105.0
47.00	102.0
49.00	532.0
50.00	2230.0
51.00	717.0
56.00	169.0
57.00	364.0
59.90	115.0
60.90	489.0
62.00	611.0
63.00	536.0
64.80	144.0
68.00	1089.0
68.90	1215.0
70.10	120.0
73.00	523.0
74.00	2001.0
75.00	5964.0
76.00	526.0
78.90	432.0
79.90	124.0
80.90	533.0
86.90	490.0
87.90	501.0
92.00	331.0
92.90	473.0
94.00	1377.0
95.00	11538.0
95.90	700.0
103.90	101.0
140.90	114.0
142.80	230.0
172.00	216.0
173.90	10357.0
174.90	826.0
175.90	10357.0
176.90	641.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	102.0
37.00	609.0
38.00	532.0
39.00	265.0
43.90	280.0
47.10	112.0
49.00	432.0
50.00	2124.0
51.00	713.0
56.00	163.0
57.00	339.0
59.90	113.0
61.00	490.0
61.90	647.0
62.90	537.0
64.80	153.0
68.00	1060.0
69.00	1103.0
73.00	467.0
74.00	1886.0
75.00	5636.0
76.00	457.0
78.80	407.0
79.90	117.0
80.90	499.0
86.90	473.0
87.90	469.0
92.00	321.0
92.90	489.0
94.00	1256.0
95.00	11116.0
95.90	668.0
103.90	101.0
140.90	135.0
142.80	199.0
172.00	190.0
173.90	9941.0
174.90	772.0
175.90	9939.0
176.90	586.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44