

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083019\
 Data File : VU034075.D
 Acq On : 29 Aug 2019 20:19
 Operator : JC/SP
 Sample : K4528-25
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-Q3-(1.9)

Quant Time: Aug 30 05:28:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	466270	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	748705	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	742453	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.47	152	357515	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	296792	49.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.36%	
35) Dibromofluoromethane	4.86	113	242934	46.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.56%	
50) Toluene-d8	7.55	98	974634	50.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.24%	
62) 4-Bromofluorobenzene	10.29	95	340176	44.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.96%	
Target Compounds						
16) Acetone	2.31	43	23317	7.649	ug/l	99
20) Methylene Chloride	2.69	84	13116	2.273	ug/l	99
43) Isopropyl Acetate	5.53	43	91904	7.618	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU083019\
Data File : VU034075.D
Acq On : 29 Aug 2019 20:19
Operator : JC/SP
Sample : K4528-25
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-Q3-(1.9)

Quant Time: Aug 30 05:28:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

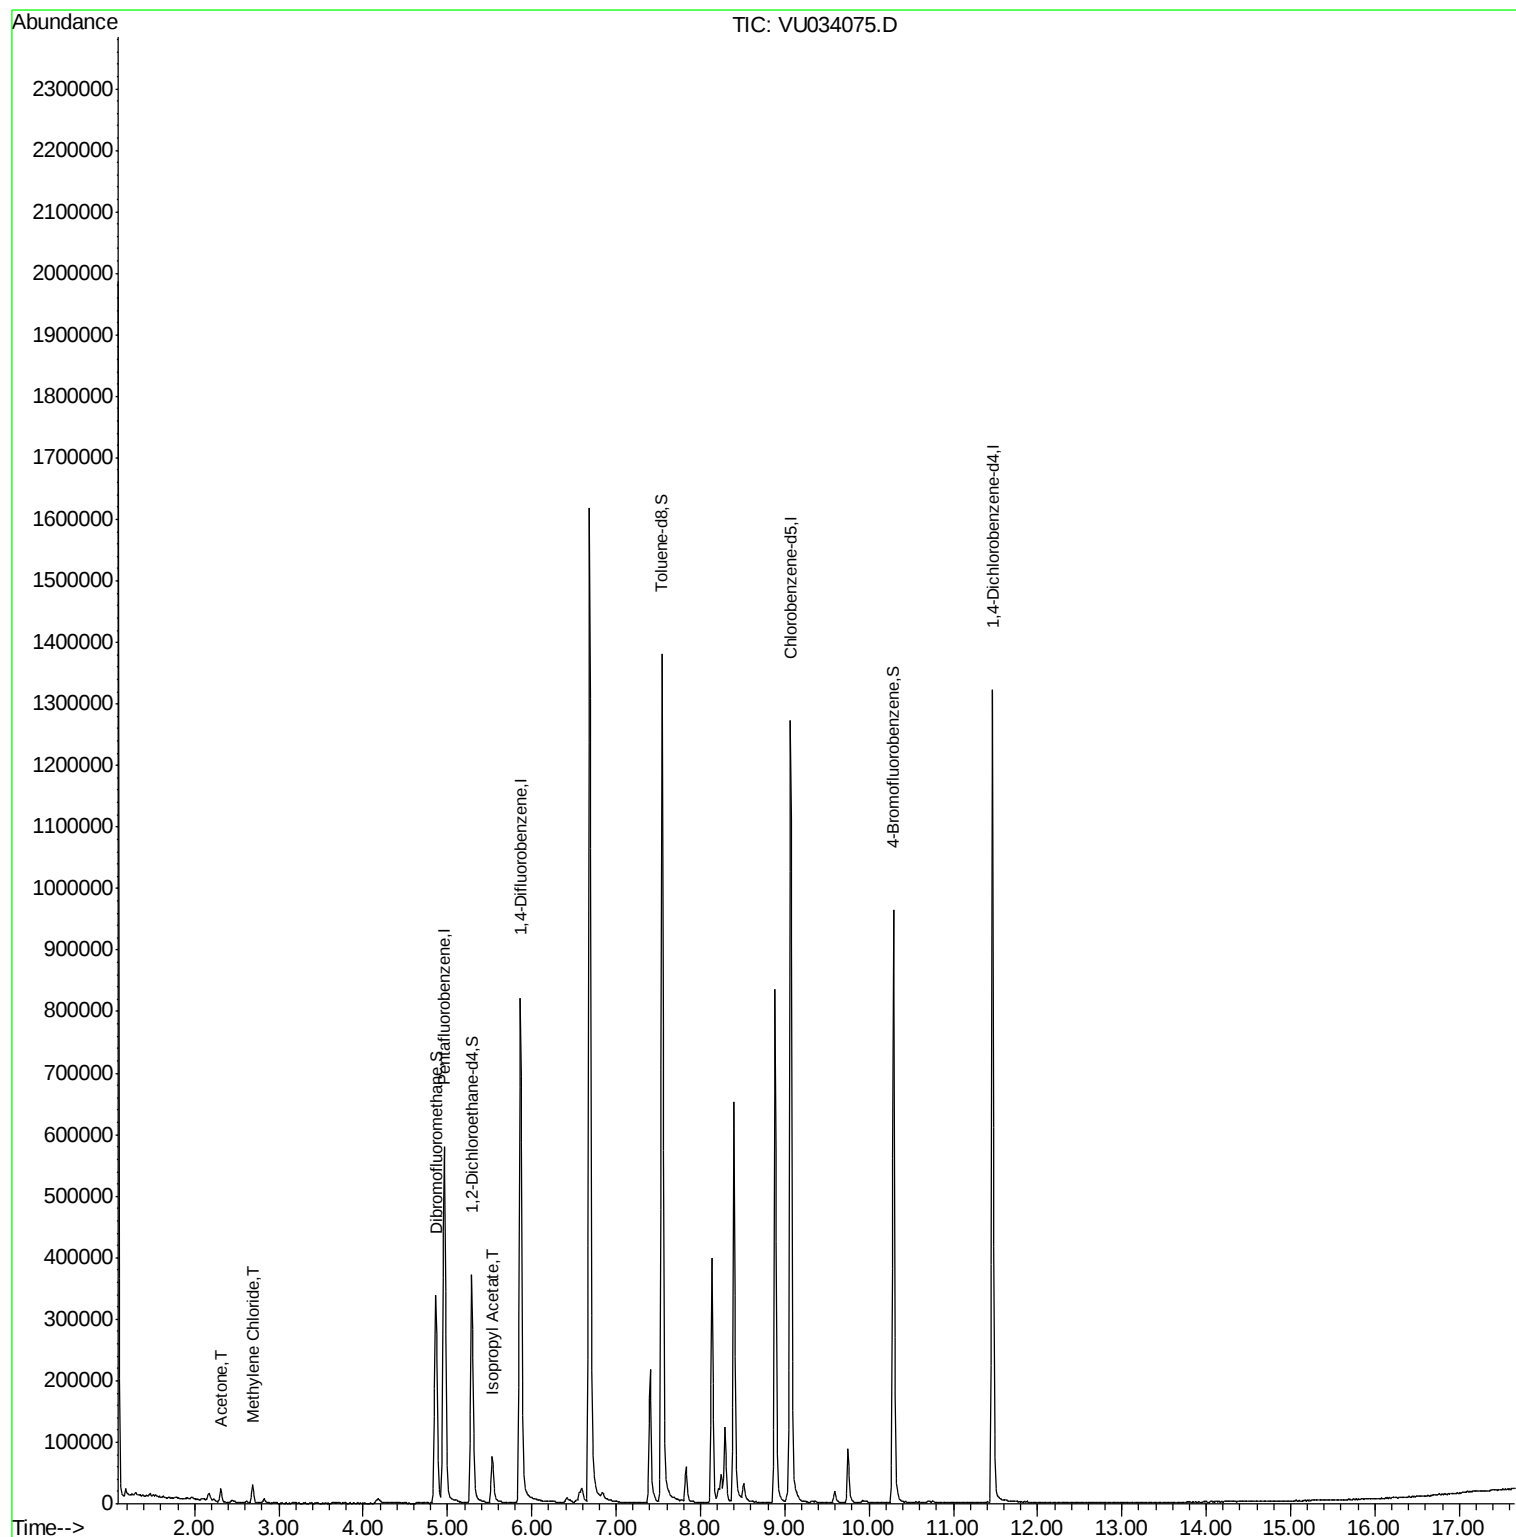

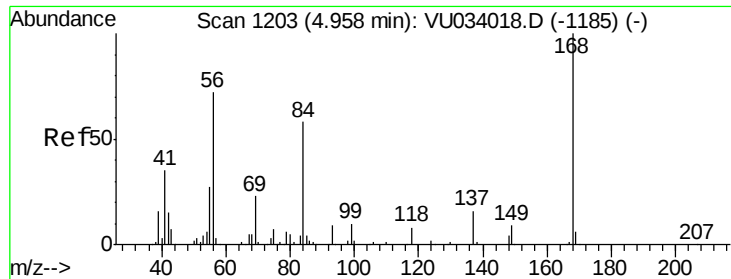

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19


Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-Q3-(1.9)

Tot Ion:168 Resp: 466270

Ion Ratio Lower Upper

168 100

99 53.5 42.3 63.5

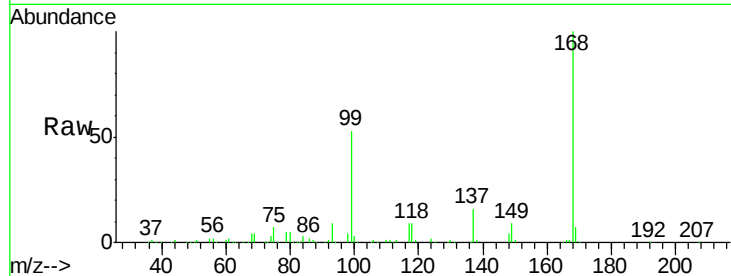

Abundance Ion 167.90 (167.60 to 168.60): VU034018.D (-1185) (-)

Ion 98.90 (98.60 to 99.60): VU034018.D (-1185) (-)

4.96

200000

150000



100000

50000

0

4.90 5.00 5.10

Time-->

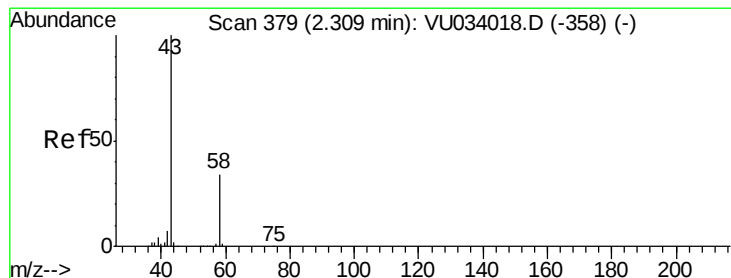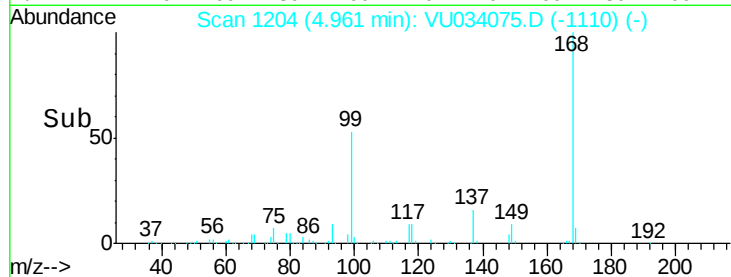

#16

Acetone

Concen: 7.649 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034075.D


Acq: 29 Aug 2019 20:19

Tgt Ion: 43 Resp: 23317

Ion Ratio Lower Upper

43 100

58 34.3 26.8 40.2

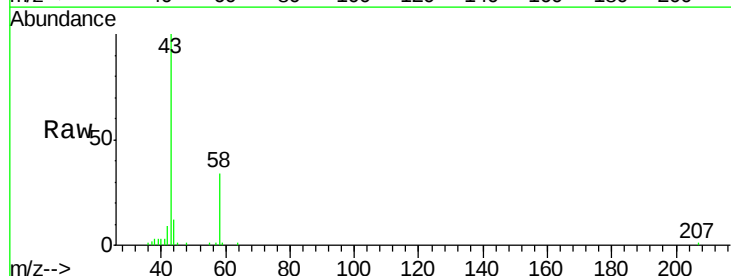

Abundance Ion 43.00 (42.70 to 43.70): VU034018.D (-358) (-)

Ion 58.00 (57.70 to 58.70): VU034018.D (-358) (-)

2.31

15000


10000


5000

0

2.30 2.40

Time-->




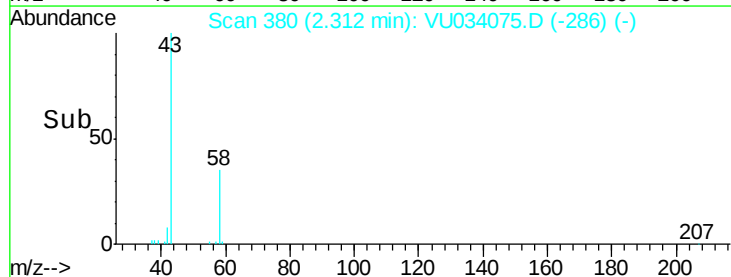


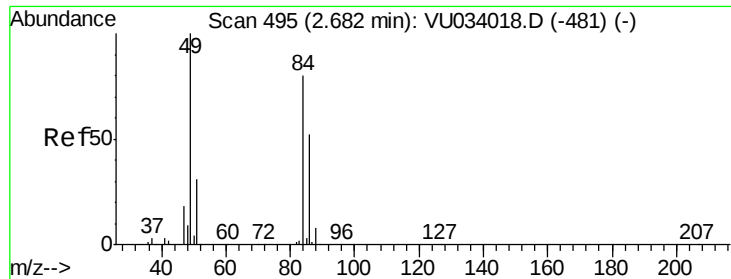

#20
Methvlene Chloride
Concen: 2.273 ug/l
RT: 2.69 min Scan# 497
Delta R.T. 0.01 min
Lab File: VU034075.D
Acq: 29 Aug 2019 20:19




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-Q3-(1.9)


Tot Ion:	84	Resp:	13116
Ion	Ratio	Lower	Upper
84	100		
49	125.8	100.2	150.4
51	39.0	30.8	46.2
86	64.0	52.5	78.7

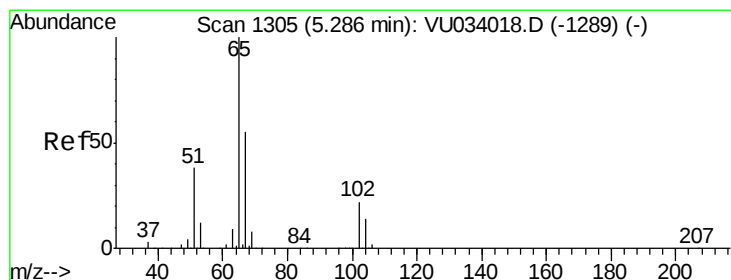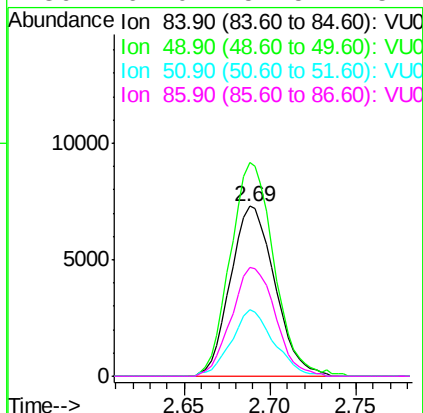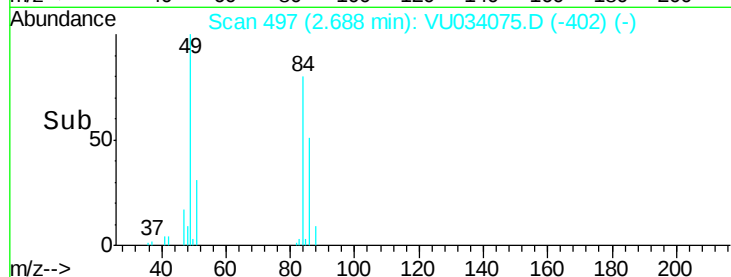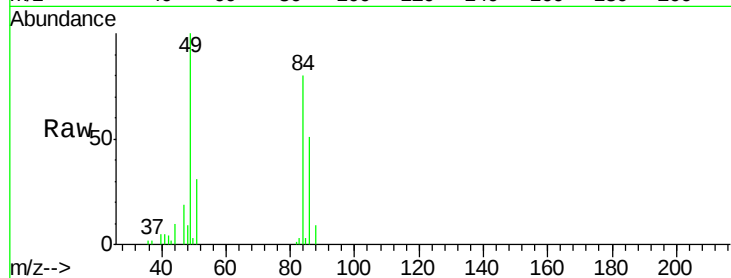

#33
1,2-Dichloroethane-d4
Concen: 49.676 ug/l
RT: 5.29 min Scan# 1306
Delta R.T. 0.00 min
Lab File: VU034075.D
Acq: 29 Aug 2019 20:19

Tgt Ion:	65	Resp:	296792
Ion	Ratio	Lower	Upper
65	100		
67	54.3	0.0	110.6

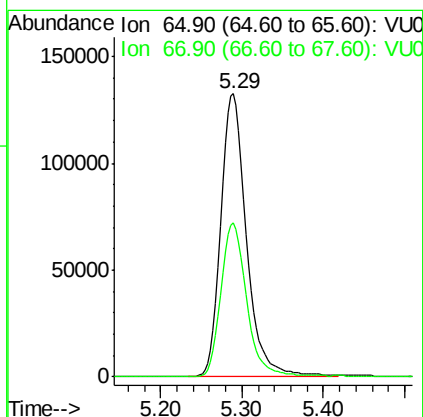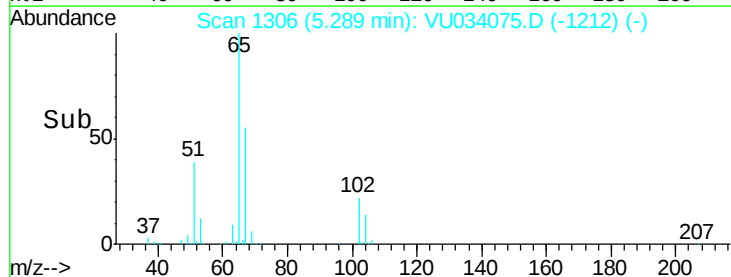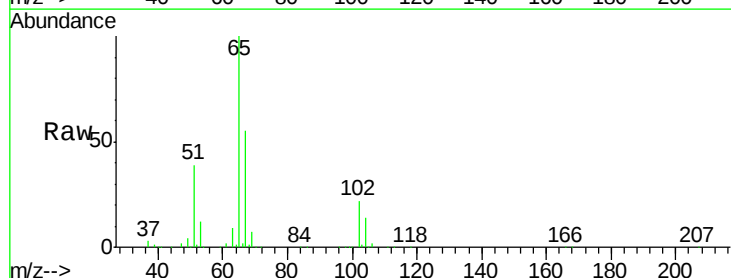

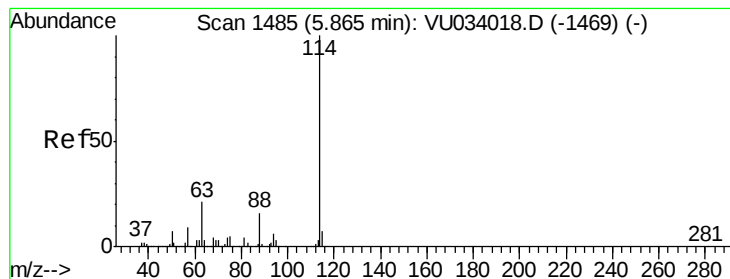

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.87 min Scan# 1486

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-Q3-(1.9)


Tot Ion:114 Resp: 748705

Ion Ratio Lower Upper

114 100

63 20.8 0.0 42.0




88 16.1 0.0 32.0

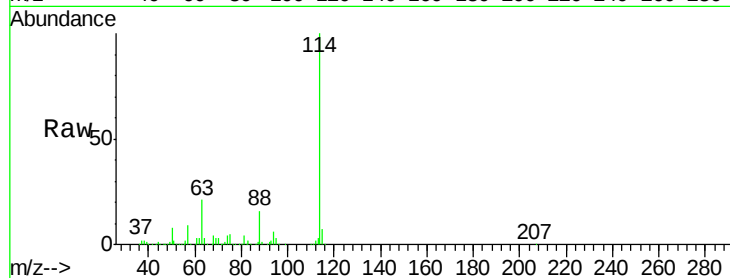

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

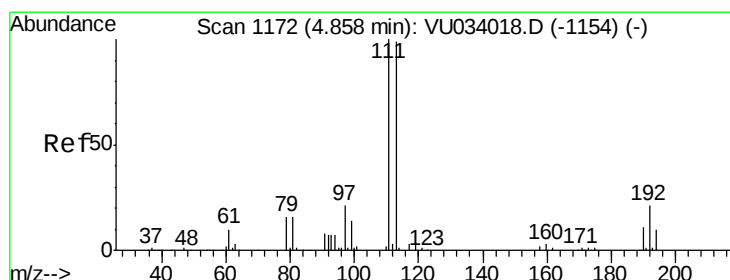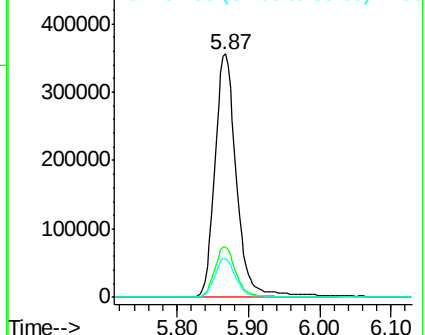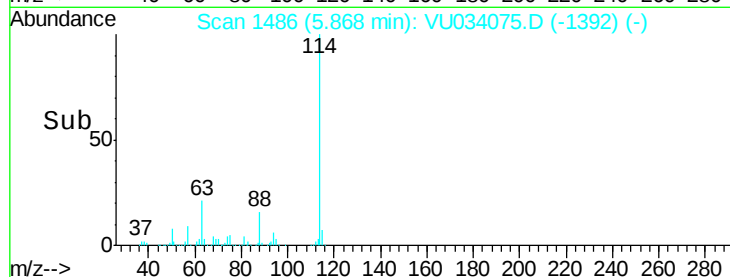

#35

Dibromofluoromethane

Concen: 46.781 ug/l

RT: 4.86 min Scan# 1173

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19


Tgt Ion:113 Resp: 242934

Ion Ratio Lower Upper

113 100

111 103.7 81.7 122.5



192 21.4 17.1 25.7

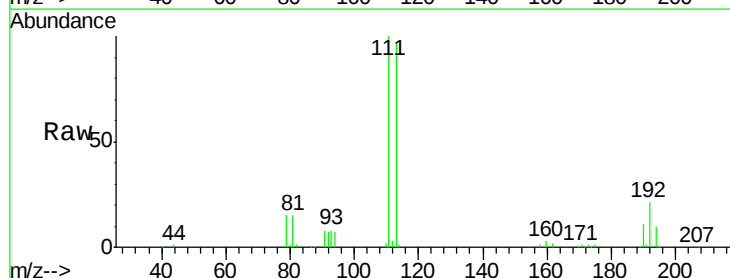


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

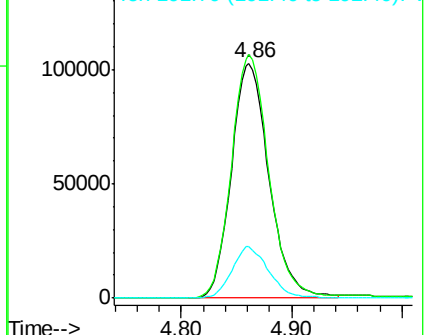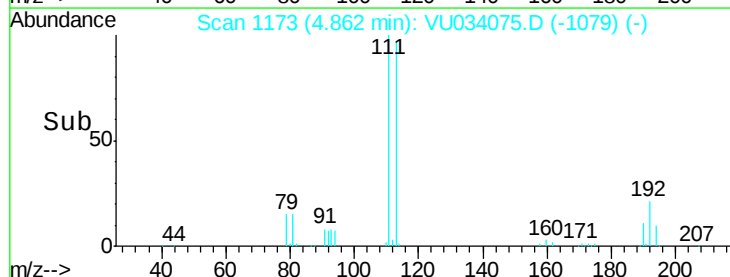

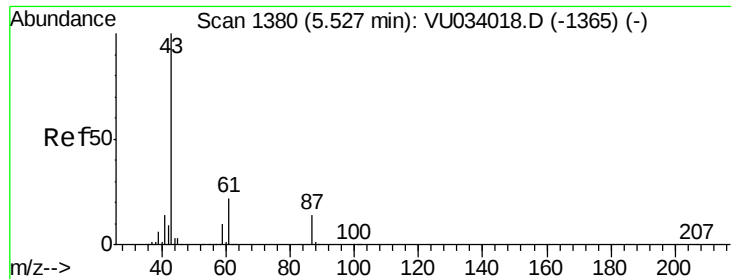

#43

Isopropyl Acetate

Concen: 7.618 ug/l

RT: 5.53 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-Q3-(1.9)


Tot Ion: 43 Resp: 91904

Ion Ratio Lower Upper

43 100

61 20.0 17.2 25.8

87 12.9 10.8 16.2

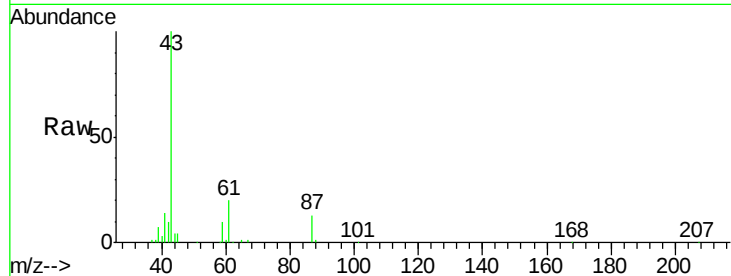


Abundance Ion 43.00 (42.70 to 43.70): VU034075.D (-1287) (-)

Ion 61.00 (60.70 to 61.70): VU034075.D (-1287) (-)


Ion 87.00 (86.70 to 87.70): VU034075.D (-1287) (-)

5.53

Time-->

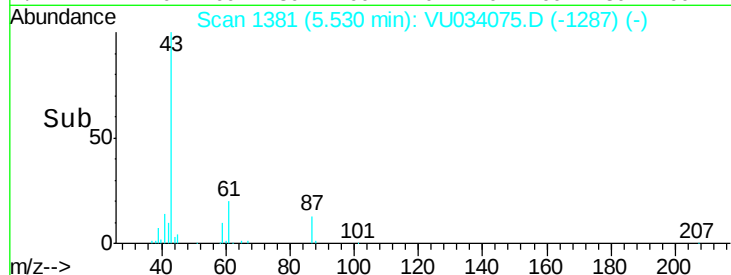

Time-->

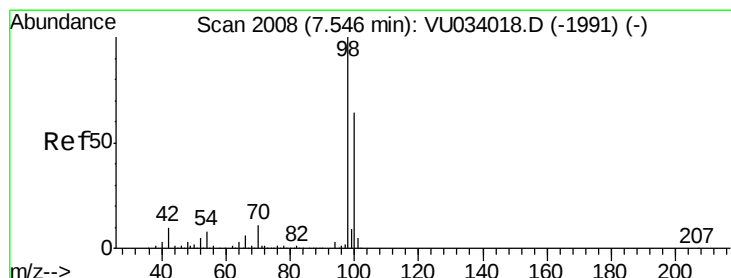

#50

Toluene-d8

Concen: 50.124 ug/l

RT: 7.55 min Scan# 2008

Delta R.T. 0.00 min

Lab File: VU034075.D


Acq: 29 Aug 2019 20:19

Tgt Ion: 98 Resp: 974634

Ion Ratio Lower Upper

98 100

100 63.6 50.3 75.5

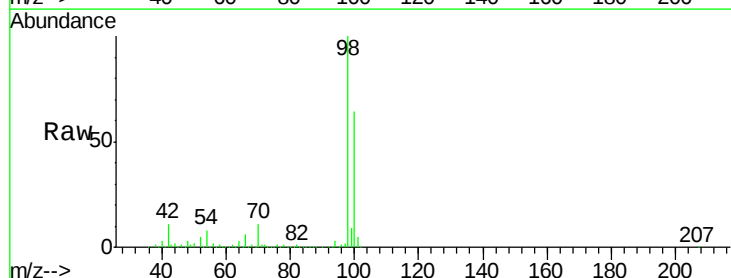


Abundance Ion 98.00 (97.70 to 98.70): VU034075.D (-1915) (-)


Ion 100.00 (99.70 to 100.70): VU034075.D (-1915) (-)

7.55

Time-->

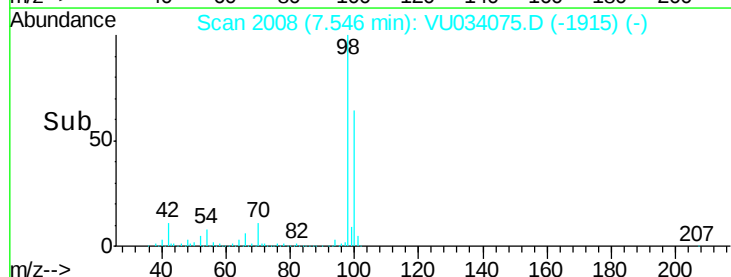

Time-->

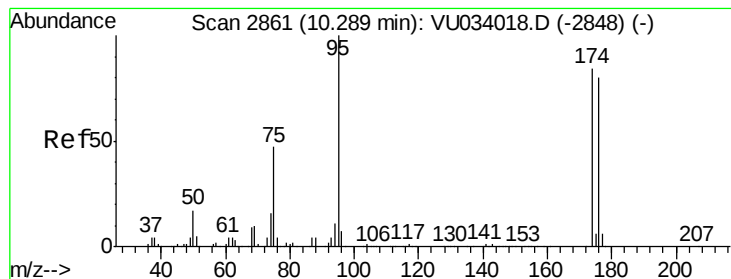

#62

4-Bromofluorobenzene

Concen: 44.975 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-Q3-(1.9)


Tot Ion: 95 Resp: 340176

Ion Ratio Lower Upper

95 100

174 84.0 0.0 168.8




176 80.2 0.0 161.8

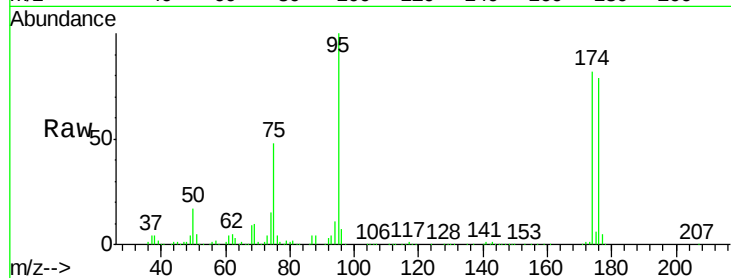

Abundance Ion 94.90 (94.60 to 95.60): VU034018.D (-2848) (-)

Ion 173.80 (173.50 to 174.50): VU034018.D (-2848) (-)

Ion 175.80 (175.50 to 176.50): VU034018.D (-2848) (-)

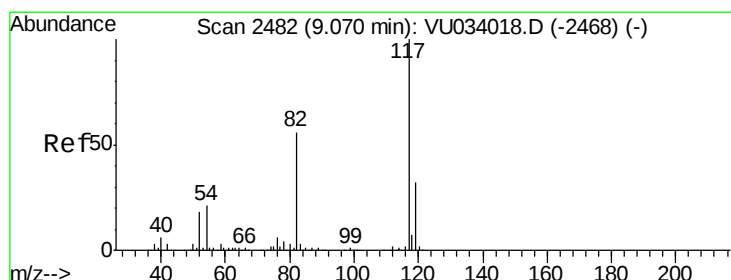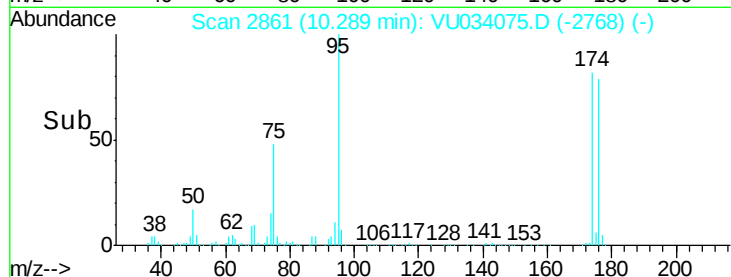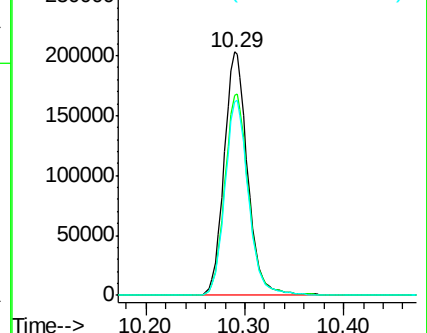

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. 0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19


Tgt Ion: 117 Resp: 742453

Ion Ratio Lower Upper

117 100

82 56.9 45.1 67.7



119 32.1 25.4 38.0

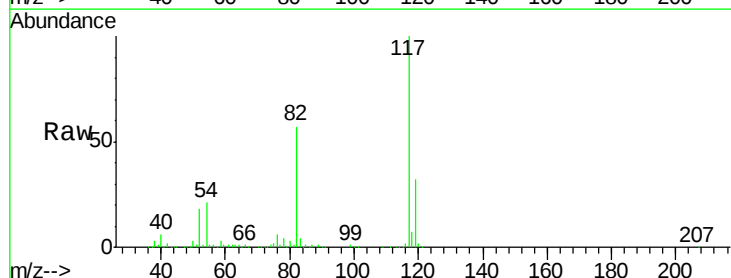


Abundance Ion 116.90 (116.60 to 117.60): VU034018.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034018.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034018.D (-2468) (-)

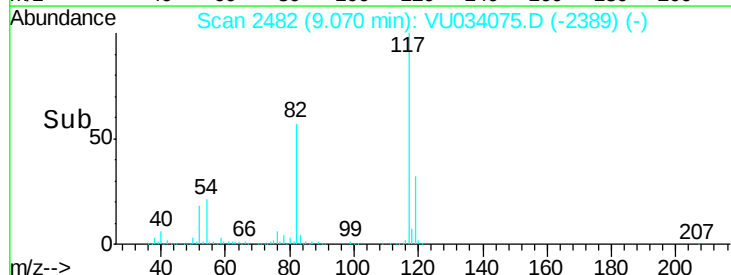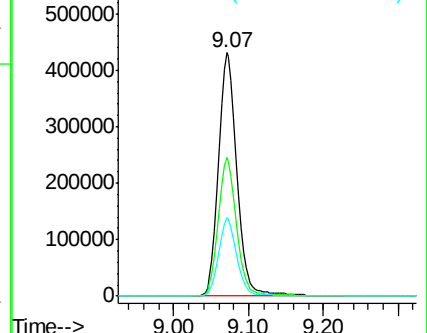

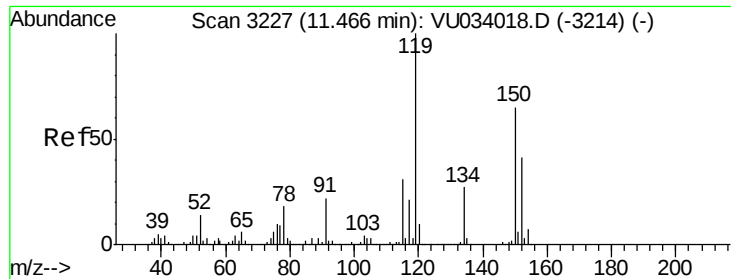

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.47 min Scan# 3227

Delta R.T. -0.00 min

Lab File: VU034075.D

Acq: 29 Aug 2019 20:19

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-Q3-(1.9)


Tot Ion:152 Resp: 357515

Ion Ratio Lower Upper

152 100

115 58.2 41.1 123.3

150 156.9 0.0 348.8

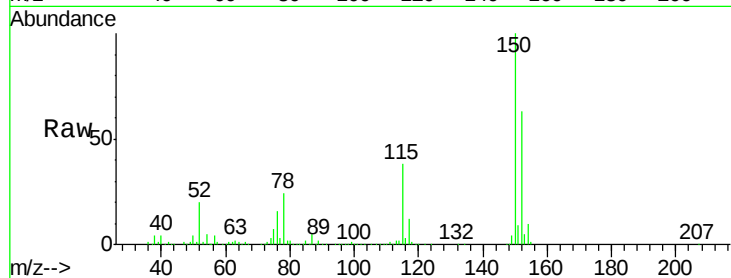

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

