




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050524.D
 Acq On : 30 Aug 2022 18:53
 Operator : SY/MD
 Sample : N4344-06ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
 Supervised By :Mahesh Dadoda 09/05/2022

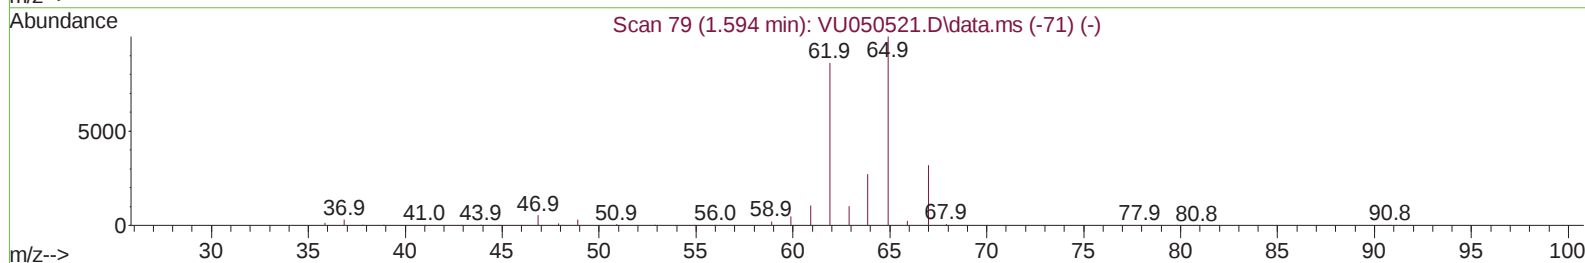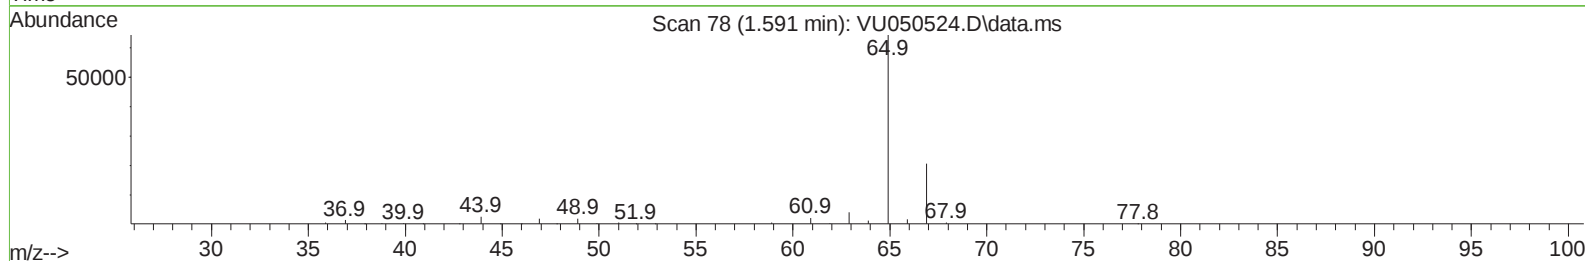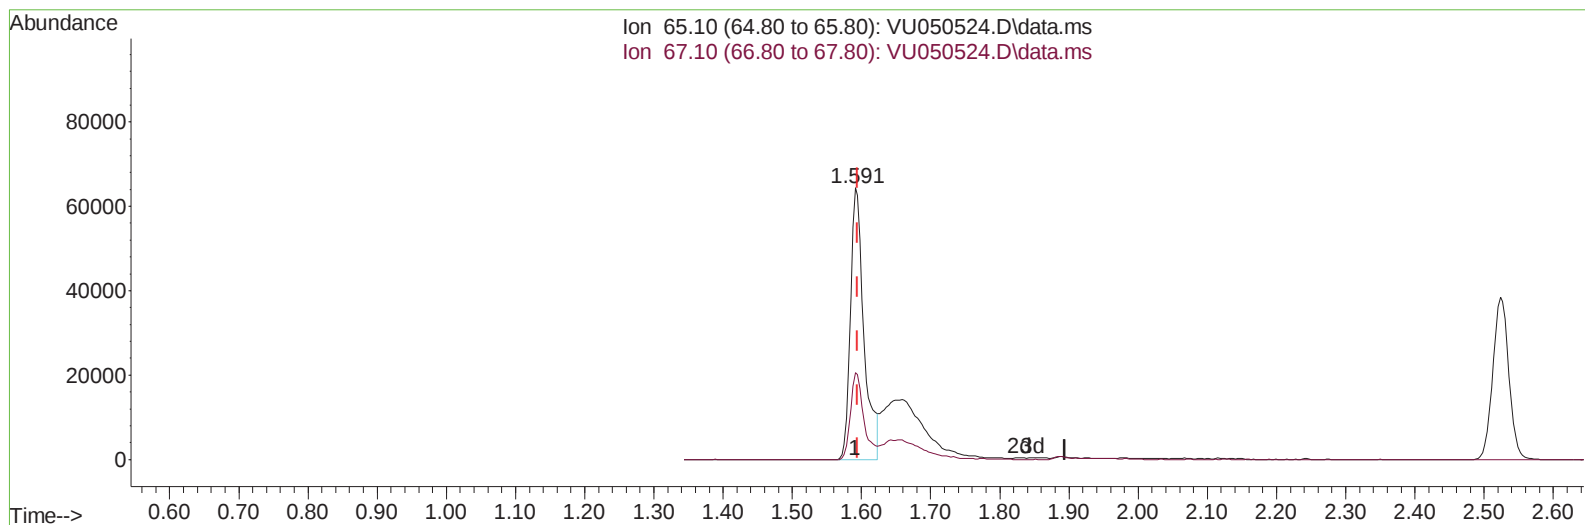

TIC: VU050524.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 23.65 ug/L

response 87287

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	31.95
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050524.D
 Acq On : 30 Aug 2022 18:53
 Operator : SY/MD
 Sample : N4344-06ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
 Supervised By :Mahesh Dadoda 09/05/2022

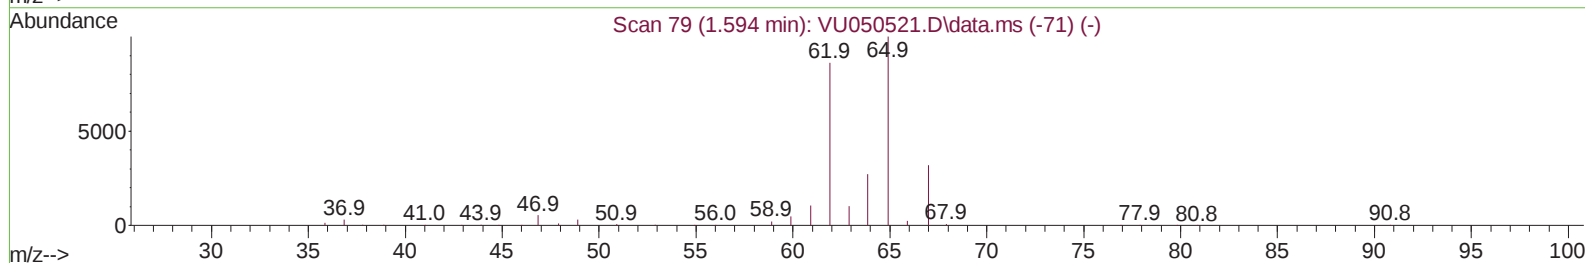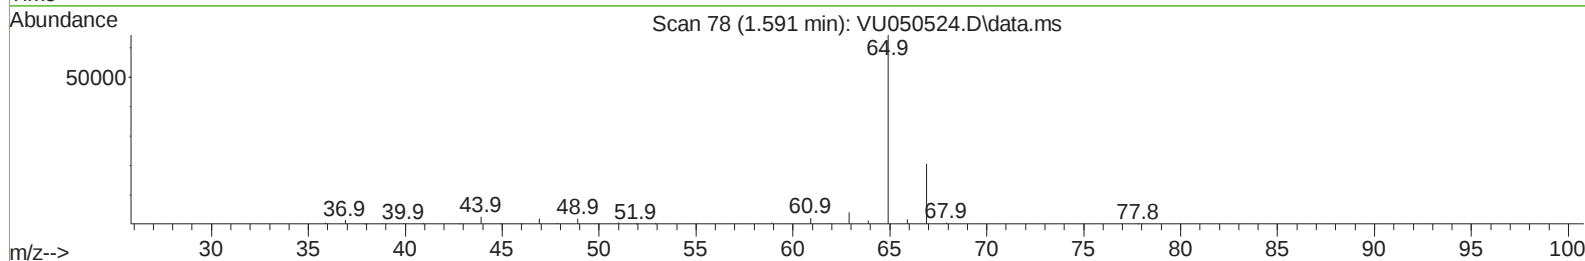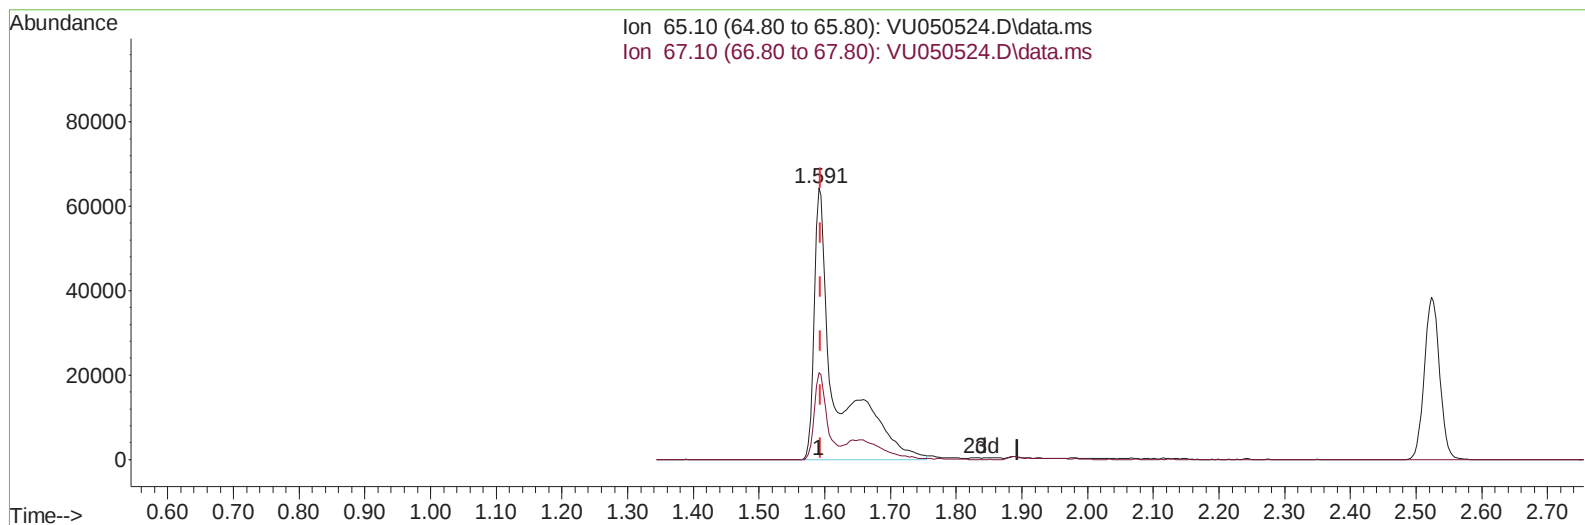

TIC: VU050524.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 39.68 ug/L m

response 146475

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	19.04#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050524.D
 Acq On : 30 Aug 2022 18:53
 Operator : SY/MD
 Sample : N4344-06ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
 Supervised By :Mahesh Dadoda 09/05/2022

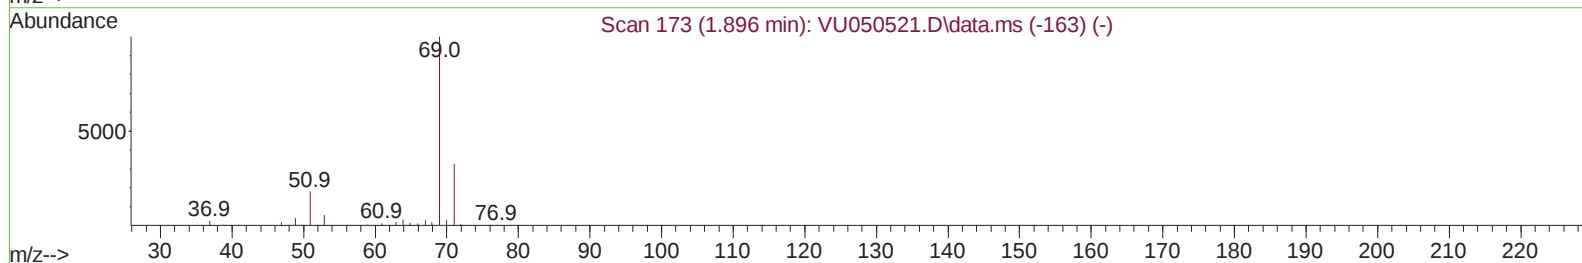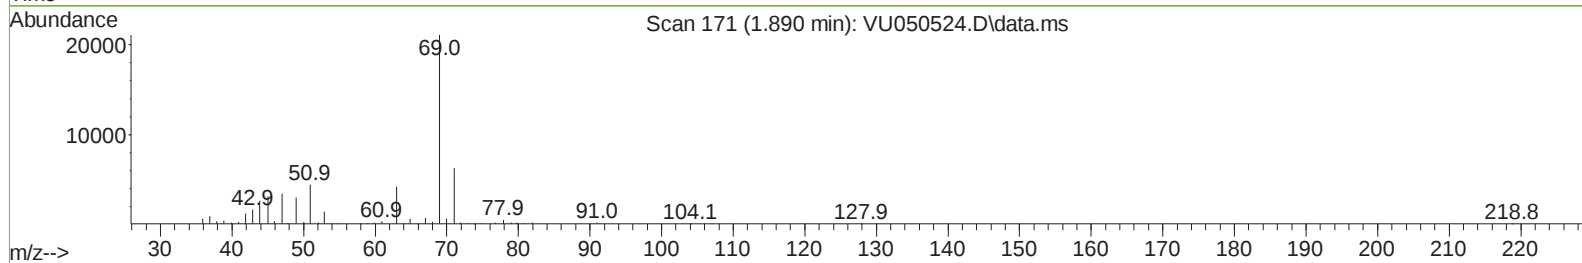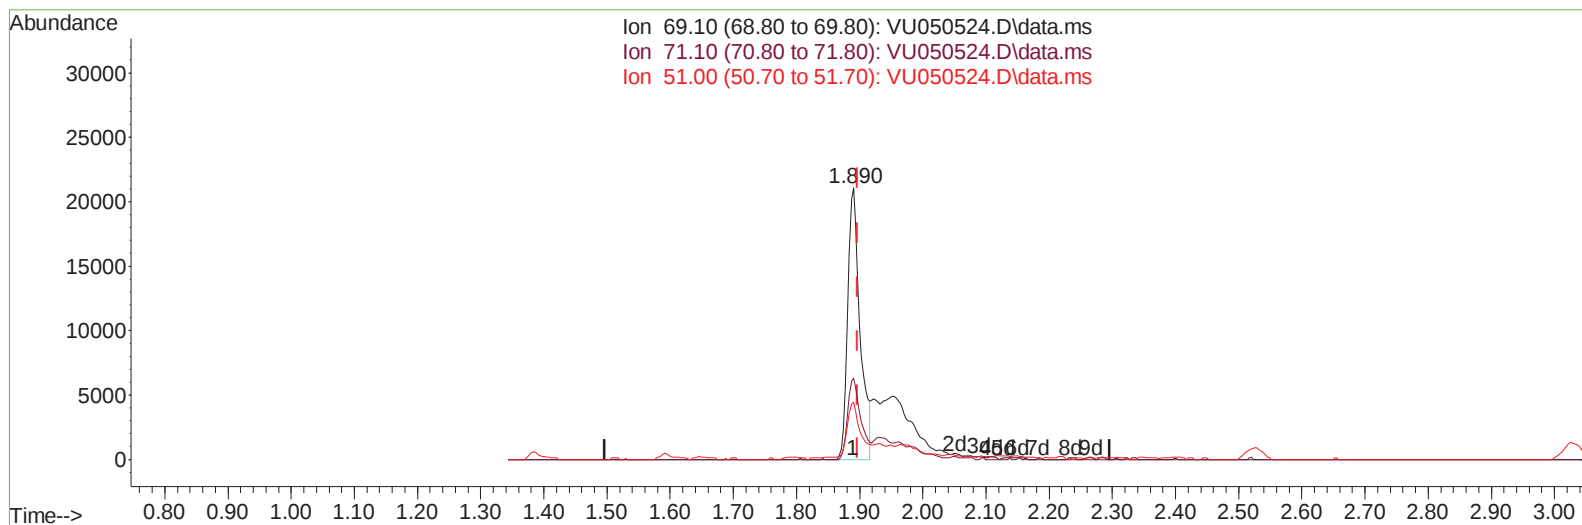

TIC: VU050524.D\data.ms

(7) Chloroethane-d5 (S)

1.890min (-0.006) 9.97 ug/L

response 28693

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	32.72
51.00	18.40	21.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050524.D
 Acq On : 30 Aug 2022 18:53
 Operator : SY/MD
 Sample : N4344-06ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
 Supervised By :Mahesh Dadoda 09/05/2022

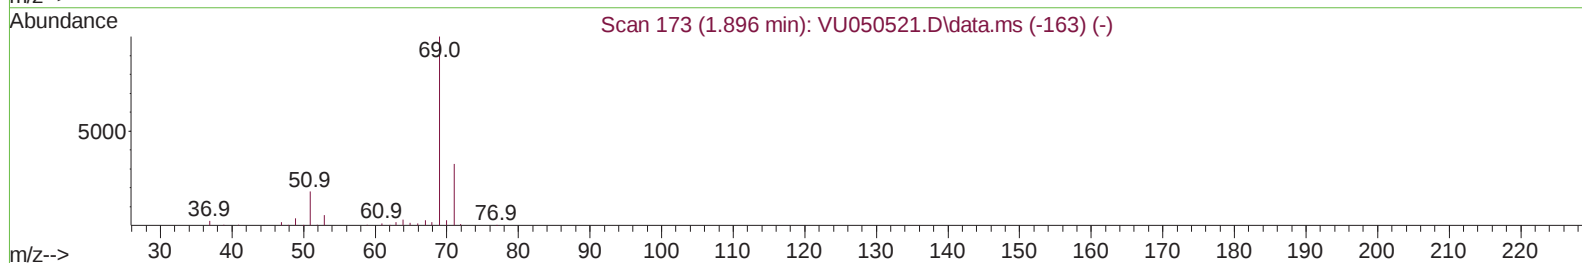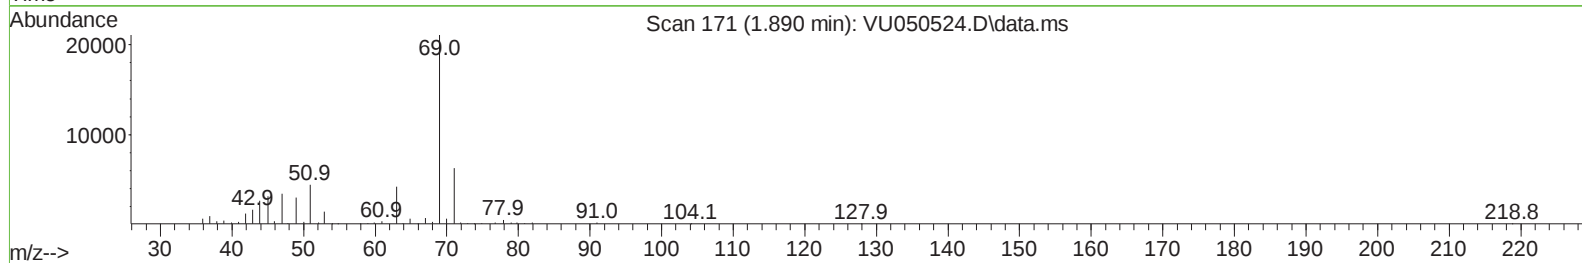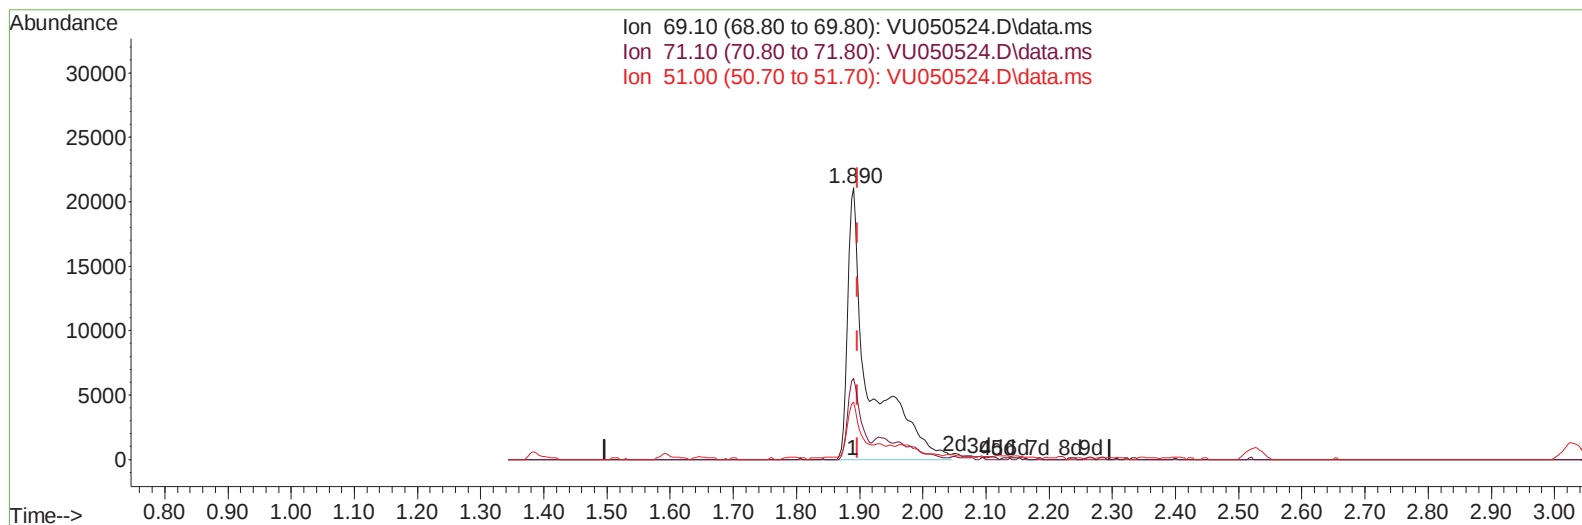

TIC: VU050524.D\data.ms

(7) Chloroethane-d5 (S)

1.890min (-0.006) 17.34 ug/L m

response 49904

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	18.81#
51.00	18.40	12.59#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050524.D
 Acq On : 30 Aug 2022 18:53
 Operator : SY/MD
 Sample : N4344-06ME
 Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
 Supervised By :Mahesh Dadoda 09/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	481268	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	446220	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	166177	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.591	65	146475m	39.683	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	79.360%	
7) Chloroethane-d5	1.890	69	49904m	17.341	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	34.680%#	
11) 1,1-Dichloroethene-d2	2.523	63	193645	31.072	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	62.140%	
21) 2-Butanone-d5	4.649	46	242548	75.135	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	75.130%	
24) Chloroform-d	5.060	84	262535	36.554	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	73.100%	
26) 1,2-Dichloroethane-d4	5.700	65	173334	37.154	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.300%	
32) Benzene-d6	5.719	84	574636	41.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.100%	
36) 1,2-Dichloropropane-d6	6.690	67	185536	40.290	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	80.580%	
41) Toluene-d8	7.896	98	486905	40.468	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	80.940%	
43) trans-1,3-Dichloroprop...	8.182	79	64754	34.964	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	69.920%	
47) 2-Hexanone-d5	8.661	63	150657	90.358	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	90.360%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	256426	35.700	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	71.400%	
66) 1,2-Dichlorobenzene-d4	12.198	152	143543	39.897	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.800%#	
Target Compounds						
					Qvalue	
46) Tetrachloroethene	8.552	164	11315	4.348	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050524.D
Acq On : 30 Aug 2022 18:53
Operator : SY/MD
Sample : N4344-06ME
Misc : 5.26g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 31 01:47:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/05/2022
Supervised By :Mahesh Dadoda 09/05/2022

