




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050526.D
 Acq On : 30 Aug 2022 19:41
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

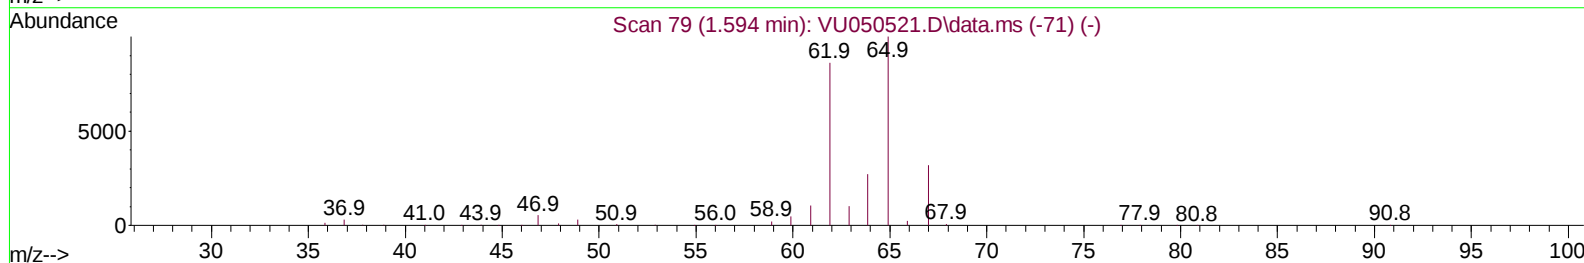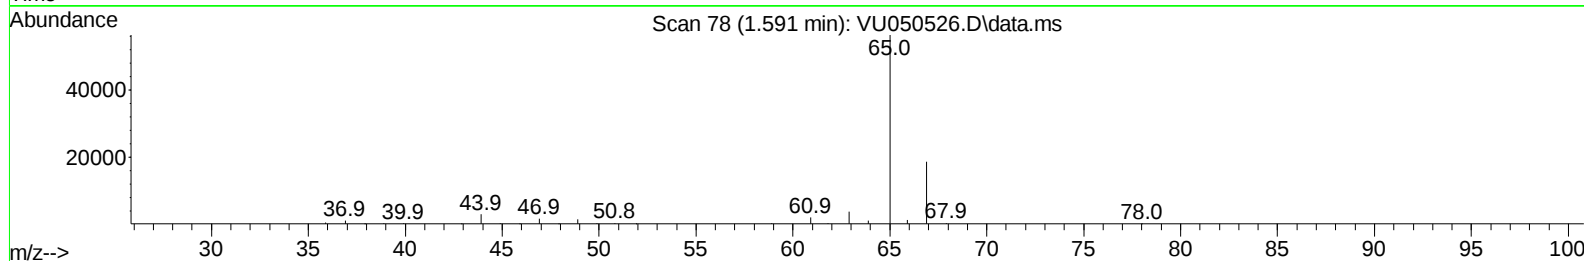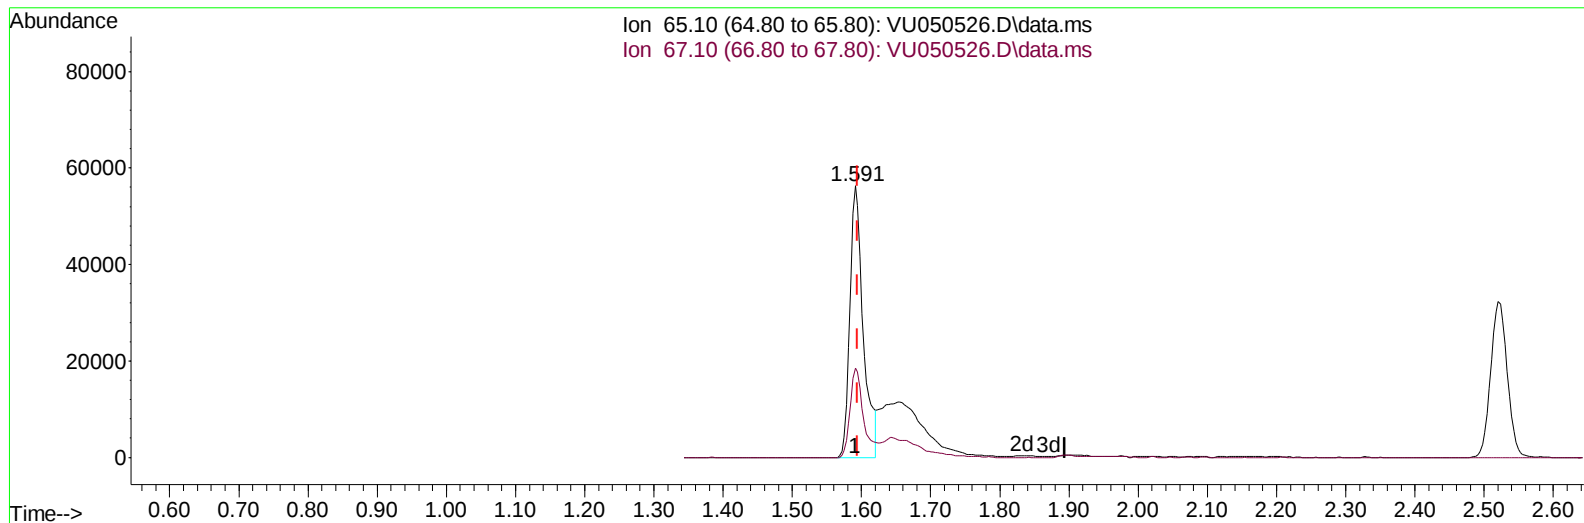

TIC: VU050526.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 17.71 ug/L

response 74676

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	34.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050526.D
 Acq On : 30 Aug 2022 19:41
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

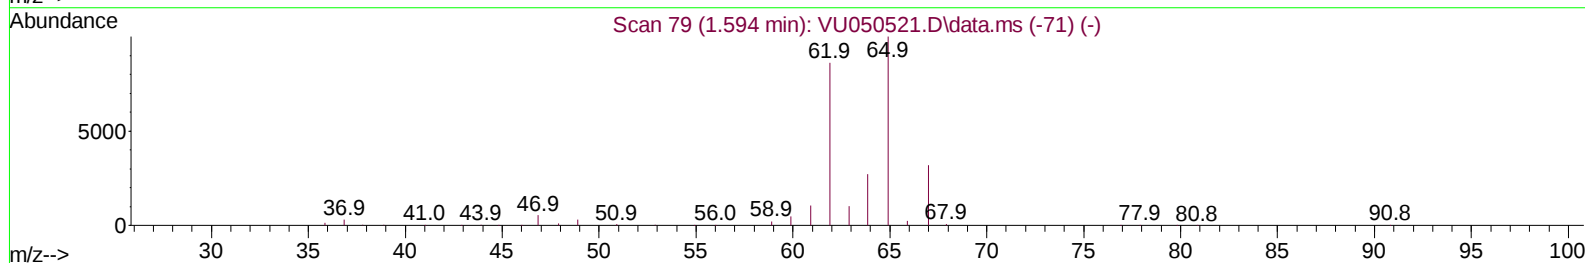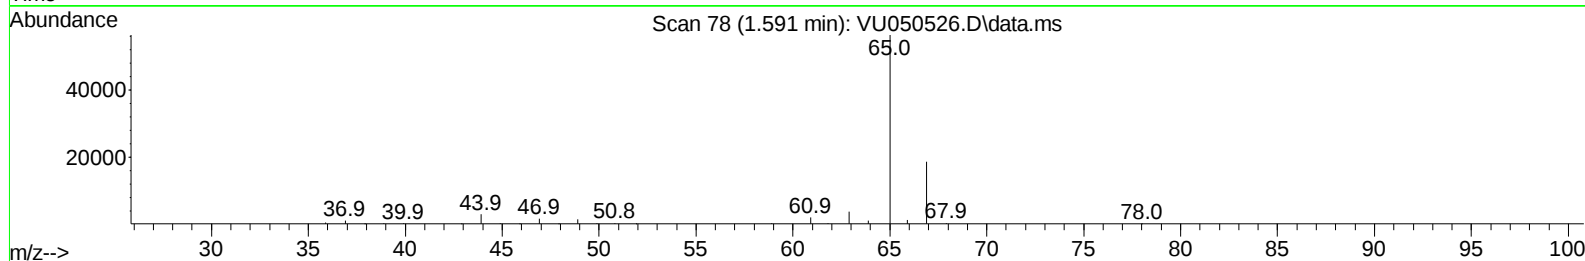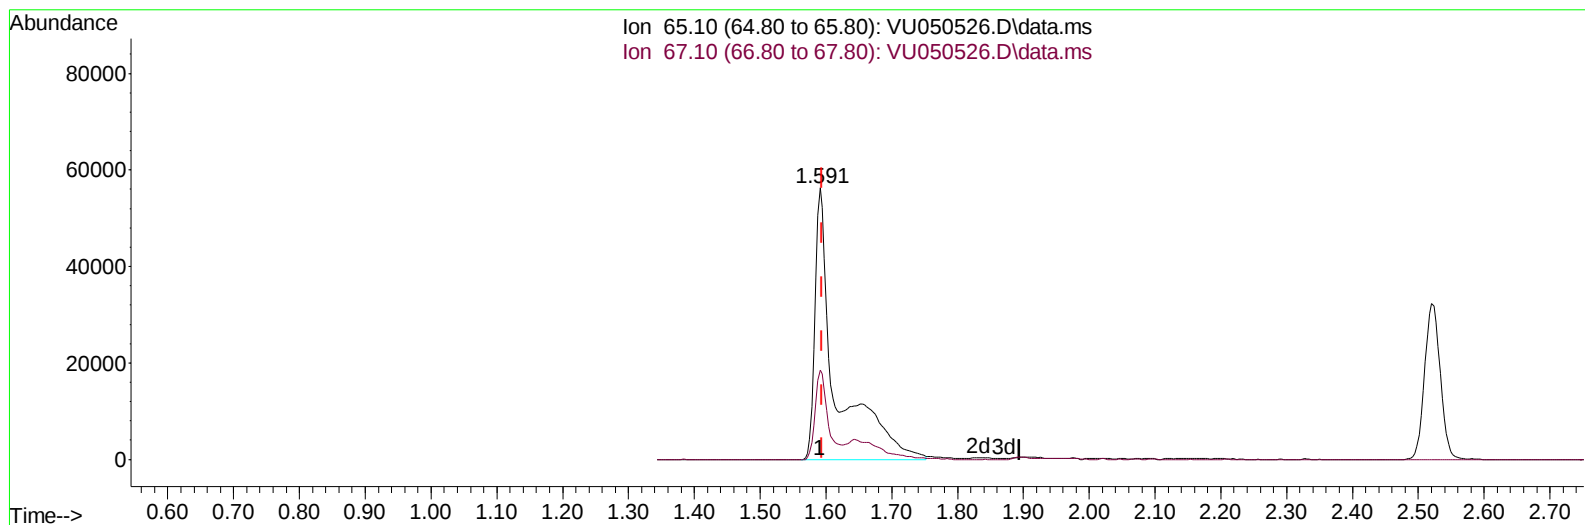

TIC: VU050526.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.591min (-0.003) 29.74 ug/L m

response 125403

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	32.20	20.50#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050526.D
 Acq On : 30 Aug 2022 19:41
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

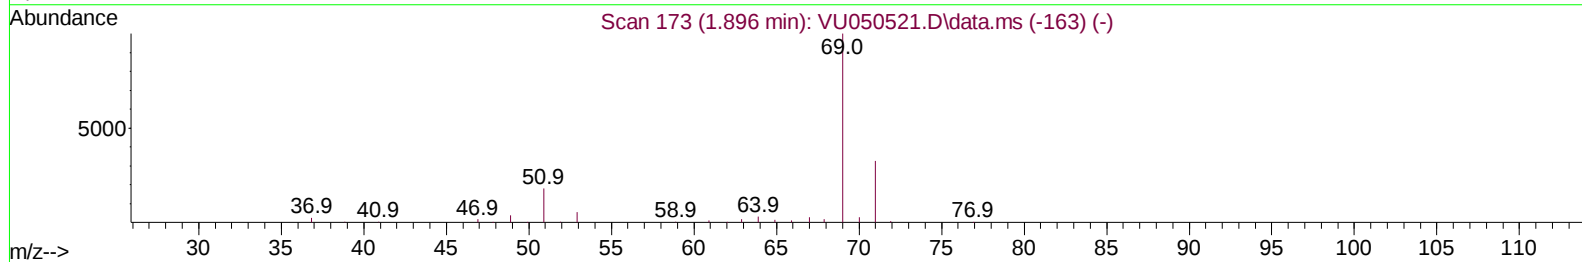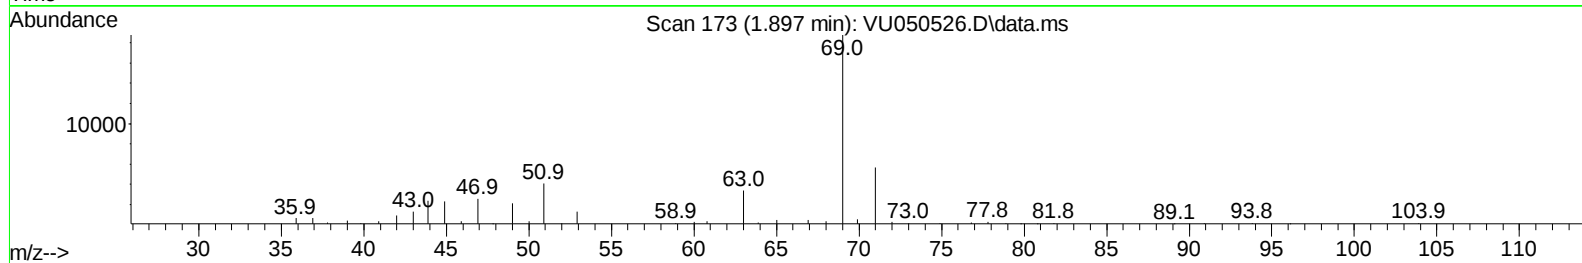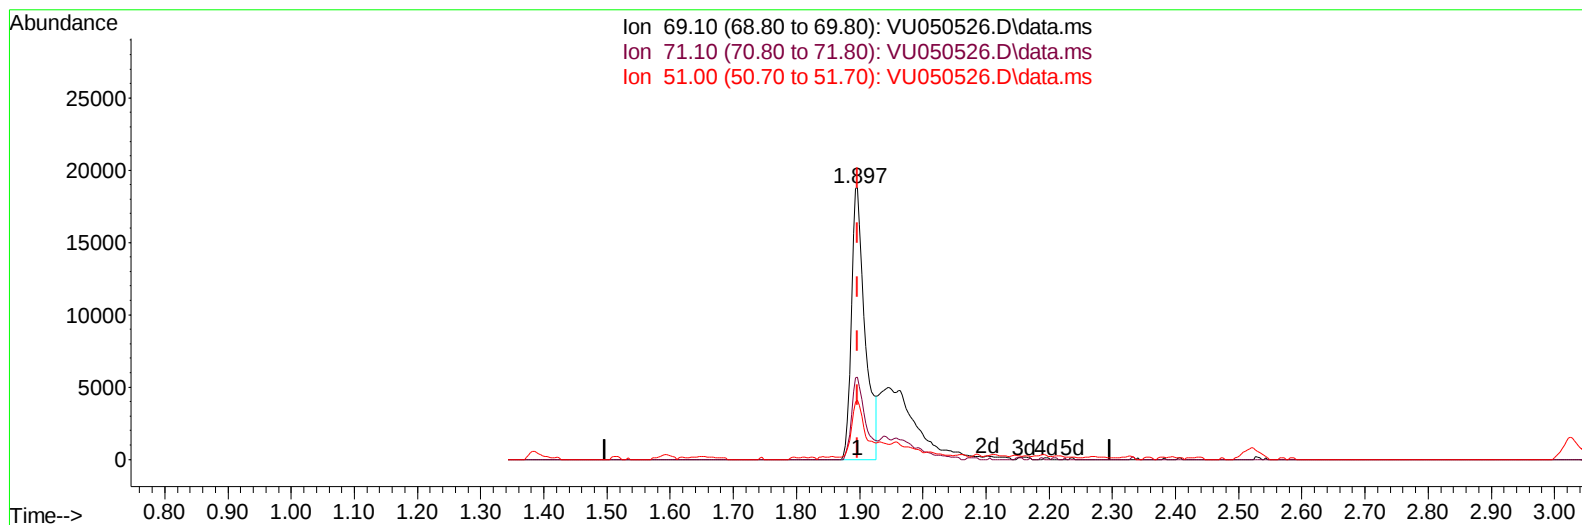

TIC: VU050526.D\data.ms

(7) Chloroethane-d5 (S)

1.897min (+ 0.000) 8.53 ug/L

response 28028

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	31.68
51.00	18.40	20.99
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050526.D
Acq On : 30 Aug 2022 19:41
Operator : SY/MD
Sample : N4345-13ME
Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT1ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 31 01:47:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

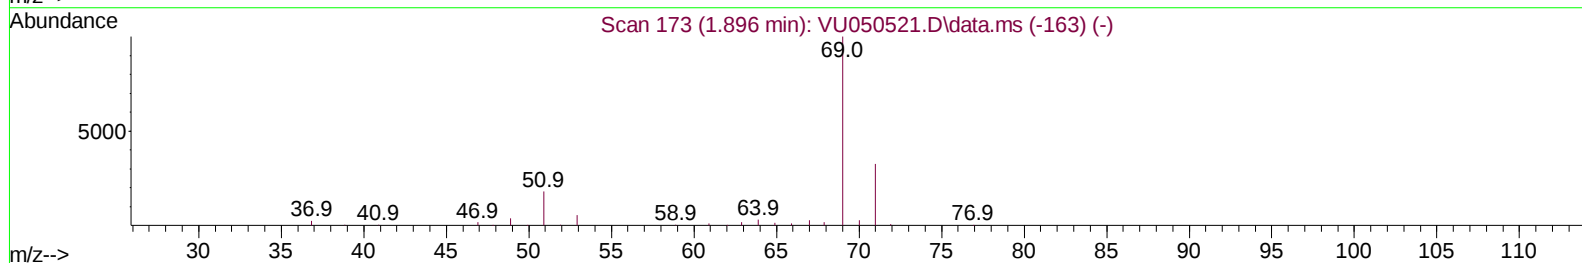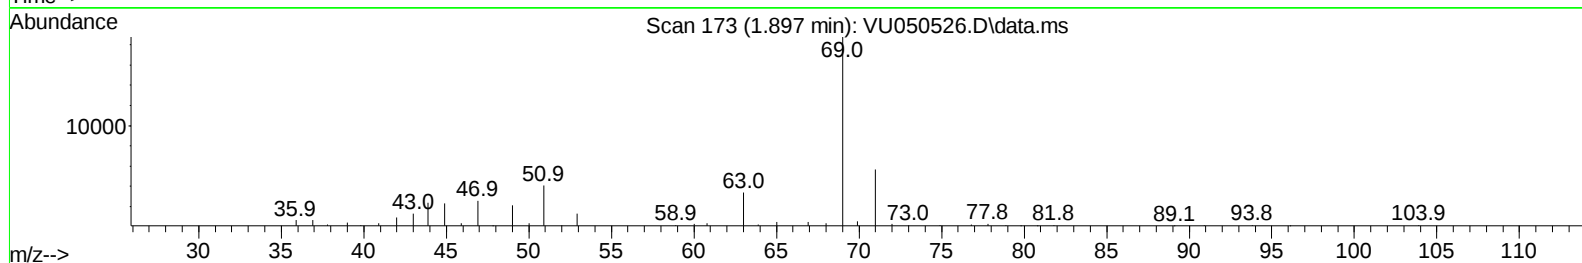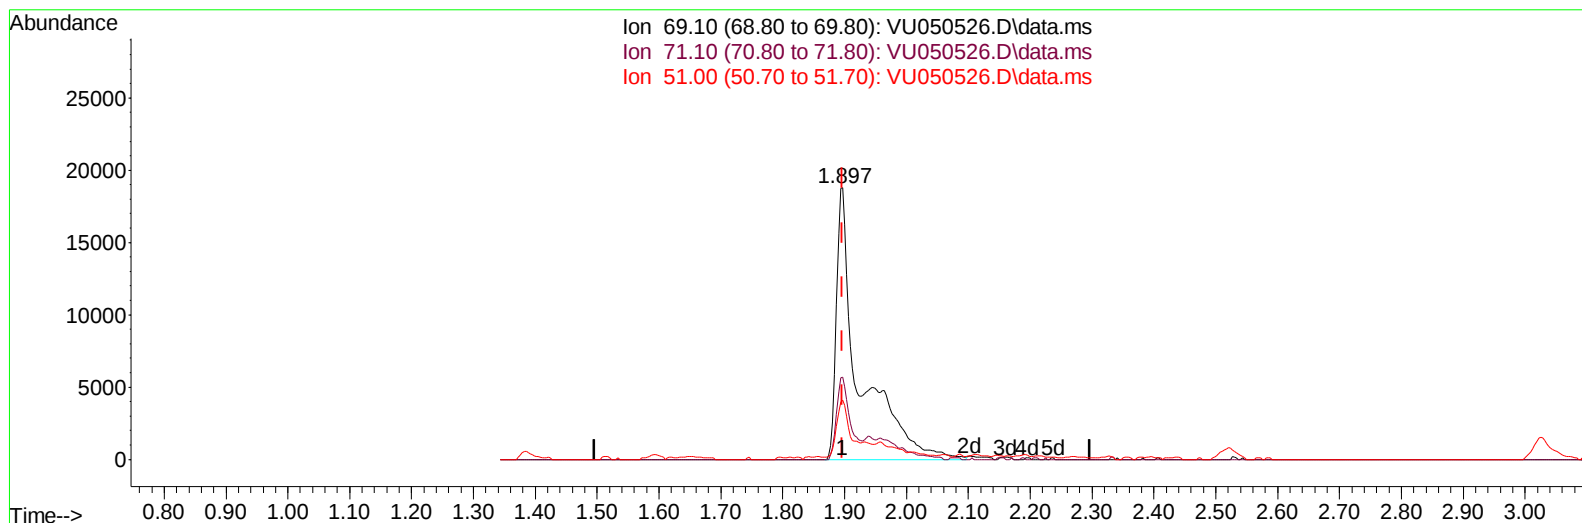

TIC: VU050526.D\data.ms

(7) Chloroethane-d5 (S)

1.897min (+ 0.000) 14.76 ug/L m

response 48523

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	18.30#
51.00	18.40	12.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
 Data File : VU050526.D
 Acq On : 30 Aug 2022 19:41
 Operator : SY/MD
 Sample : N4345-13ME
 Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVT1ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:58:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 31 01:47:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	549697	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	505958	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	185971	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.591	65	125403m	29.745	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	59.480%#	
7) Chloroethane-d5	1.897	69	48523m	14.762	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	29.520%#	
11) 1,1-Dichloroethene-d2	2.520	63	168517	23.674	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	47.340%#	
21) 2-Butanone-d5	4.655	46	207990	56.409	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	56.410%	
24) Chloroform-d	5.060	84	223807	27.282	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	54.560%#	
26) 1,2-Dichloroethane-d4	5.700	65	151479	28.427	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	56.860%#	
32) Benzene-d6	5.720	84	491944	31.371	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	62.740%#	
36) 1,2-Dichloropropane-d6	6.691	67	160549	30.748	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	61.500%#	
41) Toluene-d8	7.900	98	420102	30.793	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	61.580%#	
43) trans-1,3-Dichloroprop...	8.182	79	52489	24.995	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	50.000%#	
47) 2-Hexanone-d5	8.665	63	126925	67.136	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	67.140%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	210973	25.904	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	51.800%#	
66) 1,2-Dichlorobenzene-d4	12.198	152	130331	32.369	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	64.740%#	
Target Compounds						
					Qvalue	
46) Tetrachloroethene	8.552	164	31201	10.575	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU083022\
Data File : VU050526.D
Acq On : 30 Aug 2022 19:41
Operator : SY/MD
Sample : N4345-13ME
Misc : 5.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVT1ME

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:58:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM083022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 31 01:47:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

